

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014030.D
 Acq On : 10 Mar 2023 14:55
 Operator : CG/JU
 Sample : 01713-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBZZ7

Quant Time: Mar 10 21:29:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	92690	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	401862	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.716	164	286535	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	713614	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	760077	20.000	ng/ul	-0.01
88) Perylene-d12	24.080	264	801004	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	7724	3.148	ng/uL	0.00
4) Pyridine-d5	3.864	84	168	0.025	ng/ul	0.00
7) Phenol-d5	7.228	99	140700	17.201	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	86771	18.189	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	105399	16.913	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	103025	15.420	ng/ul	-0.01
21) Nitrobenzene-d5	9.252	128	51902	16.187	ng/ul	0.00
24) 2-Nitrophenol-d4	9.981	143	62302	16.232	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	116621	16.148	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	123962	12.970	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	462871	19.034	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	456525	17.722	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	64543	15.061	ng/ul	0.00
60) Fluorene-d10	15.704	176	395754	19.203	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.822	200	76246	14.137	ng/ul	-0.01
73) Anthracene-d10	17.569	188	687790	19.854	ng/ul	0.00
81) Pyrene-d10	19.792	212	988504	23.580	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.915	264	942712	22.126	ng/ul	-0.01
Target Compounds					Qvalue	
16) Acetophenone	8.910	105	16041	1.486	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014030.D
Acq On : 10 Mar 2023 14:55
Operator : CG/JU
Sample : 01713-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBZZ7

Quant Time: Mar 10 21:29:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

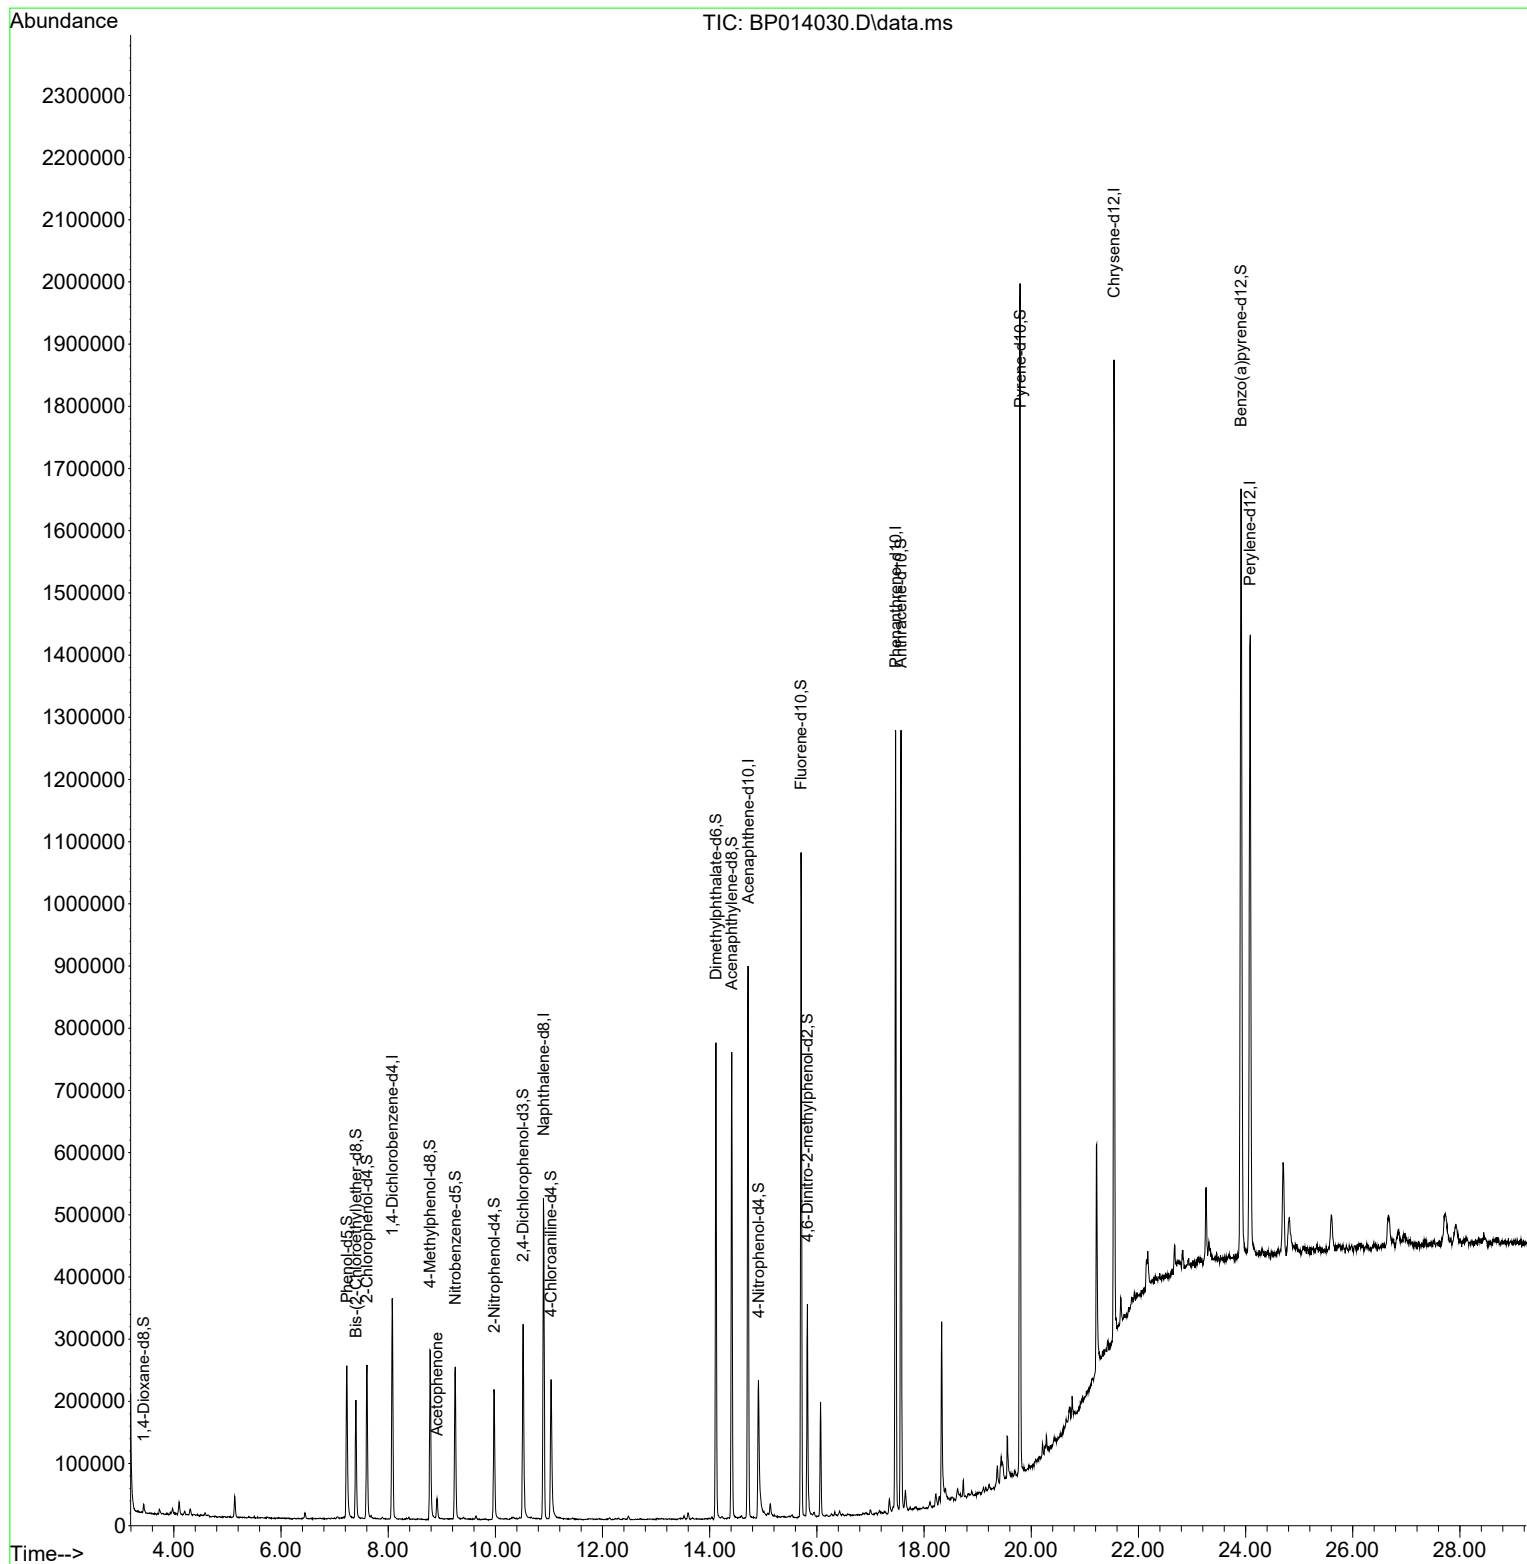

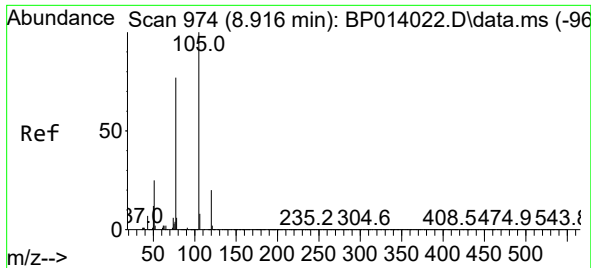

#16
Acetophenone
Concen: 1.486 ng/ul
RT: 8.910 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP014030.D
Acq: 10 Mar 2023 14:55

Instrument :
BNA_P
ClientSampleId :
DBZZ7

Tgt Ion:	105	Resp:	16041
Ion	Ratio	Lower	Upper
105	100		
77	80.5	65.4	98.2
51	26.5	21.8	32.8

