




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014034.D
 Acq On : 10 Mar 2023 17:13
 Operator : CG/JU
 Sample : 01804-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:30:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

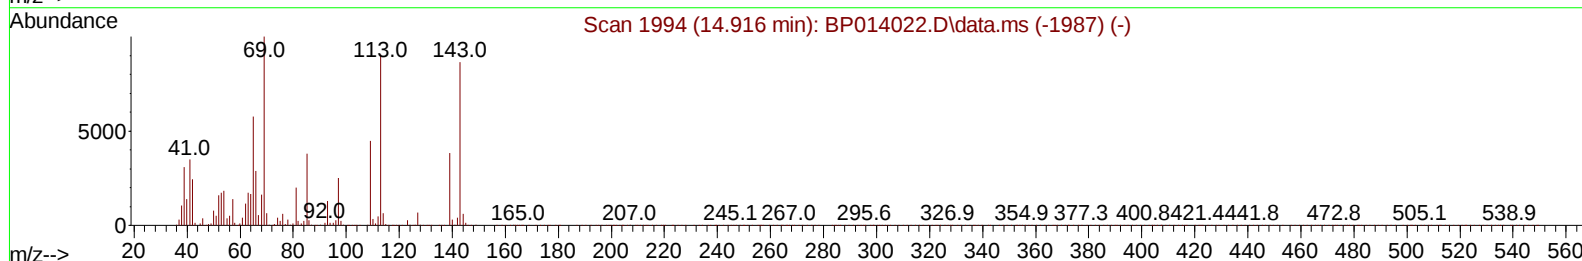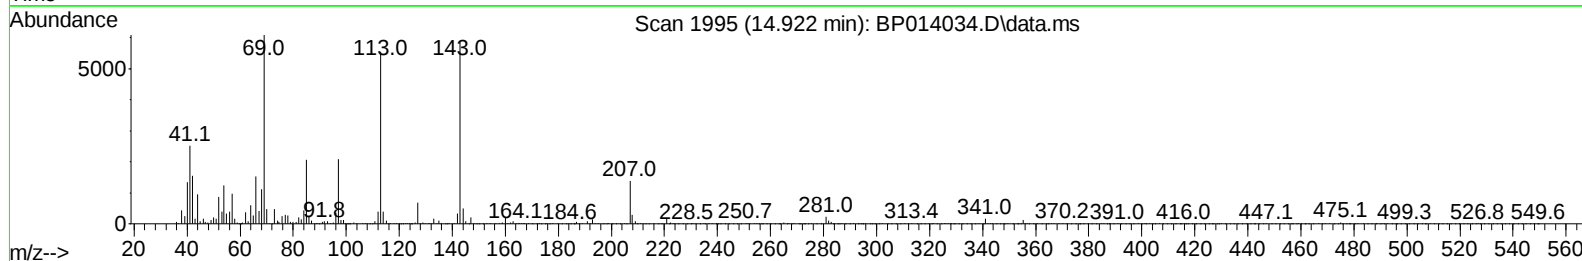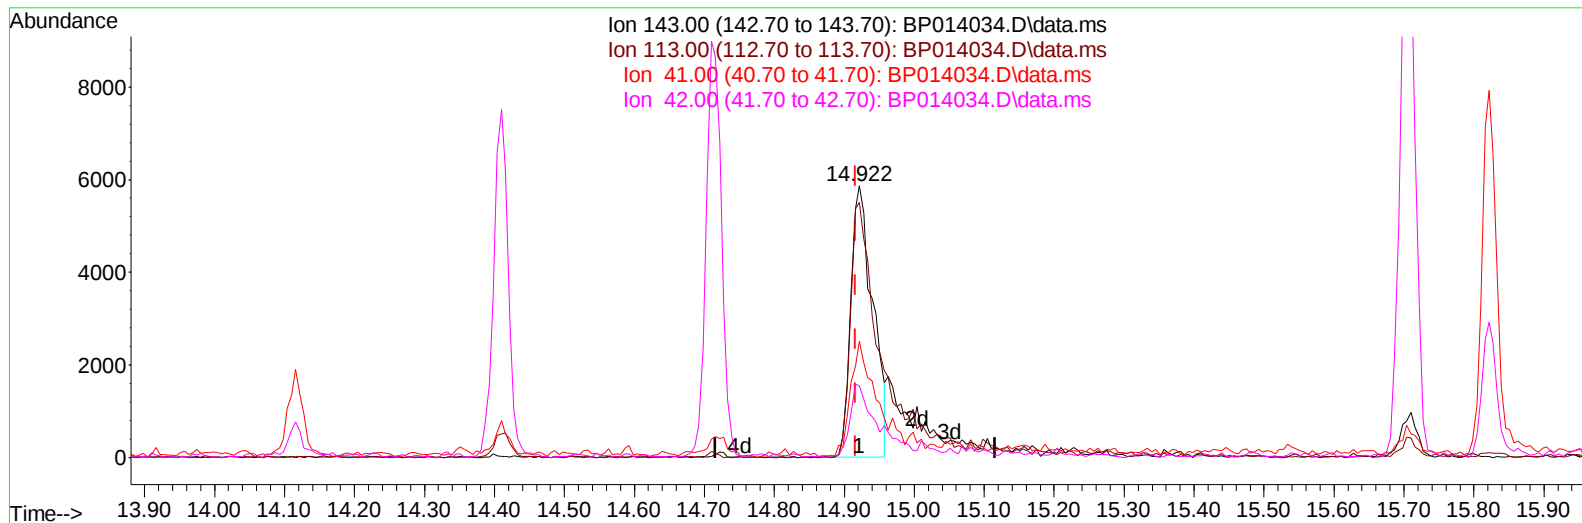

TIC: BP014034.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.006) 2.09 ng/u1

response 12724

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	94.07
41.00	40.20	42.82
42.00	28.50	26.38




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014034.D
 Acq On : 10 Mar 2023 17:13
 Operator : CG/JU
 Sample : 01804-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:30:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

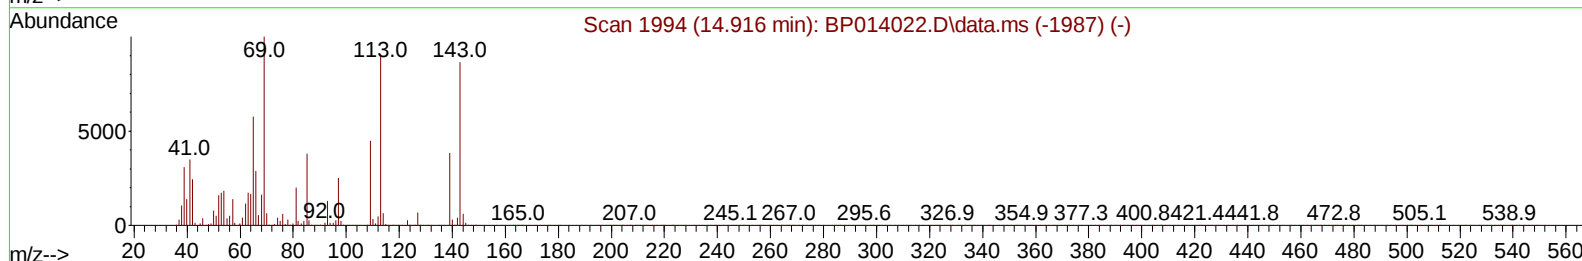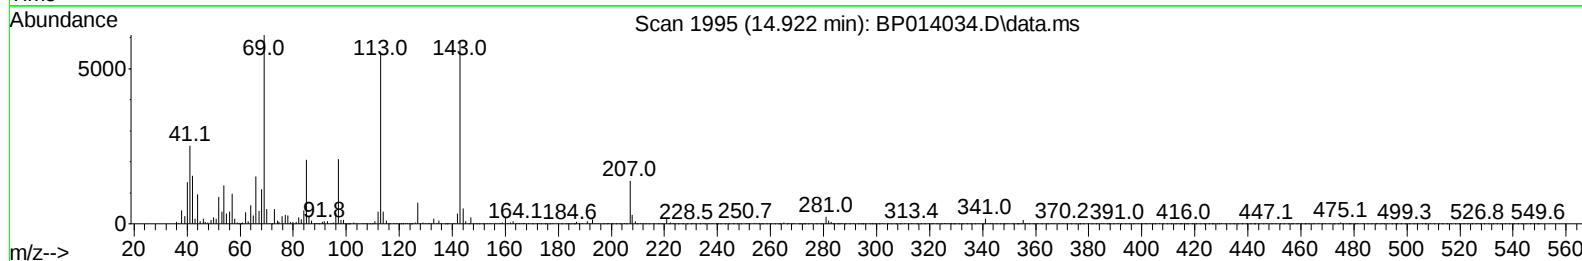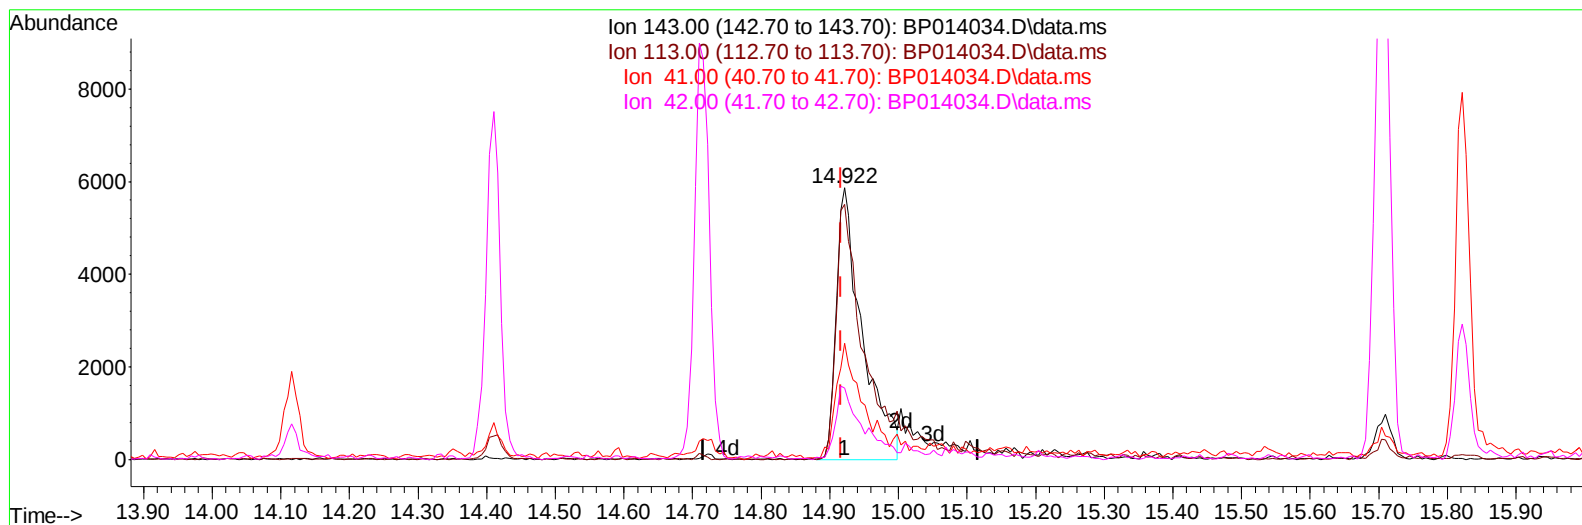

TIC: BP014034.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.006) 2.55 ng/ul m

response 15538

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	94.07
41.00	40.20	42.82
42.00	28.50	26.38

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014034.D
 Acq On : 10 Mar 2023 17:13
 Operator : CG/JU
 Sample : 01804-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 10 21:30:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	138067	20.000	ng/ul	0.00
20) Naphthalene-d8	10.898	136	591872	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.716	164	407903	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	987091	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1023068	20.000	ng/ul	-0.01
88) Perylene-d12	24.086	264	1098546	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	13598	3.721	ng/uL	0.00
4) Pyridine-d5	3.875	84	56764	5.610	ng/ul	0.00
7) Phenol-d5	7.228	99	48255	3.961	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	181993	25.612	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	153788	16.567	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	97693	9.816	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	113211	23.973	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	120612	21.336	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	202389	19.027	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	237925	16.902	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	842897	24.349	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	854757	23.308	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	15538m	2.547	ng/ul	0.00
60) Fluorene-d10	15.704	176	742866	25.320	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.822	200	156709	21.005	ng/ul	-0.01
73) Anthracene-d10	17.569	188	1345047	28.069	ng/ul	0.00
81) Pyrene-d10	19.792	212	1702071	30.165	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	1660789	28.421	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014034.D
Acq On : 10 Mar 2023 17:13
Operator : CG/JU
Sample : 01804-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 10 21:30:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

