




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014035.D
 Acq On : 10 Mar 2023 17:48
 Operator : CG/JU
 Sample : 01804-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA4

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

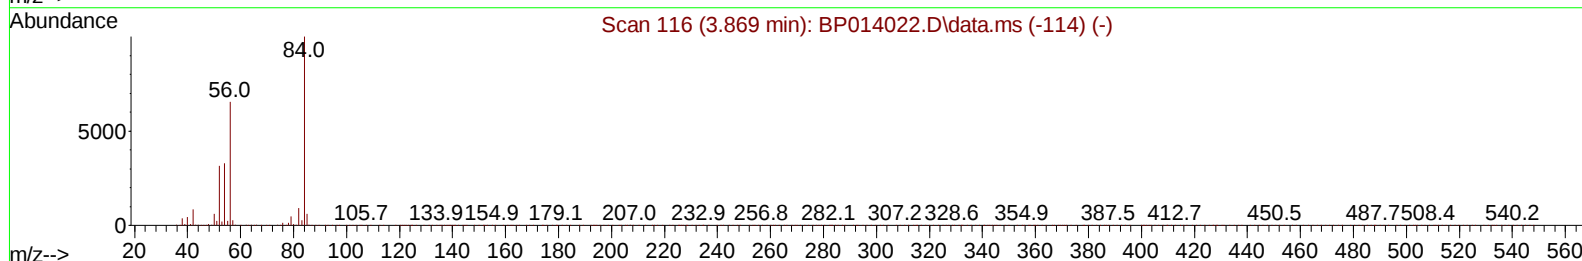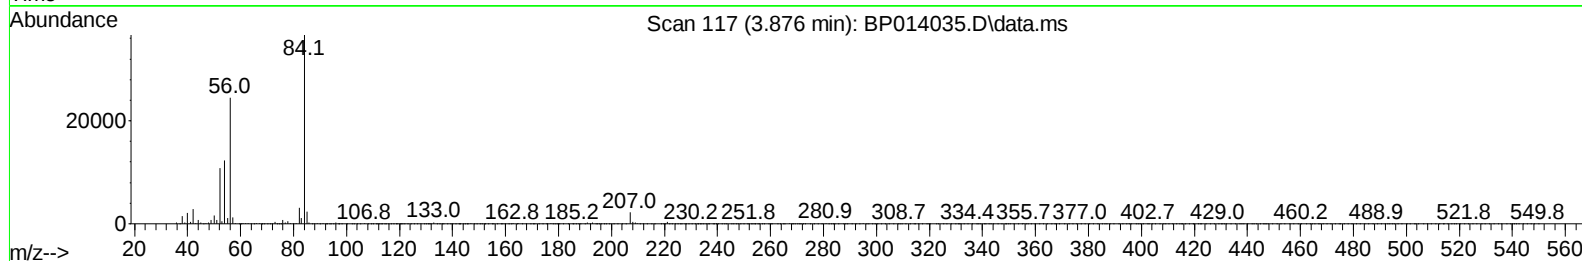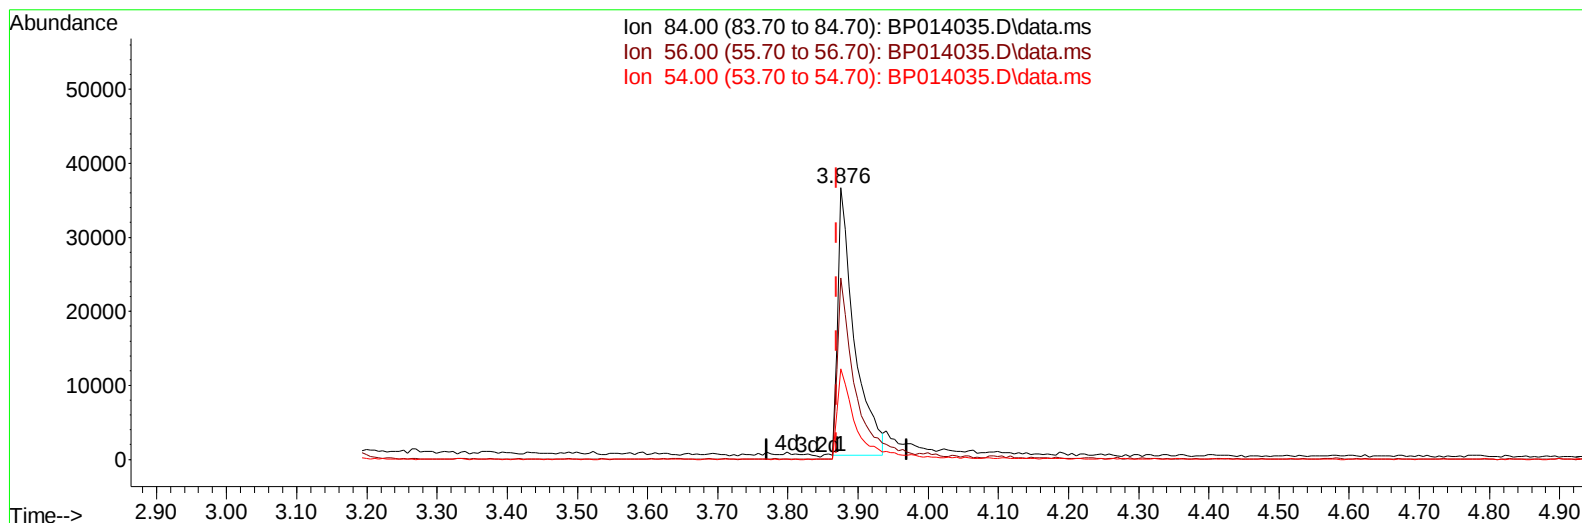

TIC: BP014035.D\data.ms

(4) Pyridine-d5 (S)

3.876min (+ 0.006) 5.95 ng/u1

response 58959

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	62.80	66.86
54.00	33.20	33.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014035.D
 Acq On : 10 Mar 2023 17:48
 Operator : CG/JU
 Sample : 01804-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA4

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

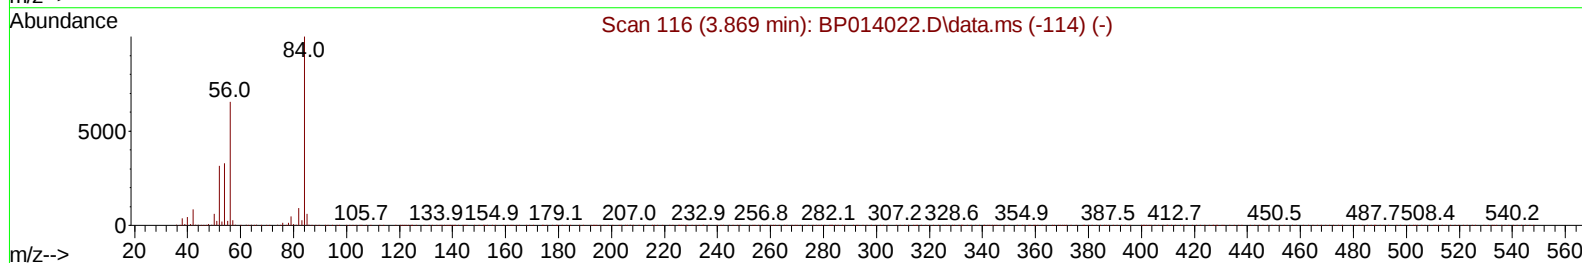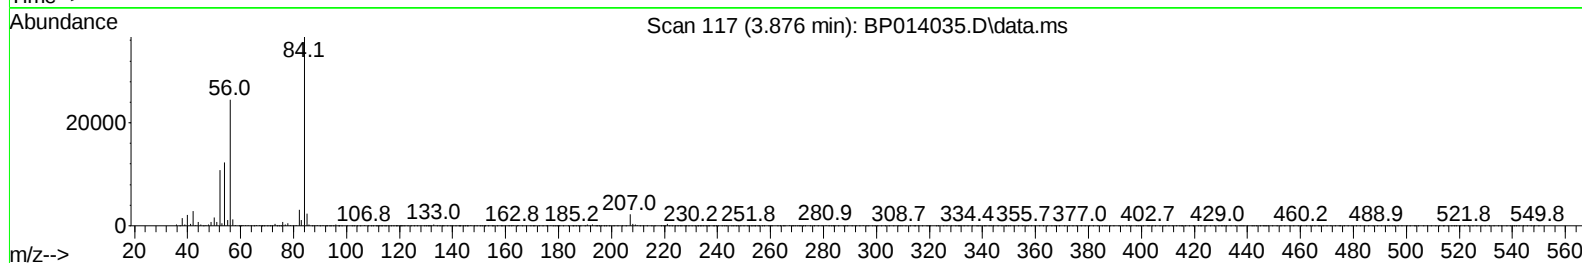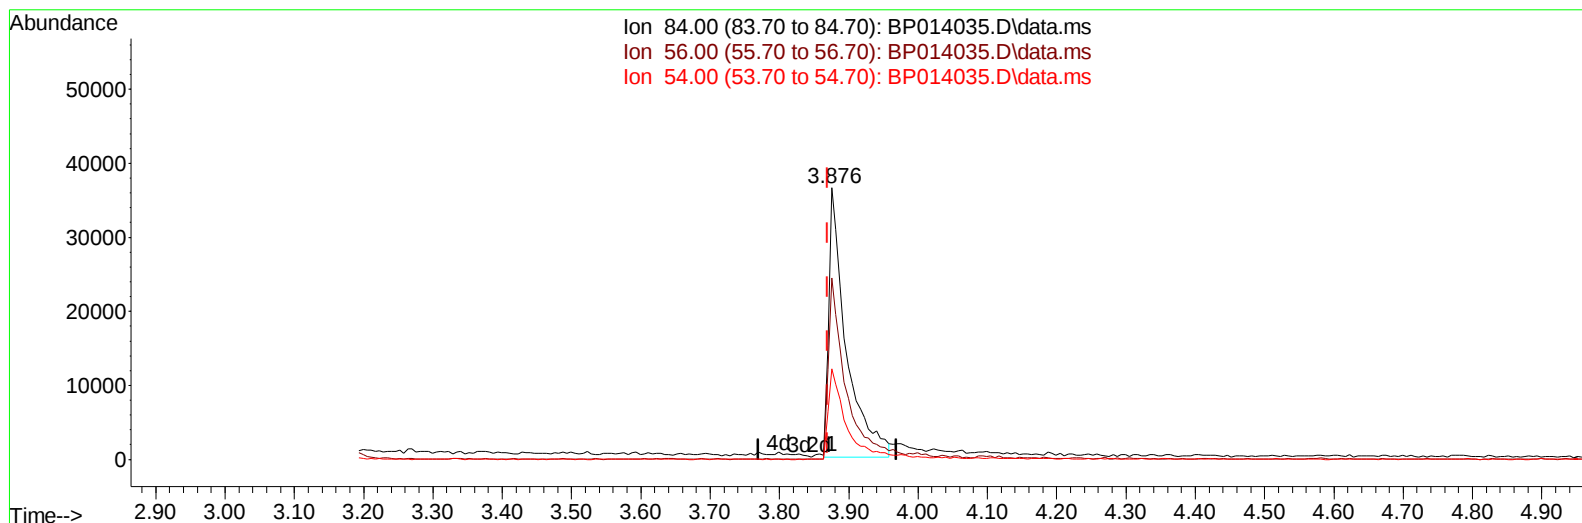

TIC: BP014035.D\data.ms

(4) Pyridine-d5 (S)

3.876min (+ 0.006) 6.43 ng/u1 m

response 63689

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	62.80	66.86
54.00	33.20	33.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014035.D
 Acq On : 10 Mar 2023 17:48
 Operator : CG/JU
 Sample : 01804-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA4

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

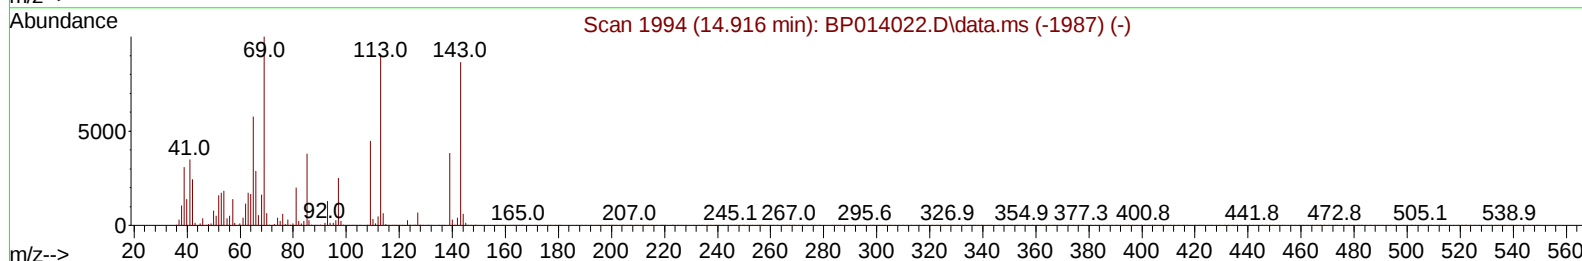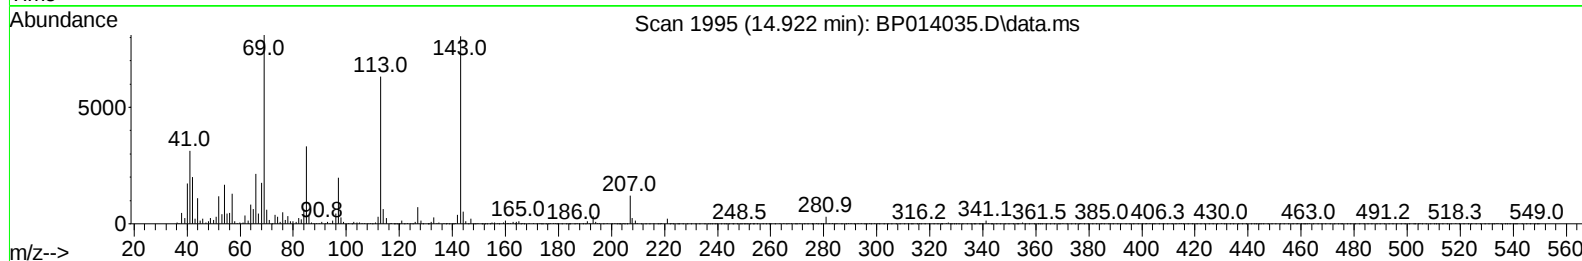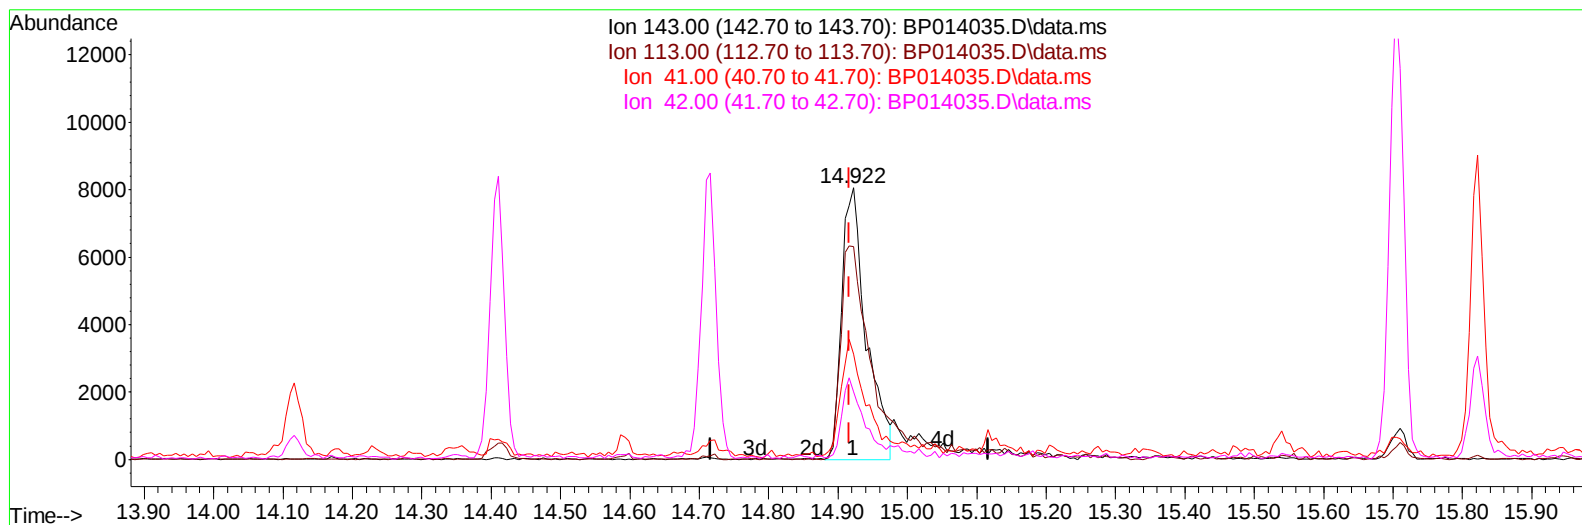

TIC: BP014035.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.006) 3.31 ng/u1

response 19835

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	78.32#
41.00	40.20	38.76
42.00	28.50	24.79




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014035.D
 Acq On : 10 Mar 2023 17:48
 Operator : CG/JU
 Sample : 01804-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA4

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

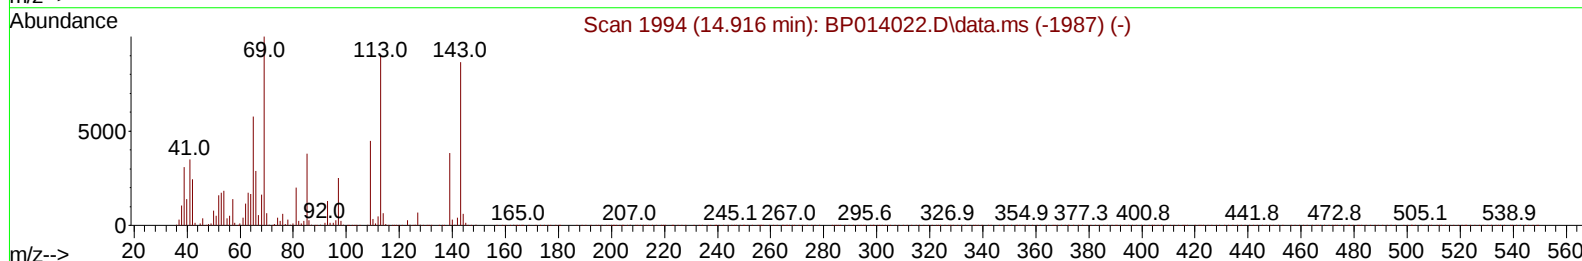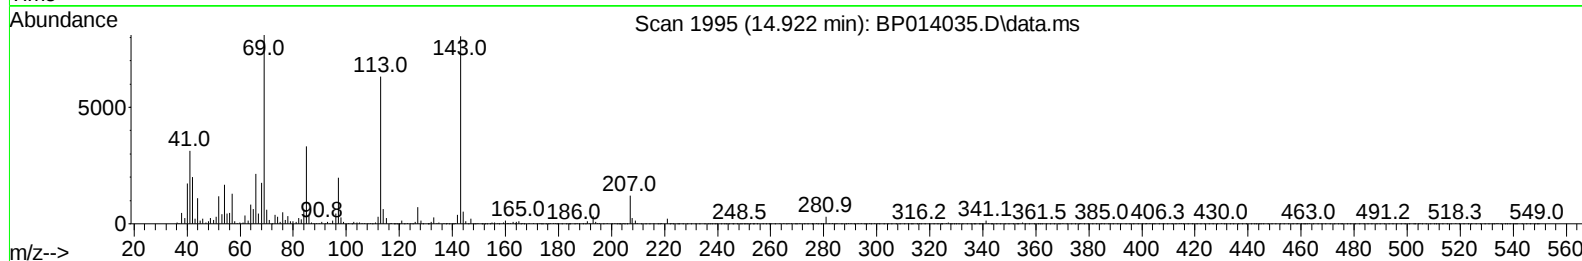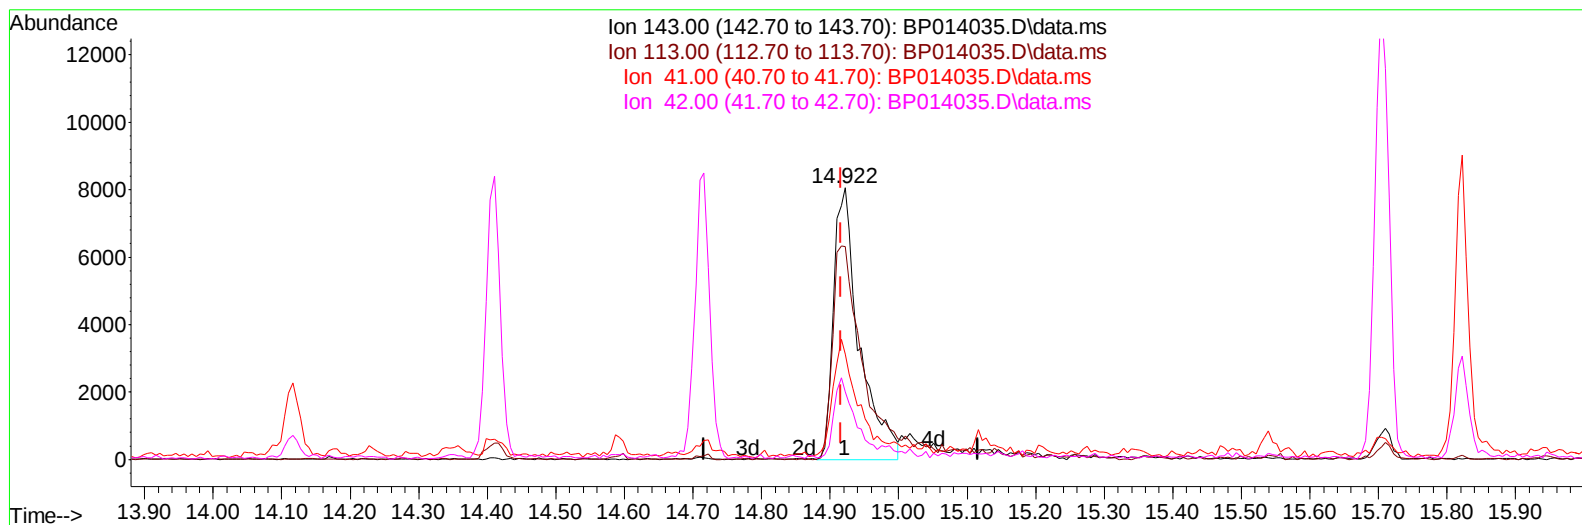

TIC: BP014035.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.006) 3.50 ng/ul m

response 21000

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	78.32#
41.00	40.20	38.76
42.00	28.50	24.79

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014035.D
 Acq On : 10 Mar 2023 17:48
 Operator : CG/JU
 Sample : 01804-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 10 21:31:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	135122	20.000	ng/ul	0.00
20) Naphthalene-d8	10.899	136	559068	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.716	164	400945	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	927723	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	996339	20.000	ng/ul	-0.01
88) Perylene-d12	24.086	264	1008554	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	13367	3.738	ng/uL	0.00
4) Pyridine-d5	3.876	84	63689m	6.432	ng/ul	0.00
7) Phenol-d5	7.228	99	57196	4.797	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	182186	26.198	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	168372	18.533	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	111915	11.490	ng/ul	-0.01
21) Nitrobenzene-d5	9.252	128	111857	25.076	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	121938	22.836	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	204868	20.390	ng/ul	0.00
31) 4-Chloroaniline-d4	11.040	131	234773	17.657	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	868800	25.533	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	890052	24.692	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	21000m	3.502	ng/ul	0.00
60) Fluorene-d10	15.704	176	753657	26.134	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.822	200	162714	23.206	ng/ul	-0.01
73) Anthracene-d10	17.569	188	1296459	28.787	ng/ul	0.00
81) Pyrene-d10	19.792	212	1682714	30.622	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.922	264	1618273	30.165	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014035.D
Acq On : 10 Mar 2023 17:48
Operator : CG/JU
Sample : 01804-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 10 21:31:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

