




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014038.D
 Acq On : 10 Mar 2023 19:31
 Operator : CG/JU
 Sample : 01804-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

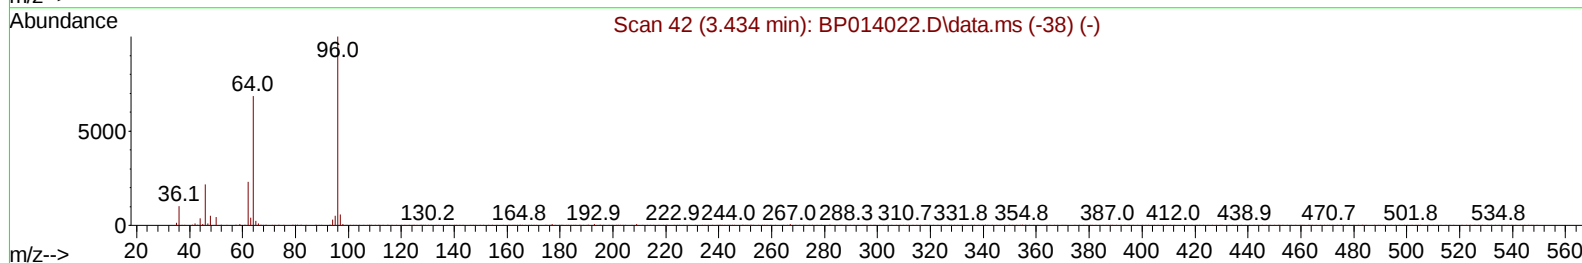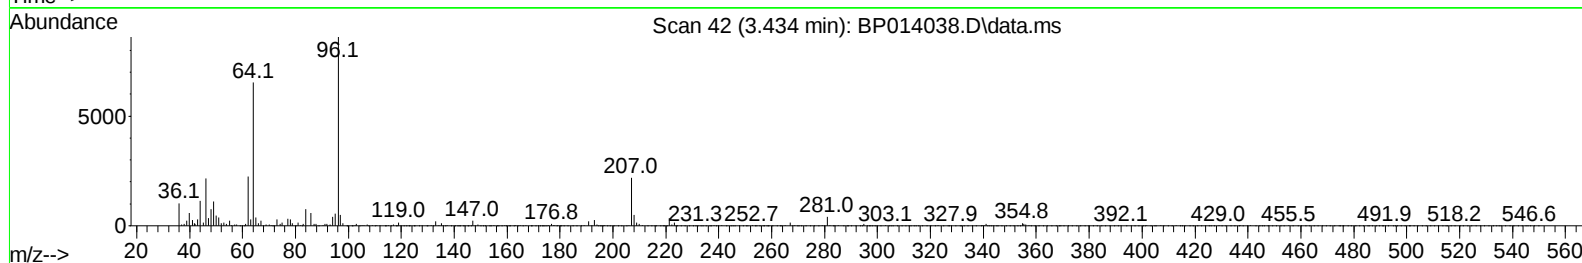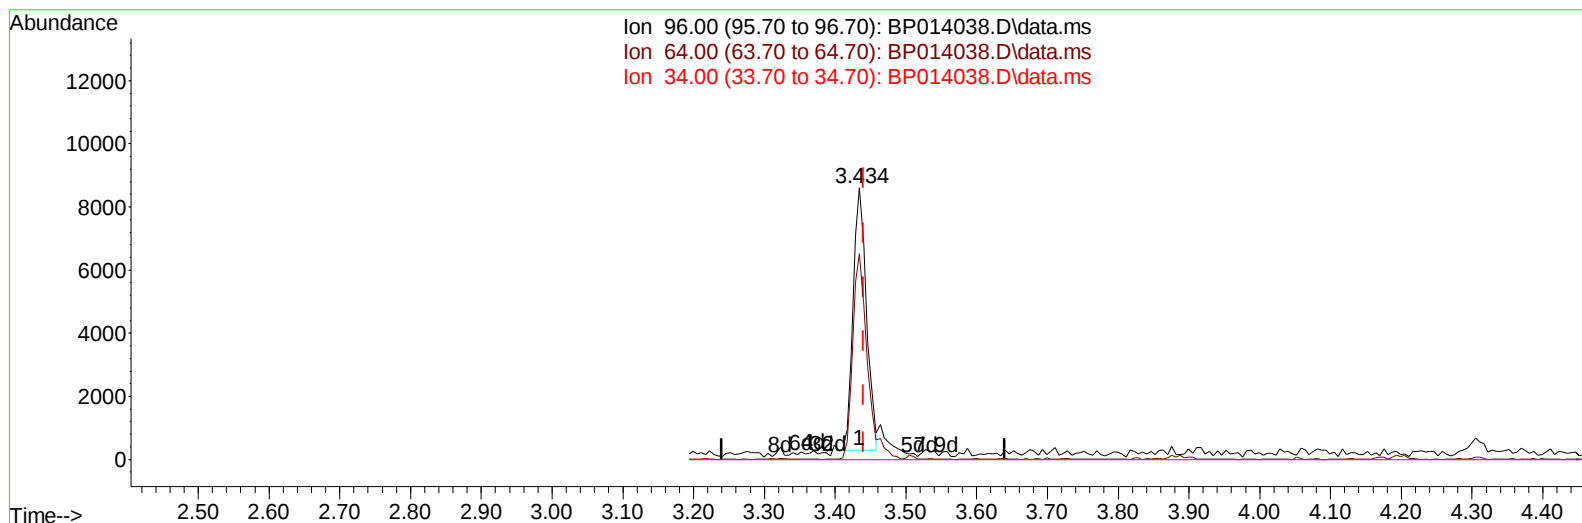

TIC: BP014038.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.434min (-0.006) 3.29 ng/uL

response 10905

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	66.60	75.85
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014038.D
 Acq On : 10 Mar 2023 19:31
 Operator : CG/JU
 Sample : 01804-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

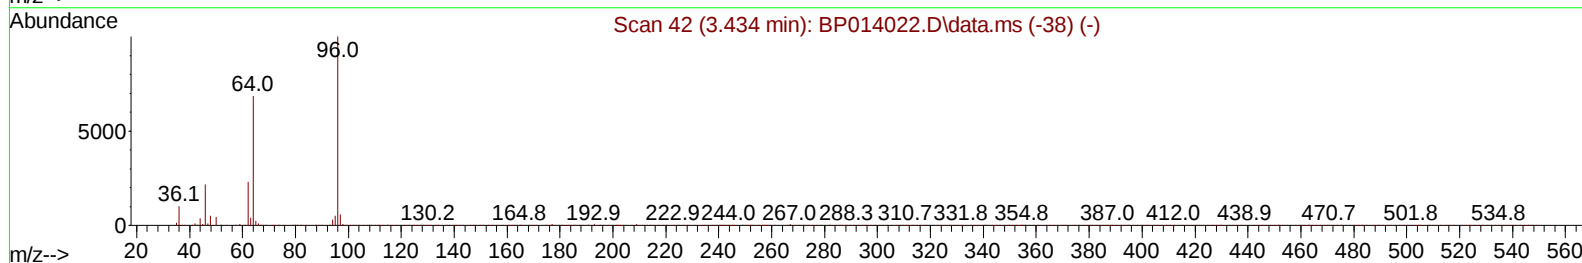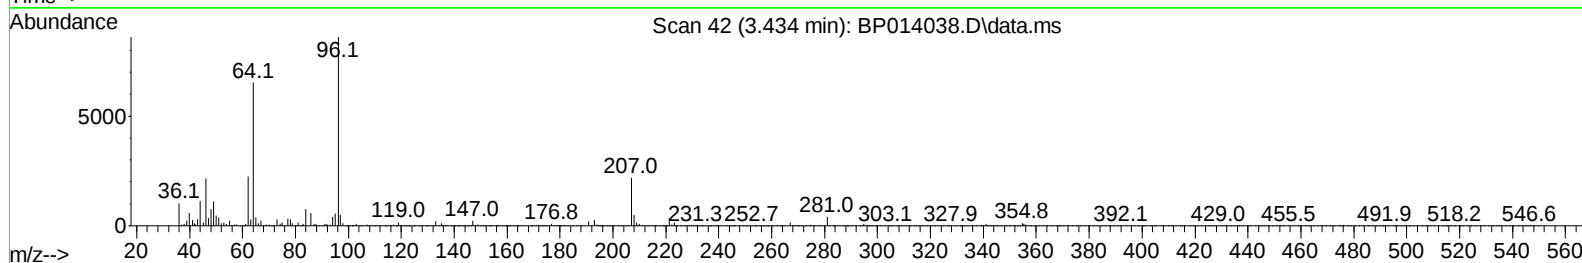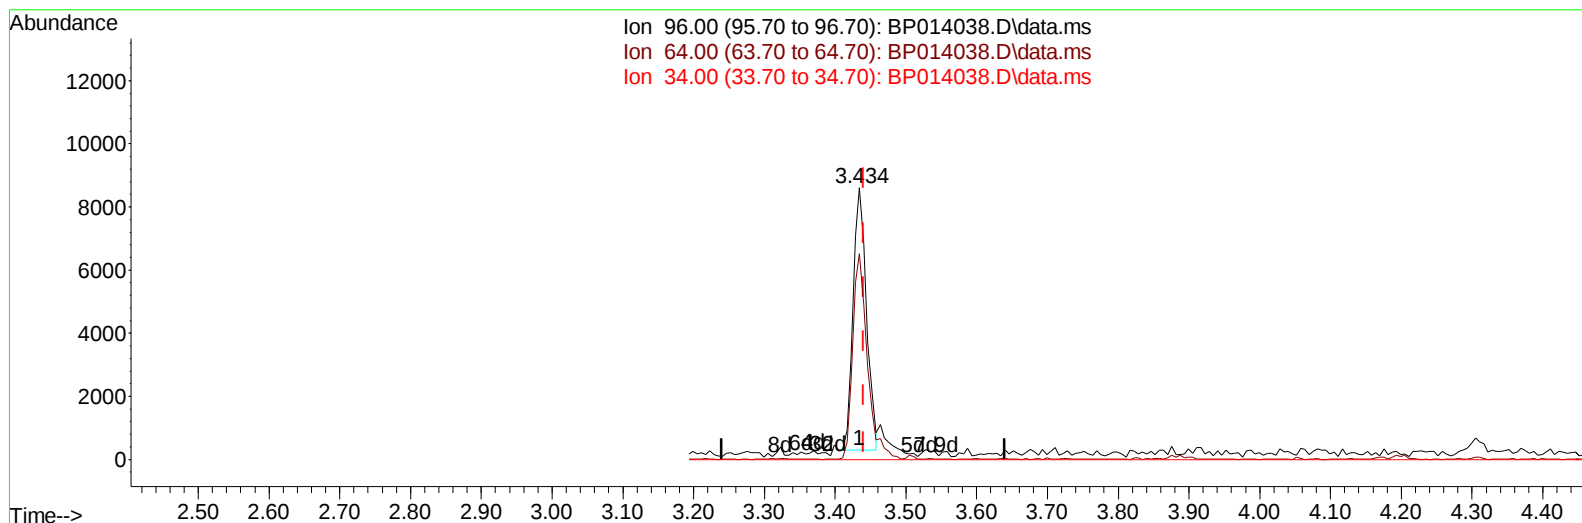

TIC: BP014038.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.434min (-0.006) 3.29 ng/uL

response 10905

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	66.60	75.85
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014038.D
 Acq On : 10 Mar 2023 19:31
 Operator : CG/JU
 Sample : 01804-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

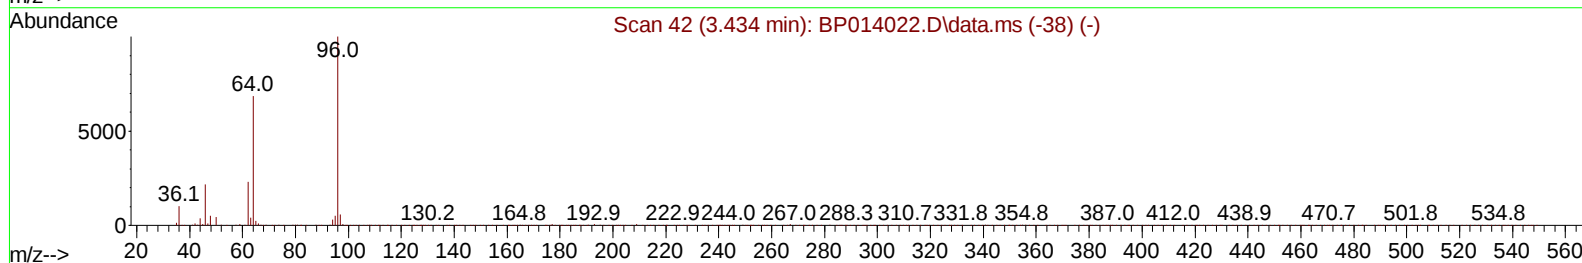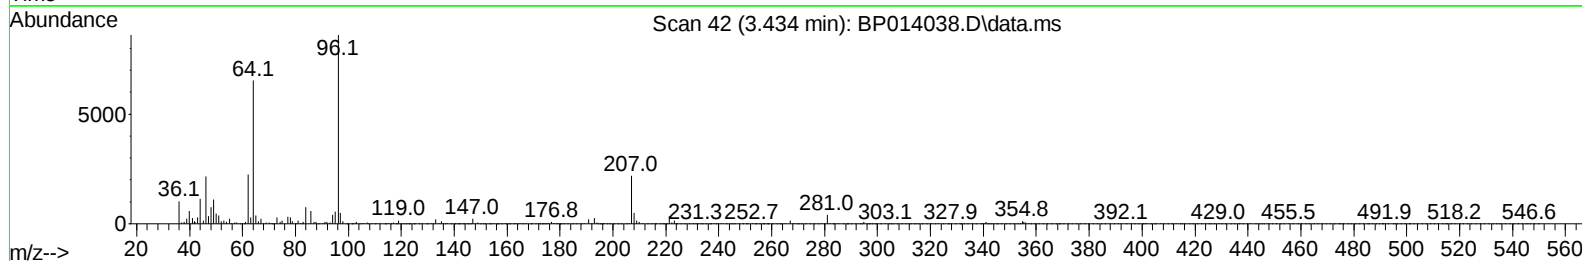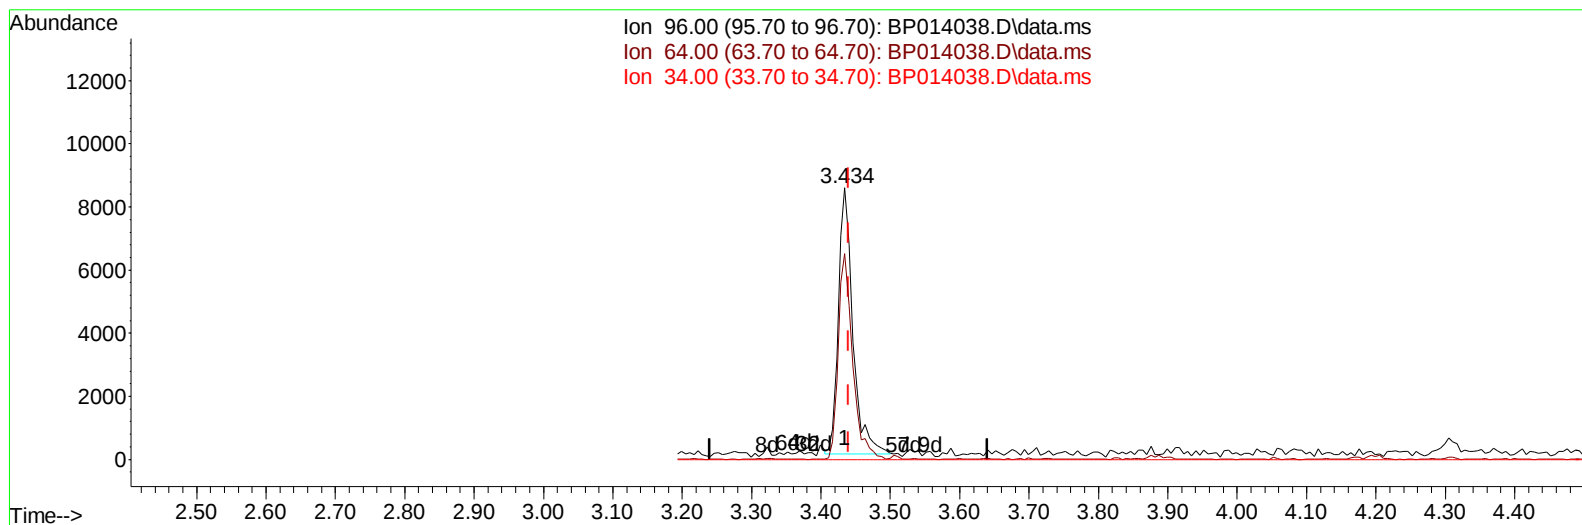

TIC: BP014038.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.434min (-0.006) 3.67 ng/uL m

response 12153

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	66.60	75.85
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014038.D
Acq On : 10 Mar 2023 19:31
Operator : CG/JU
Sample : 01804-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA5

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 10 21:31:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

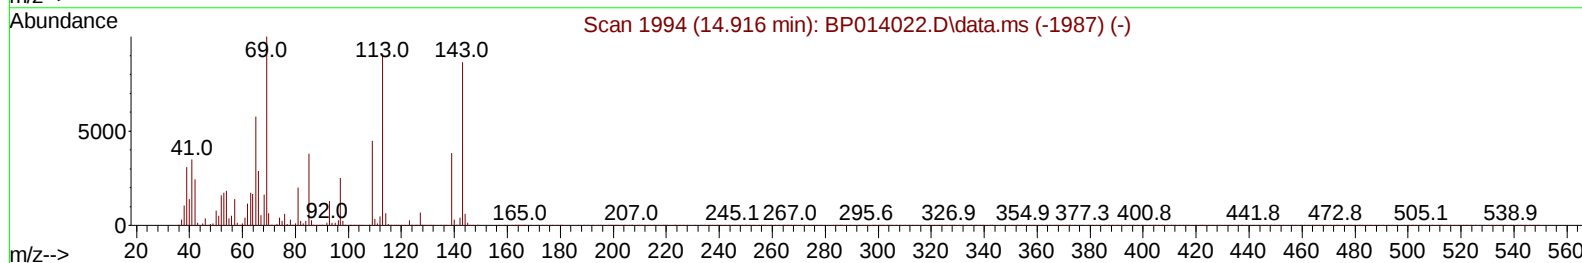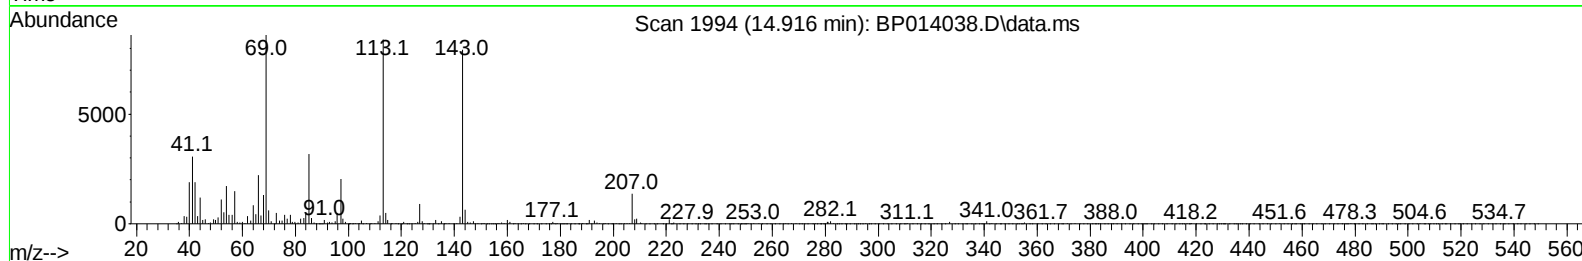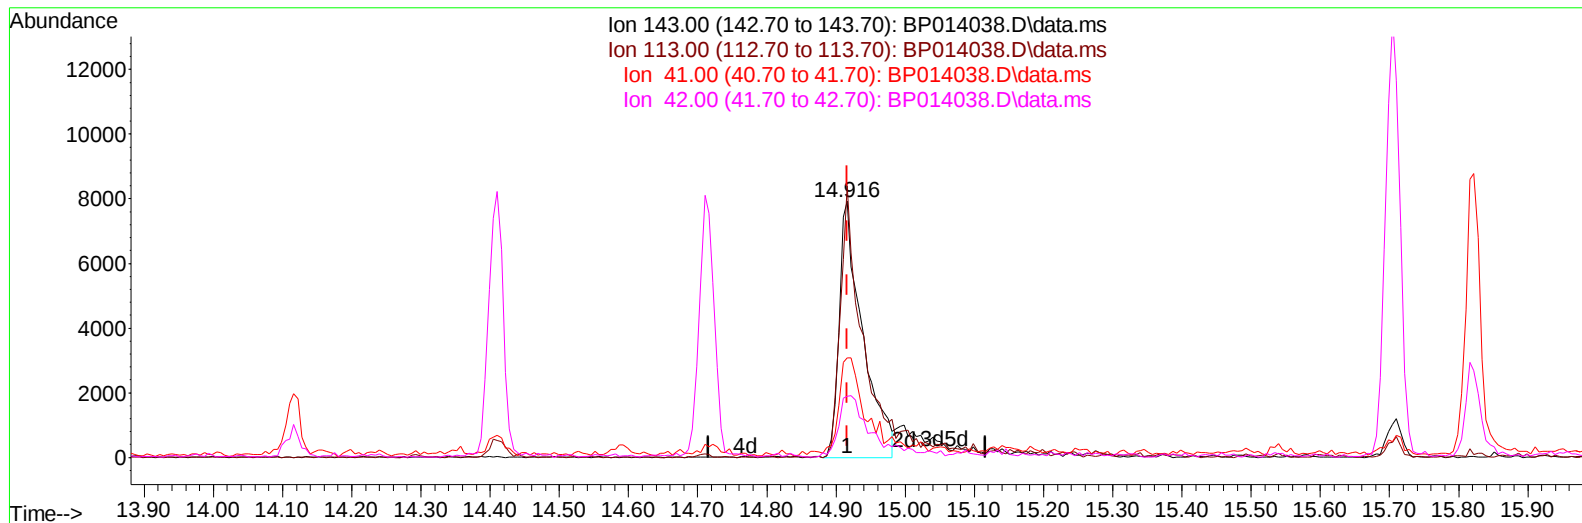

TIC: BP014038.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.916min (+ 0.000) 3.36 ng/u1****response 18550**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	105.94
41.00	40.20	38.79
42.00	28.50	23.98




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014038.D
 Acq On : 10 Mar 2023 19:31
 Operator : CG/JU
 Sample : 01804-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

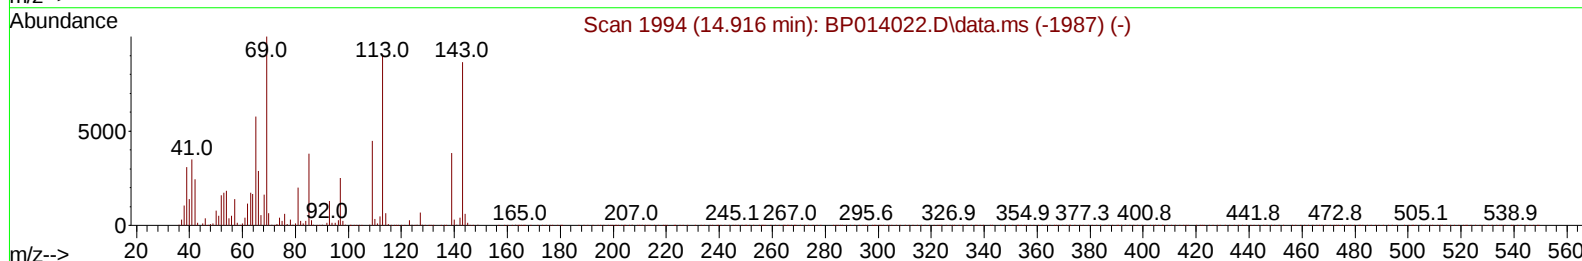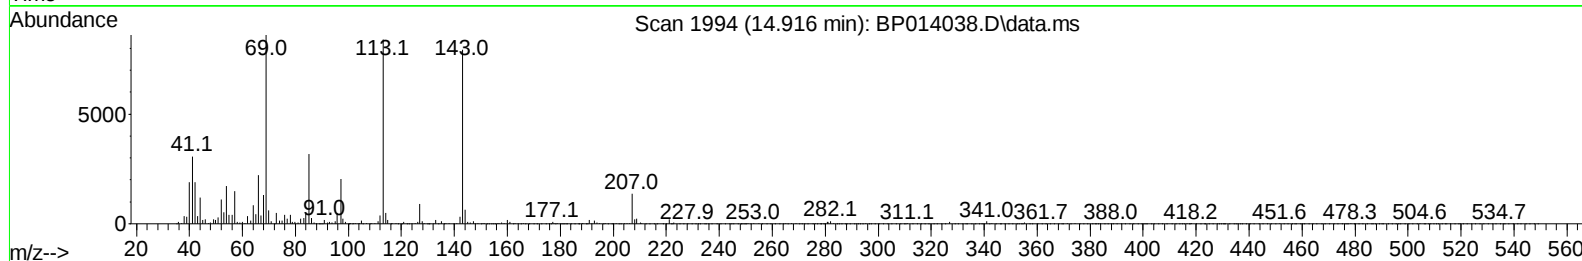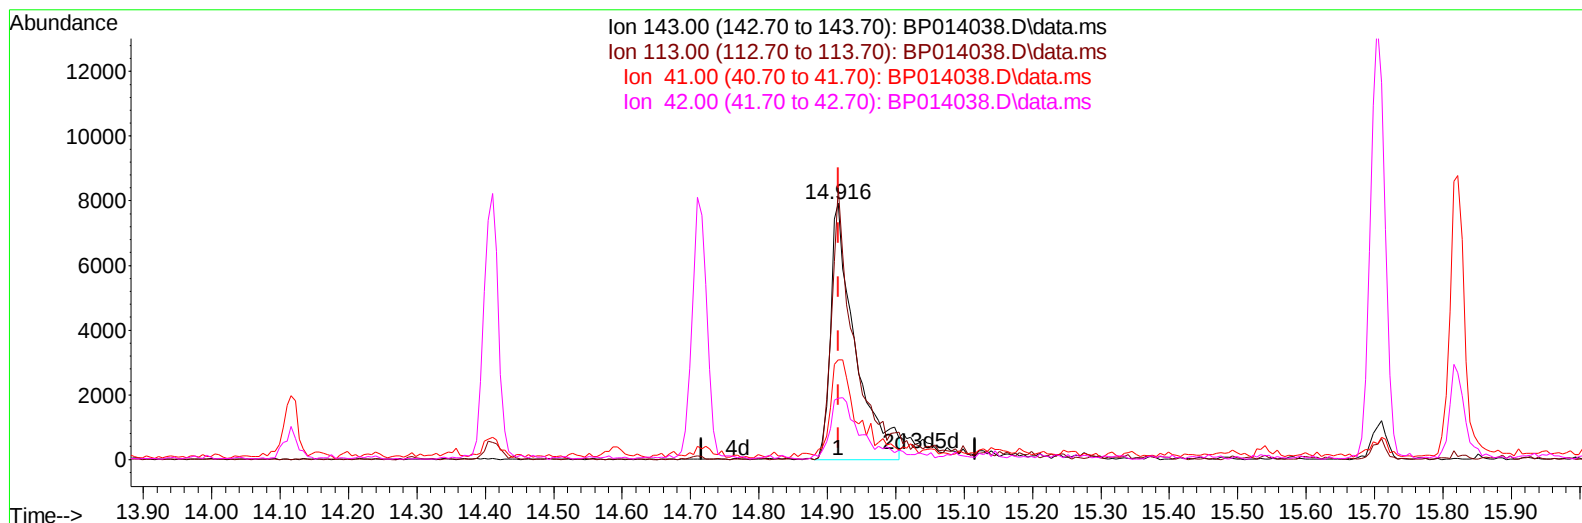

TIC: BP014038.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.000) 3.58 ng/ul m

response 19790

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	105.94
41.00	40.20	38.79
42.00	28.50	23.98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014038.D
 Acq On : 10 Mar 2023 19:31
 Operator : CG/JU
 Sample : 01804-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 21:31:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 09 01:10:12 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	125060	20.000	ng/ul	0.00
20) Naphthalene-d8	10.899	136	543582	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.716	164	369310	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	898990	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1005658	20.000	ng/ul	-0.01
88) Perylene-d12	24.086	264	1063070	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	12153m	3.672	ng/uL	0.00
4) Pyridine-d5	3.876	84	61588	6.720	ng/ul	0.00
7) Phenol-d5	7.228	99	53912	4.885	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.399	67	187445	29.123	ng/ul	0.00
11) 2-Chlorophenol-d4	7.605	132	167899	19.968	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	106690	11.835	ng/ul	-0.01
21) Nitrobenzene-d5	9.246	128	115444	26.617	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.975	143	129404	24.924	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	216514	22.163	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	222554	17.215	ng/ul	-0.01
46) Dimethylphthalate-d6	14.116	166	871303	27.799	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	907657	27.337	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	19790m	3.583	ng/ul	0.00
60) Fluorene-d10	15.704	176	767872	28.908	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.822	200	172362	25.367	ng/ul	-0.01
73) Anthracene-d10	17.569	188	1415611	32.437	ng/ul	0.00
81) Pyrene-d10	19.792	212	1867784	33.675	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.916	264	1955608	34.584	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014038.D
Acq On : 10 Mar 2023 19:31
Operator : CG/JU
Sample : 01804-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA5

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 10 21:31:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 09 01:10:12 2023
Response via : Initial Calibration

