




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014050.D
Acq On : 11 Mar 2023 02:57
Operator : CG/JU
Sample : 01810-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAF7

Manual IntegrationsAPPROVED

Quant Time: Mar 11 03:50:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 22:47:08 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

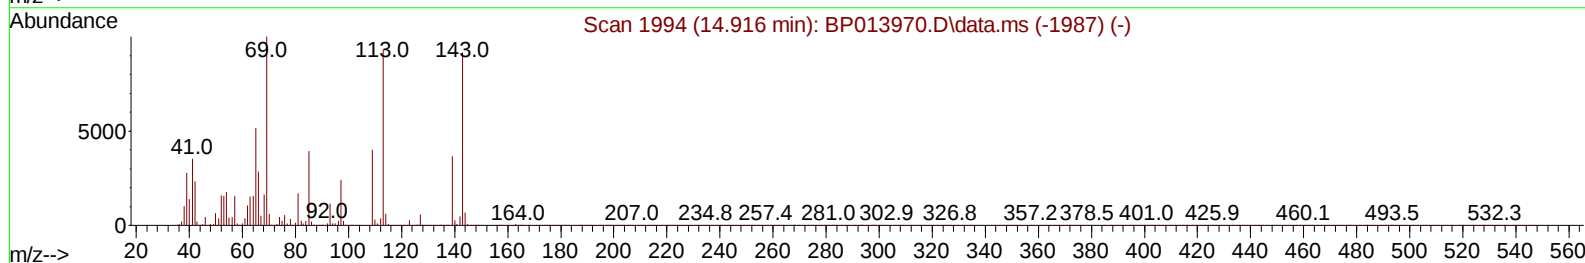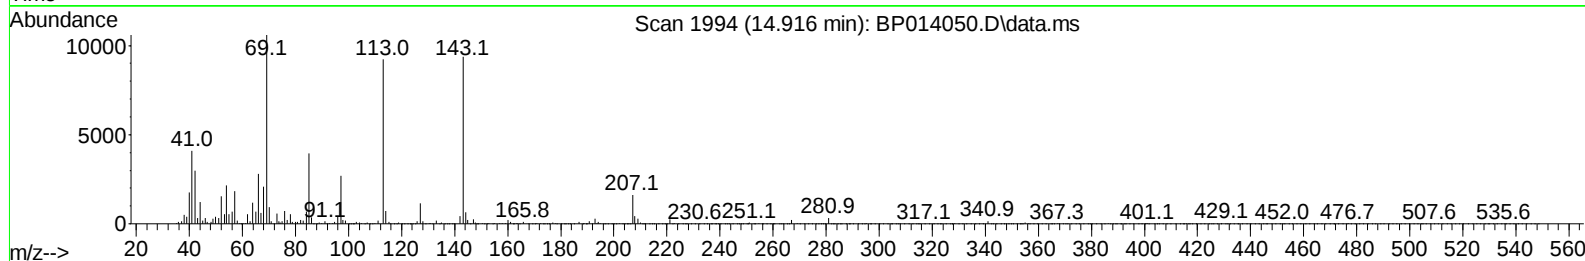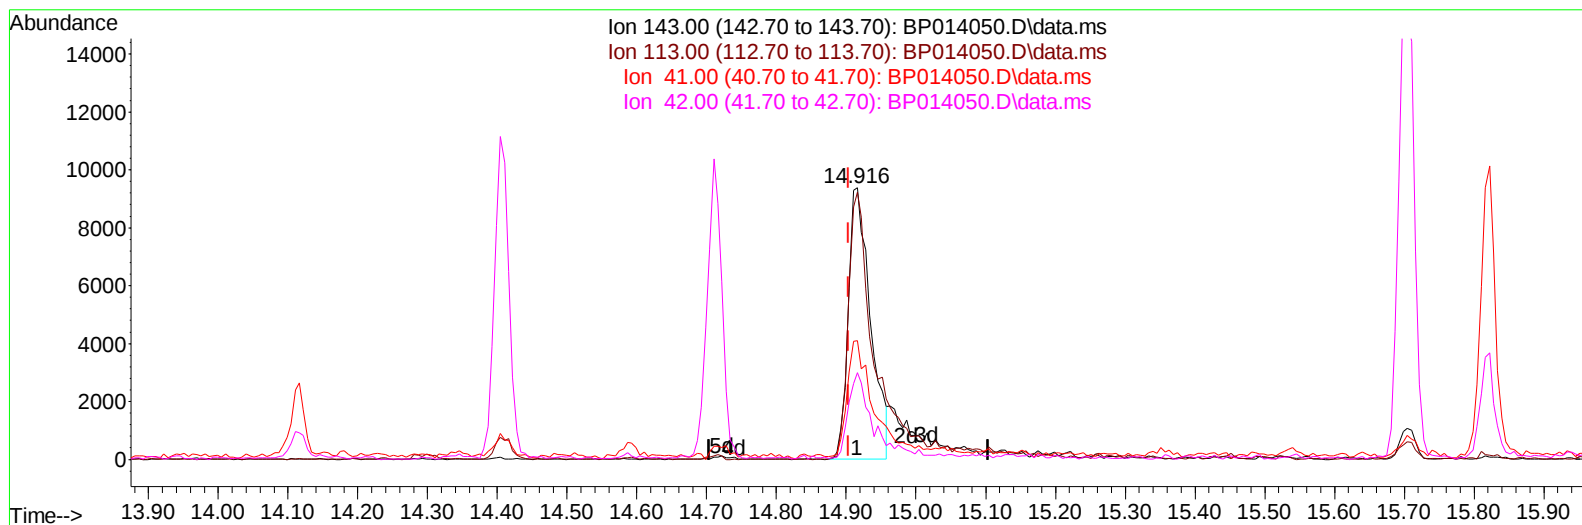

TIC: BP014050.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.012) 3.09 ng/u1

response 20763

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	98.43
41.00	40.20	43.68
42.00	28.50	31.89




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014050.D
Acq On : 11 Mar 2023 02:57
Operator : CG/JU
Sample : 01810-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAF7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 11 03:50:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 22:47:08 2023
Response via : Initial Calibration

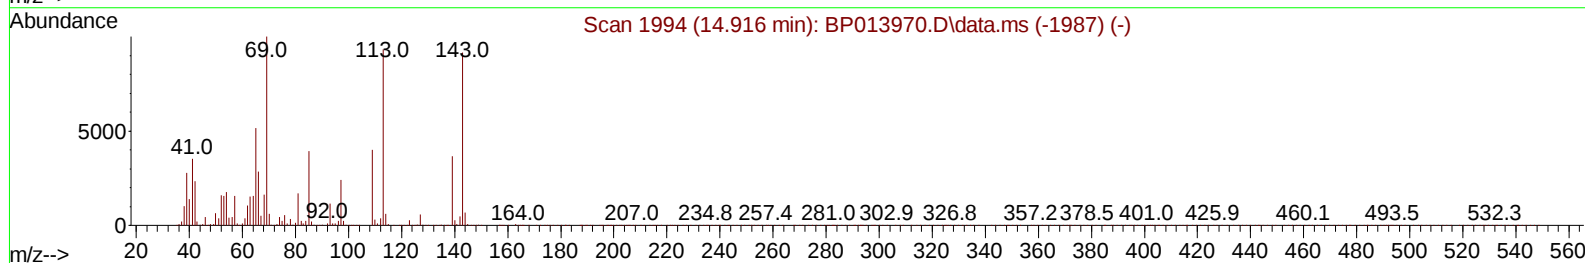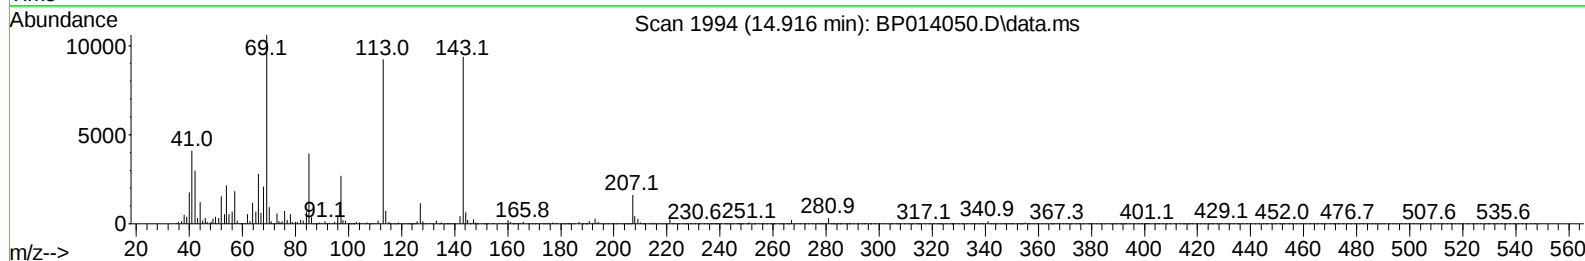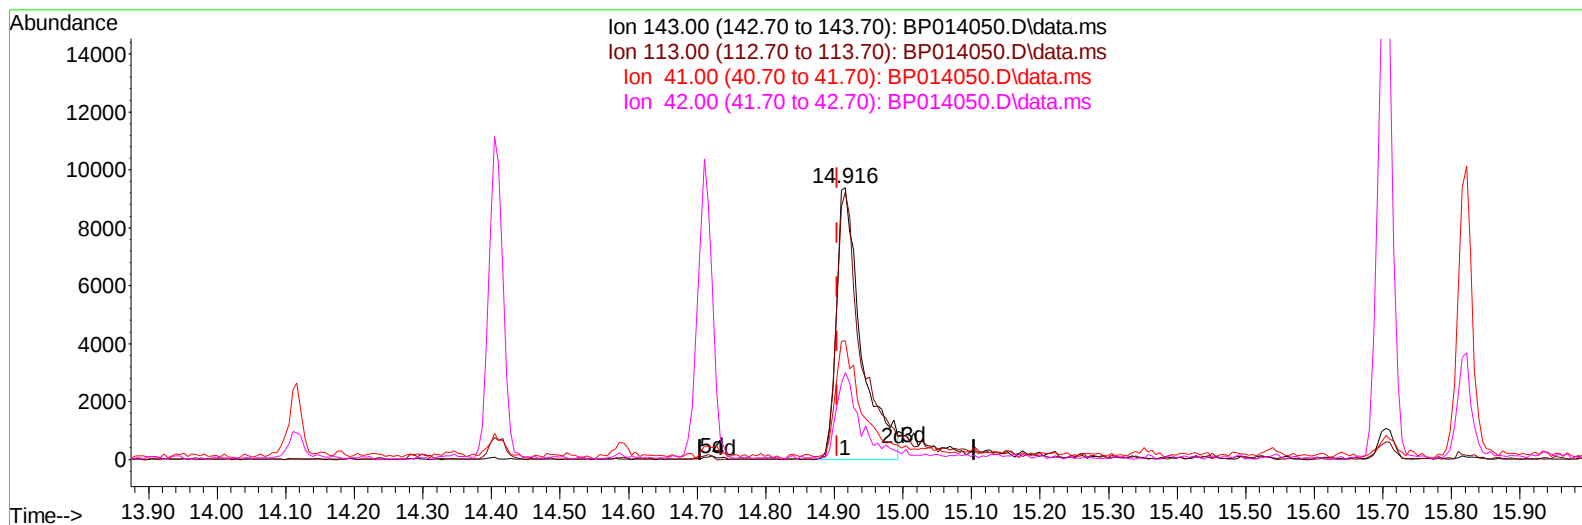

TIC: BP014050.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.012) 3.52 ng/ul m

response 23665

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	98.43
41.00	40.20	43.68
42.00	28.50	31.89

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014050.D
 Acq On : 11 Mar 2023 02:57
 Operator : CG/JU
 Sample : 01810-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAF7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 11 03:50:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 10 22:47:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	145827	20.000	ng/ul	0.00
20) Naphthalene-d8	10.899	136	623871	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	448950	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.469	188	1078318	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1041830	20.000	ng/ul	0.00
88) Perylene-d12	24.080	264	1128547	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	16772	4.345	ng/uL	0.00
4) Pyridine-d5	3.876	84	71204	6.663	ng/ul	0.01
7) Phenol-d5	7.228	99	71708	5.572	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.393	67	240601	32.058	ng/ul	0.00
11) 2-Chlorophenol-d4	7.599	132	212297	21.653	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	143393	13.641	ng/ul	0.00
21) Nitrobenzene-d5	9.246	128	152597	30.655	ng/ul	0.00
24) 2-Nitrophenol-d4	9.975	143	166619	27.962	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	272029	24.263	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	343930	23.180	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	1112665	29.203	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	1193090	29.560	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	23665m	3.525	ng/ul	0.01
60) Fluorene-d10	15.704	176	979475	30.333	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	197255	24.203	ng/ul	0.00
73) Anthracene-d10	17.569	188	1699427	32.465	ng/ul	0.00
81) Pyrene-d10	19.786	212	2146630	37.359	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.916	264	2021645	33.677	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014050.D
Acq On : 11 Mar 2023 02:57
Operator : CG/JU
Sample : 01810-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAF7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 11 03:50:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 22:47:08 2023
Response via : Initial Calibration

