




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014058.D
Acq On : 11 Mar 2023 08:04
Operator : CG/JU
Sample : 01804-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 13 00:50:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 22:47:08 2023
Response via : Initial Calibration

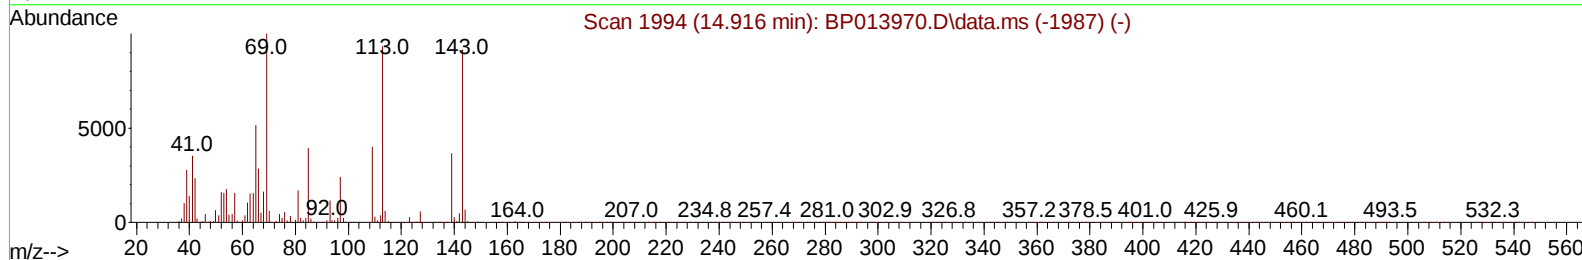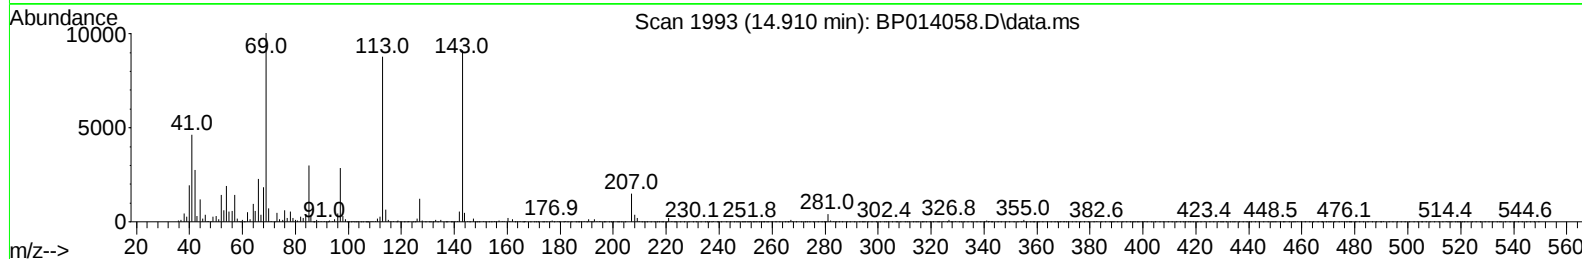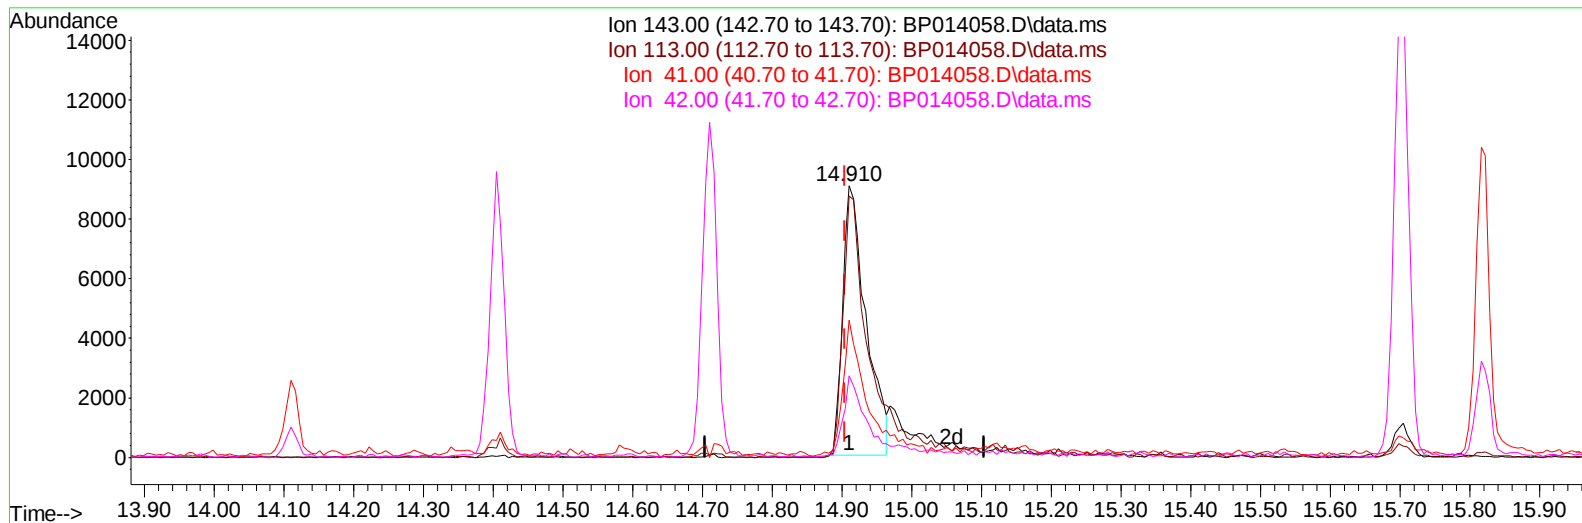

TIC: BP014058.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.006) 2.89 ng/u1

response 20948

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	96.26
41.00	40.20	50.65#
42.00	28.50	30.10




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014058.D
Acq On : 11 Mar 2023 08:04
Operator : CG/JU
Sample : 01804-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 13 00:50:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 22:47:08 2023
Response via : Initial Calibration

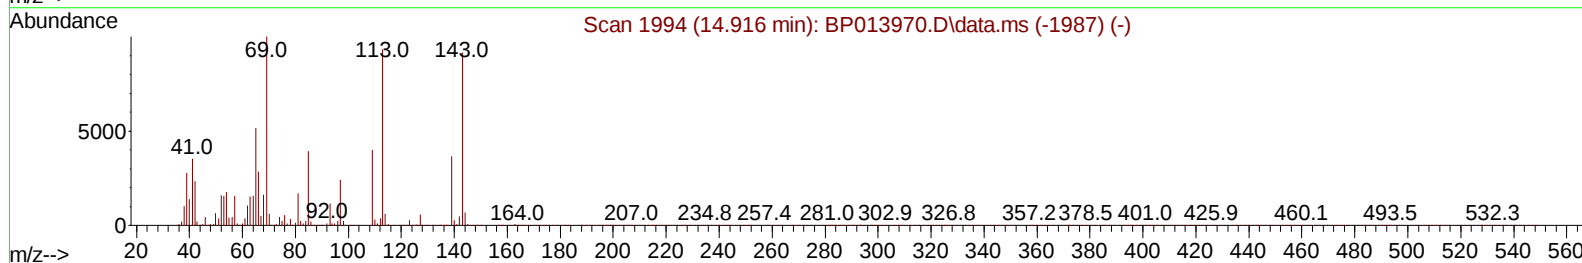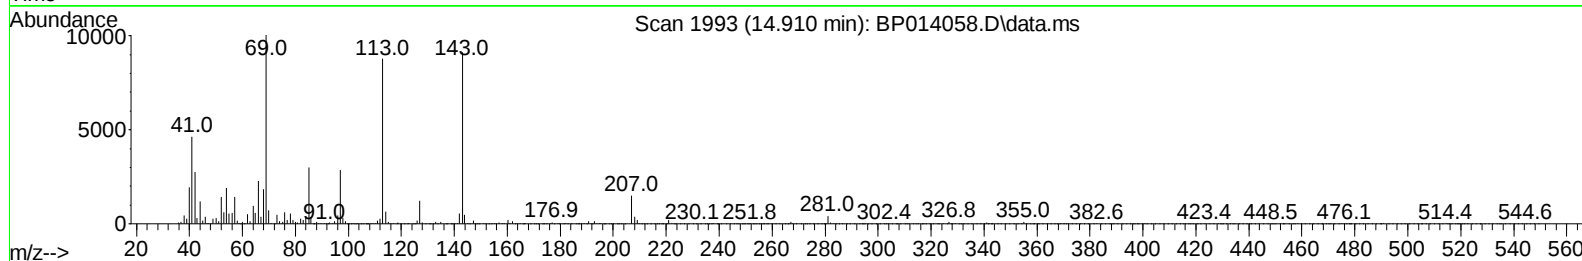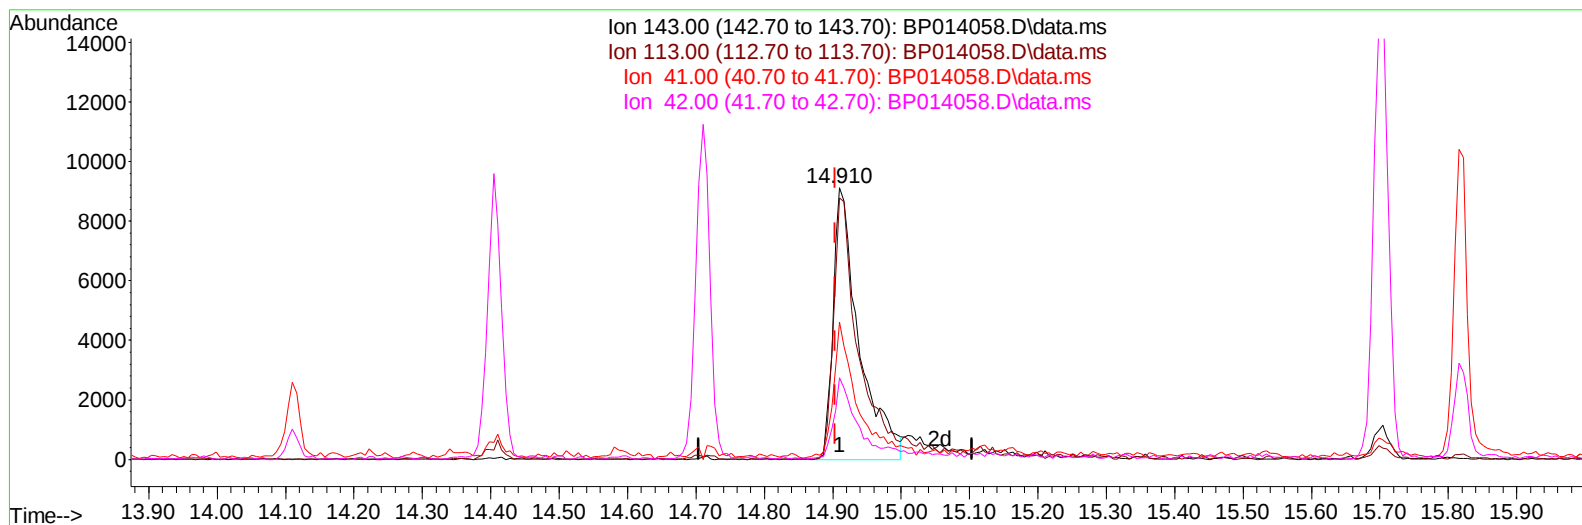

TIC: BP014058.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.006) 3.29 ng/ul m

response 23880

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	96.26
41.00	40.20	50.65#
42.00	28.50	30.10

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014058.D
 Acq On : 11 Mar 2023 08:04
 Operator : CG/JU
 Sample : 01804-09
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 13 00:50:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 10 22:47:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.069	152	159472	20.000	ng/ul	0.00
20) Naphthalene-d8	10.893	136	675399	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	484737	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1144686	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1224587	20.000	ng/ul	0.00
88) Perylene-d12	24.080	264	1195669	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	17047	4.039	ng/uL	0.00
4) Pyridine-d5	3.875	84	66256	5.670	ng/ul	0.01
7) Phenol-d5	7.222	99	68212	4.847	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.393	67	213295	25.988	ng/ul	0.00
11) 2-Chlorophenol-d4	7.599	132	194561	18.146	ng/ul	0.00
15) 4-Methylphenol-d8	8.781	113	129869	11.298	ng/ul	0.00
21) Nitrobenzene-d5	9.246	128	126090	23.398	ng/ul	0.00
24) 2-Nitrophenol-d4	9.969	143	142604	22.106	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	238271	19.630	ng/ul	0.00
31) 4-Chloroaniline-d4	11.034	131	235987	14.691	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	966021	23.482	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	1007721	23.124	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	23880m	3.294	ng/ul	0.00
60) Fluorene-d10	15.704	176	871127	24.986	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	183168	21.172	ng/ul	0.00
73) Anthracene-d10	17.563	188	1530591	27.544	ng/ul	0.00
81) Pyrene-d10	19.786	212	1948909	28.856	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.915	264	1810166	28.461	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014058.D
Acq On : 11 Mar 2023 08:04
Operator : CG/JU
Sample : 01804-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

Quant Time: Mar 13 00:50:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 22:47:08 2023
Response via : Initial Calibration

