

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014023.D
 Acq On : 10 Mar 2023 10:56
 Operator : CG/JU
 Sample : PB151296BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	53	rVB	37560	58280	1.50%	0.151%
2	3.870	113	116	134	rBV	351501	589372	15.13%	1.531%
3	4.199	169	172	179	rVB	7863	11394	0.29%	0.030%
4	7.228	676	687	703	rBV	570388	943467	24.22%	2.451%
5	7.399	710	716	731	rVV	458689	708845	18.20%	1.841%
6	7.605	744	751	762	rBV	569073	926249	23.78%	2.406%
7	8.075	824	831	842	rBV	462875	752149	19.31%	1.954%
8	8.781	943	951	968	rBV	686083	1179117	30.27%	3.063%
9	9.252	1024	1031	1041	rBV	561533	929638	23.86%	2.415%
10	9.975	1146	1154	1166	rBV	484386	818706	21.02%	2.127%
11	10.516	1239	1246	1260	rBV	688541	1208090	31.01%	3.138%
12	10.899	1300	1311	1320	rBV	641029	1094331	28.09%	2.843%
13	11.040	1326	1335	1355	rBV	406783	782417	20.08%	2.032%
14	12.487	1575	1581	1587	rBV2	8335	17582	0.45%	0.046%
15	13.593	1765	1769	1777	rVB4	9722	16500	0.42%	0.043%
16	13.698	1783	1787	1792	rVB8	2637	4733	0.12%	0.012%
17	14.116	1852	1858	1873	rBV	1466396	2036251	52.27%	5.290%
18	14.410	1898	1908	1919	rBV	1529326	2234765	57.37%	5.805%
19	14.716	1953	1960	1971	rVB	1093660	1594443	40.93%	4.142%
20	14.904	1986	1992	2019	rBV	517340	994464	25.53%	2.583%
21	15.710	2122	2129	2141	rBV	1962729	2871090	73.70%	7.458%
22	15.822	2142	2148	2165	rVV	713155	1028135	26.39%	2.671%
23	15.945	2166	2169	2175	rVB4	9832	15555	0.40%	0.040%
24	17.269	2392	2394	2399	rVB6	3655	4308	0.11%	0.011%
25	17.469	2421	2428	2436	rBV	1456501	2071844	53.18%	5.382%
26	17.569	2439	2445	2459	rVV2	2231828	3218375	82.61%	8.360%
27	19.369	2747	2751	2757	rBV3	30662	44706	1.15%	0.116%
28	19.439	2760	2763	2767	rVB2	25788	34009	0.87%	0.088%
29	19.792	2817	2823	2838	rBV	2990870	3895670	100.00%	10.120%
30	21.545	3116	3121	3131	rBV	1666482	2375967	60.99%	6.172%
31	23.921	3518	3525	3534	rVB2	1887512	3767632	96.71%	9.787%
32	24.086	3546	3553	3564	rVB	1091367	2267438	58.20%	5.890%




Sum of corrected areas: 38495522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014023.D
Acq On : 10 Mar 2023 10:56
Operator : CG/JU
Sample : PB151296BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

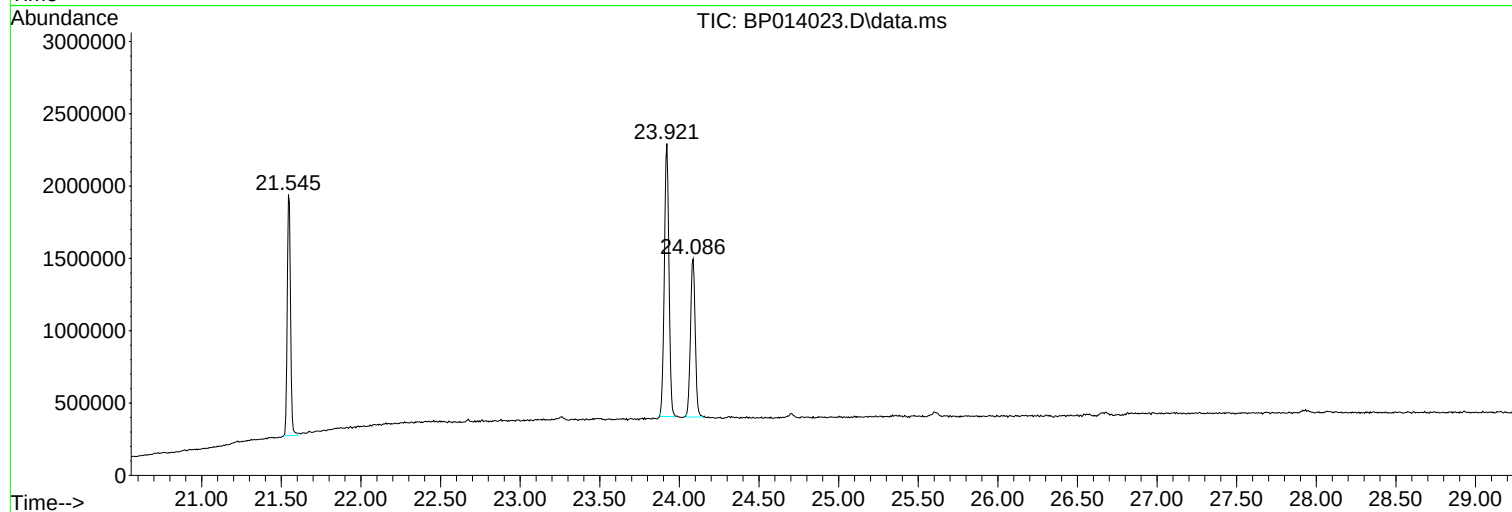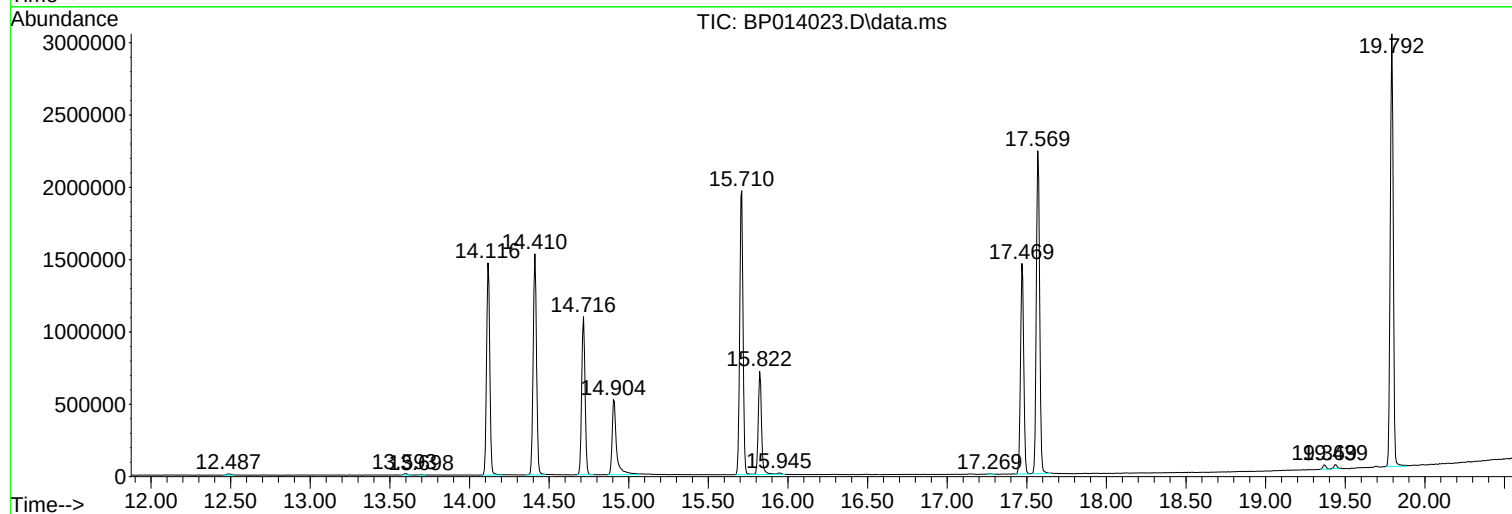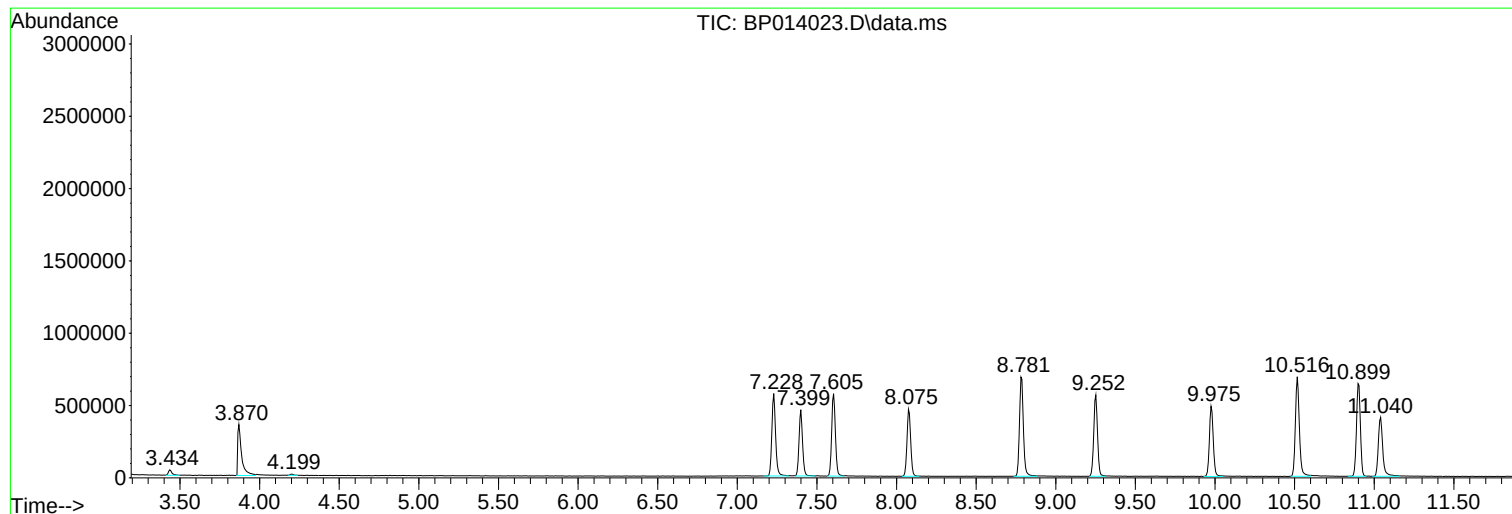

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014023.D
Acq On : 10 Mar 2023 10:56
Operator : CG/JU
Sample : PB151296BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014023.D
Acq On : 10 Mar 2023 10:56
Operator : CG/JU
Sample : PB151296BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------