

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014034.D
 Acq On : 10 Mar 2023 17:13
 Operator : CG/JU
 Sample : 01804-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	48	rBV	25398	35045	0.81%	0.092%
2	3.875	114	117	132	rBV	96759	169751	3.91%	0.447%
3	4.099	151	155	160	rVB2	11557	18594	0.43%	0.049%
4	4.199	168	172	175	rBV2	9586	12359	0.28%	0.033%
5	4.305	186	190	193	rBV5	6280	7325	0.17%	0.019%
6	5.140	328	332	340	rVB5	6783	12230	0.28%	0.032%
7	6.452	547	555	560	rVB3	6028	9961	0.23%	0.026%
8	7.228	681	687	701	rBV	78939	145728	3.36%	0.384%
9	7.399	708	716	725	rBV	401756	643910	14.83%	1.697%
10	7.604	742	751	763	rBV	366378	615551	14.18%	1.622%
11	8.075	824	831	841	rBV	545010	866814	19.96%	2.284%
12	8.787	944	952	967	rBV	259261	465407	10.72%	1.226%
13	9.251	1022	1031	1046	rBV	527189	889895	20.49%	2.345%
14	9.634	1091	1096	1104	rBV7	4908	9212	0.21%	0.024%
15	9.975	1146	1154	1167	rBV	424765	730619	16.83%	1.925%
16	10.516	1238	1246	1271	rBV	570049	1019039	23.47%	2.685%
17	10.898	1302	1311	1321	rBV	777126	1292509	29.77%	3.406%
18	11.040	1326	1335	1352	rBV	462522	851290	19.61%	2.243%
19	12.134	1515	1521	1524	rBV7	3270	4734	0.11%	0.012%
20	12.481	1574	1580	1587	rBV3	8546	16209	0.37%	0.043%
21	14.116	1849	1858	1873	rBV	1339116	1897589	43.70%	5.000%
22	14.410	1901	1908	1918	rBV	1401123	2011511	46.32%	5.300%
23	14.716	1950	1960	1970	rBV	1283998	1845498	42.50%	4.863%
24	14.922	1989	1995	2013	rBV2	40271	119933	2.76%	0.316%
25	15.122	2026	2029	2038	rVB10	4181	9997	0.23%	0.026%
26	15.704	2122	2128	2137	rBV	1908231	2810656	64.73%	7.406%
27	15.822	2142	2148	2164	rVV	730590	1041020	23.97%	2.743%
28	15.951	2165	2170	2174	rVB7	9734	16626	0.38%	0.044%
29	16.404	2242	2247	2250	rBV5	3166	5436	0.13%	0.014%
30	16.628	2278	2285	2289	rBV9	2057	6770	0.16%	0.018%
31	17.145	2369	2373	2377	rBV6	3846	7075	0.16%	0.019%
32	17.469	2421	2428	2438	rBV	1704617	2419707	55.73%	6.375%
33	17.569	2438	2445	2459	rVV2	2498021	3467526	79.86%	9.136%
34	17.733	2471	2473	2480	rVB7	3681	6341	0.15%	0.017%
35	18.327	2570	2574	2582	rBV3	29025	57535	1.33%	0.152%
36	19.363	2747	2750	2757	rBV3	35010	53148	1.22%	0.140%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014034.D
Acq On : 10 Mar 2023 17:13
Operator : CG/JU
Sample : 01804-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION

37	19.439	2759	2763	2766	rBV	31373	43098	0.99%	0.114%
38	19.557	2779	2783	2790	rBV8	26961	52171	1.20%	0.137%
39	19.792	2817	2823	2832	rBV	3319665	4304943	99.14%	11.343%
40	21.545	3116	3121	3128	rBV	2074923	2792260	64.31%	7.357%
41	23.921	3517	3525	3535	rBV2	2022675	4342179	100.00%	11.441%
42	24.086	3546	3553	3564	rVB2	1314575	2826142	65.09%	7.446%




Sum of corrected areas: 37953343

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014034.D
Acq On : 10 Mar 2023 17:13
Operator : CG/JU
Sample : 01804-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

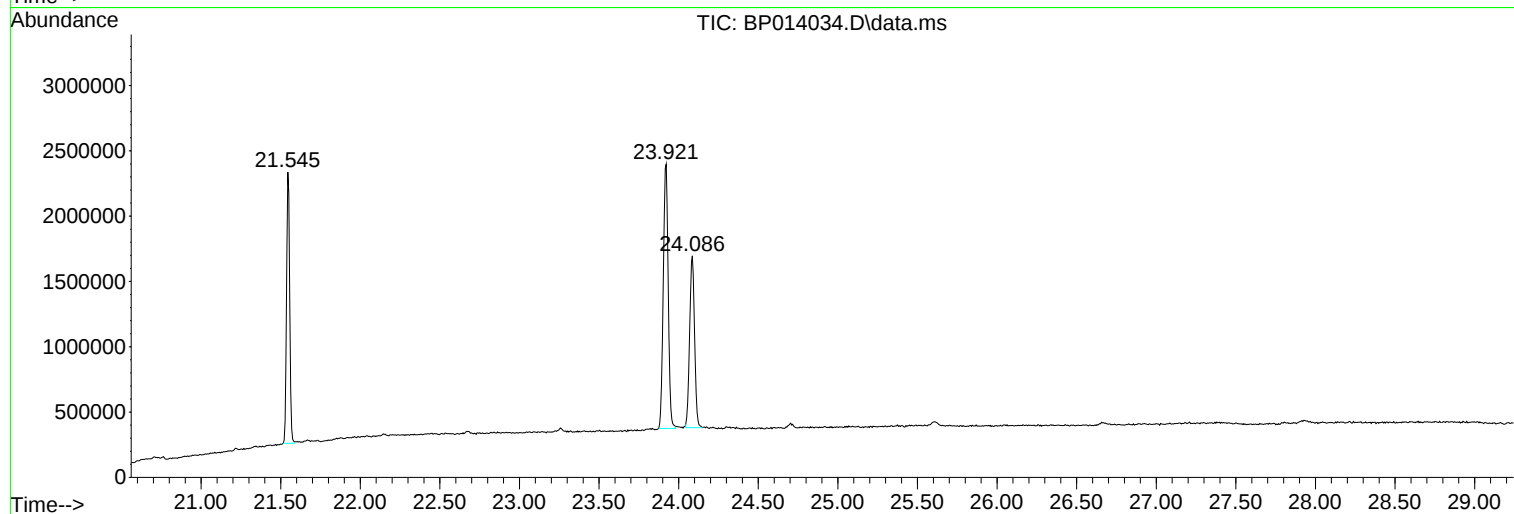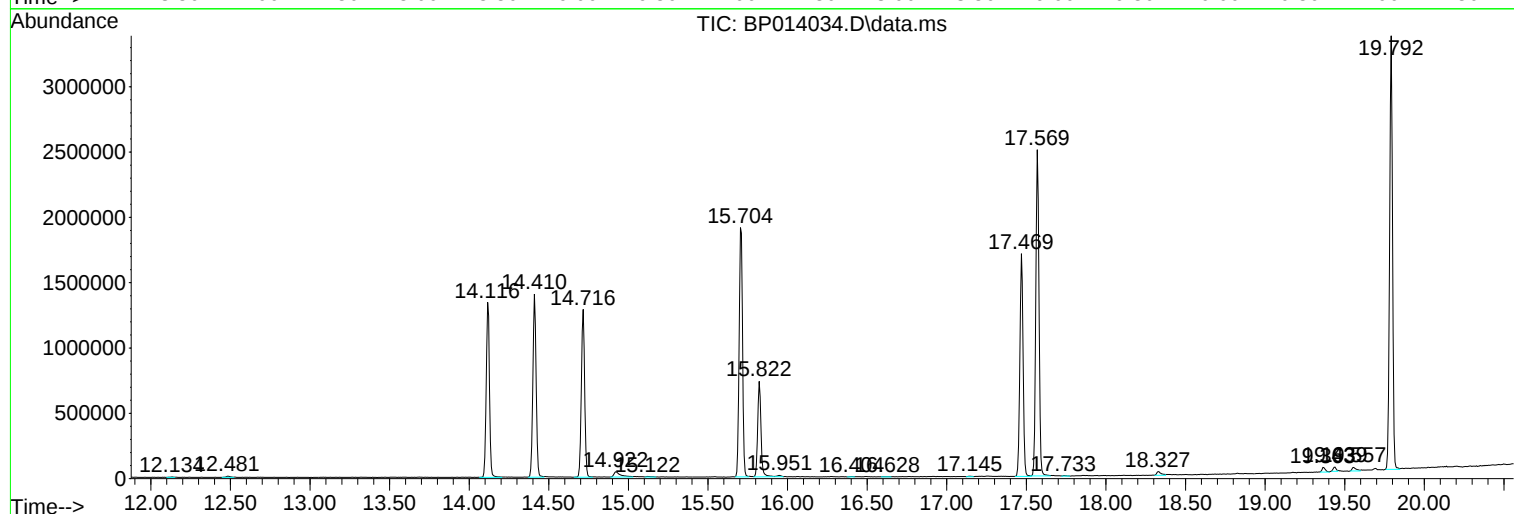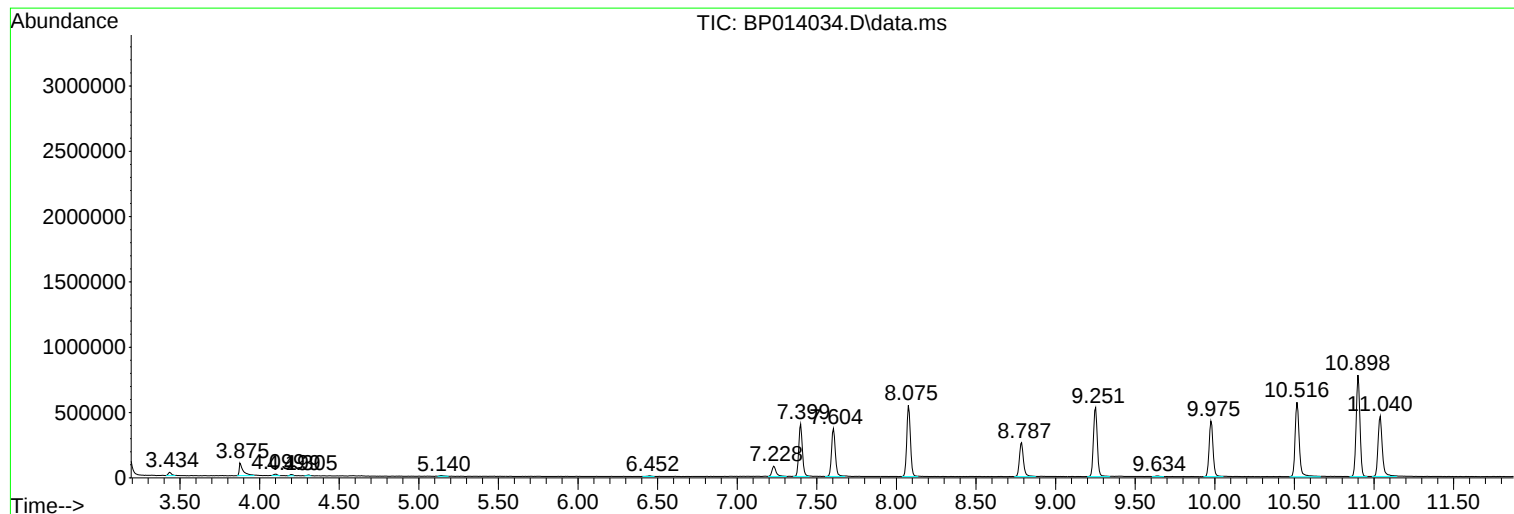

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014034.D
Acq On : 10 Mar 2023 17:13
Operator : CG/JU
Sample : 01804-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014034.D
Acq On : 10 Mar 2023 17:13
Operator : CG/JU
Sample : 01804-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc