

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014036.D
 Acq On : 10 Mar 2023 18:22
 Operator : CG/JU
 Sample : 01804-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	48	rVB	25030	33778	0.77%	0.089%
2	3.875	115	117	132	rBV	104845	193089	4.42%	0.508%
3	4.099	150	155	161	rVB	12509	19853	0.45%	0.052%
4	4.199	168	172	181	rVB	10518	16615	0.38%	0.044%
5	4.311	186	191	196	rVB6	6786	11160	0.26%	0.029%
6	5.146	327	333	337	rBV3	6418	14758	0.34%	0.039%
7	6.446	551	554	558	rVB4	6350	8755	0.20%	0.023%
8	7.228	681	687	699	rVV	95686	169978	3.89%	0.447%
9	7.399	708	716	731	rBV	400288	646127	14.80%	1.701%
10	7.605	743	751	761	rBV	383978	638525	14.63%	1.681%
11	8.075	824	831	839	rBV	504826	800182	18.33%	2.106%
12	8.781	943	951	962	rBV	298380	521973	11.96%	1.374%
13	9.246	1022	1030	1043	rBV	498480	867433	19.87%	2.283%
14	9.634	1092	1096	1102	rVB4	9058	12987	0.30%	0.034%
15	9.975	1146	1154	1172	rBV	433836	748356	17.14%	1.970%
16	10.516	1238	1246	1266	rBV	594090	1044139	23.92%	2.748%
17	10.899	1300	1311	1324	rVB	722068	1198844	27.46%	3.156%
18	11.040	1324	1335	1351	rBV	484129	918468	21.04%	2.418%
19	12.128	1516	1520	1526	rVB3	8957	13401	0.31%	0.035%
20	12.481	1574	1580	1588	rVB3	9167	19336	0.44%	0.051%
21	13.522	1750	1757	1765	rBV9	4677	8148	0.19%	0.021%
22	13.693	1780	1786	1790	rBV9	3486	5490	0.13%	0.014%
23	14.116	1851	1858	1868	rBV	1340486	1858519	42.57%	4.892%
24	14.234	1875	1878	1882	rVB5	3833	4431	0.10%	0.012%
25	14.345	1890	1897	1899	rBV8	2724	5219	0.12%	0.014%
26	14.410	1901	1908	1919	rVV	1407482	2030783	46.51%	5.345%
27	14.716	1953	1960	1969	rBV	1146056	1697290	38.88%	4.468%
28	14.828	1975	1979	1987	rVB	2085	5143	0.12%	0.014%
29	14.916	1987	1994	2009	rBV2	58164	163258	3.74%	0.430%
30	15.128	2025	2030	2040	rVB2	4998	14292	0.33%	0.038%
31	15.657	2114	2120	2122	rBV7	3415	6593	0.15%	0.017%
32	15.704	2122	2128	2141	rVV	1947673	2771371	63.48%	7.295%
33	15.822	2142	2148	2162	rVV	754162	1056575	24.20%	2.781%
34	15.945	2166	2169	2179	rVB7	11066	18991	0.43%	0.050%
35	16.069	2185	2190	2198	rVB	78781	109817	2.52%	0.289%
36	16.404	2242	2247	2250	rBV7	4183	6852	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014036.D
 Acq On : 10 Mar 2023 18:22
 Operator : CG/JU
 Sample : 01804-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	16.586	2274	2278	2285	rBV9	1977	4586	0.11%	0.012%
38	16.869	2318	2326	2330	rBV9	5335	13266	0.30%	0.035%
39	17.145	2369	2373	2379	rBV9	4952	7780	0.18%	0.020%
40	17.263	2388	2393	2394	rBV5	4169	6648	0.15%	0.017%
41	17.469	2422	2428	2438	rBV	1585289	2222607	50.91%	5.850%
42	17.569	2438	2445	2454	rBV	2489392	3416061	78.24%	8.992%
43	18.328	2569	2574	2583	rBV	98796	165020	3.78%	0.434%
44	18.604	2618	2621	2625	rBV5	5396	5724	0.13%	0.015%
45	19.369	2747	2751	2756	rBV3	35892	48682	1.12%	0.128%
46	19.439	2758	2763	2771	rVV2	37634	72220	1.65%	0.190%
47	19.551	2779	2782	2791	rBV9	36617	83061	1.90%	0.219%
48	19.686	2803	2805	2809	rBV4	15643	18410	0.42%	0.048%
49	19.792	2817	2823	2831	rBV	3251705	4320393	98.96%	11.372%
50	21.216	3062	3065	3074	rBV3	162424	241202	5.52%	0.635%
51	21.545	3116	3121	3128	rBV	2017161	2683393	61.46%	7.063%
52	23.916	3517	3524	3538	rVB2	2158983	4365893	100.00%	11.492%
53	24.086	3546	3553	3567	rVB2	1254375	2655095	60.81%	6.989%




Sum of corrected areas: 37990570

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014036.D
Acq On : 10 Mar 2023 18:22
Operator : CG/JU
Sample : 01804-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

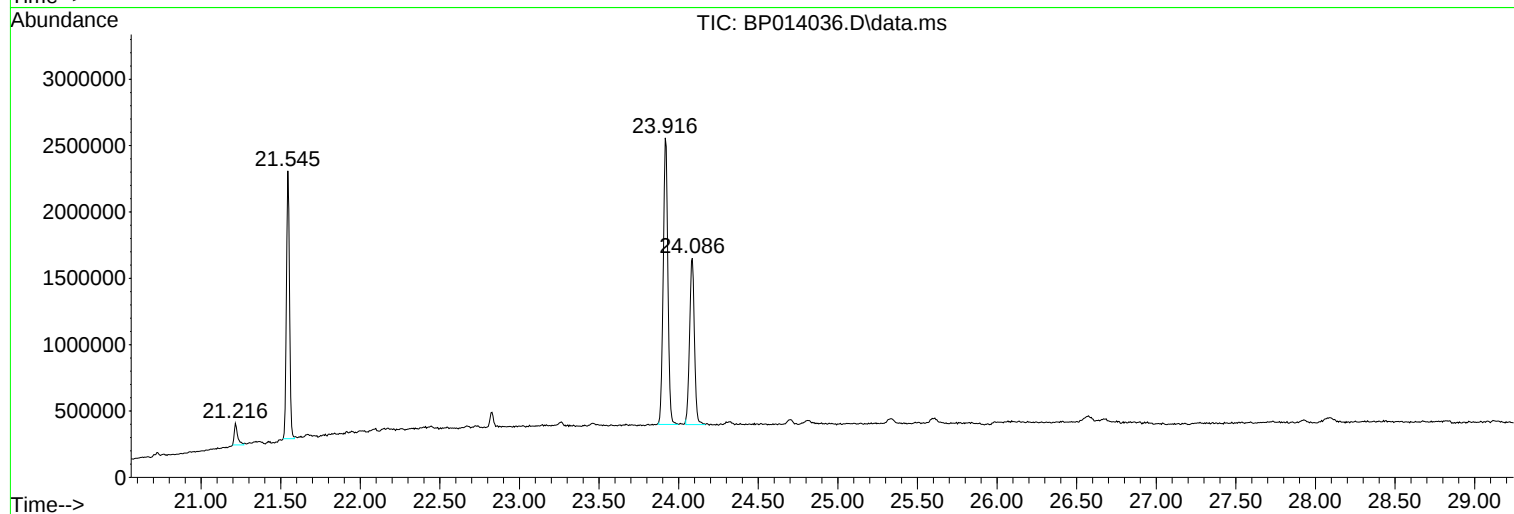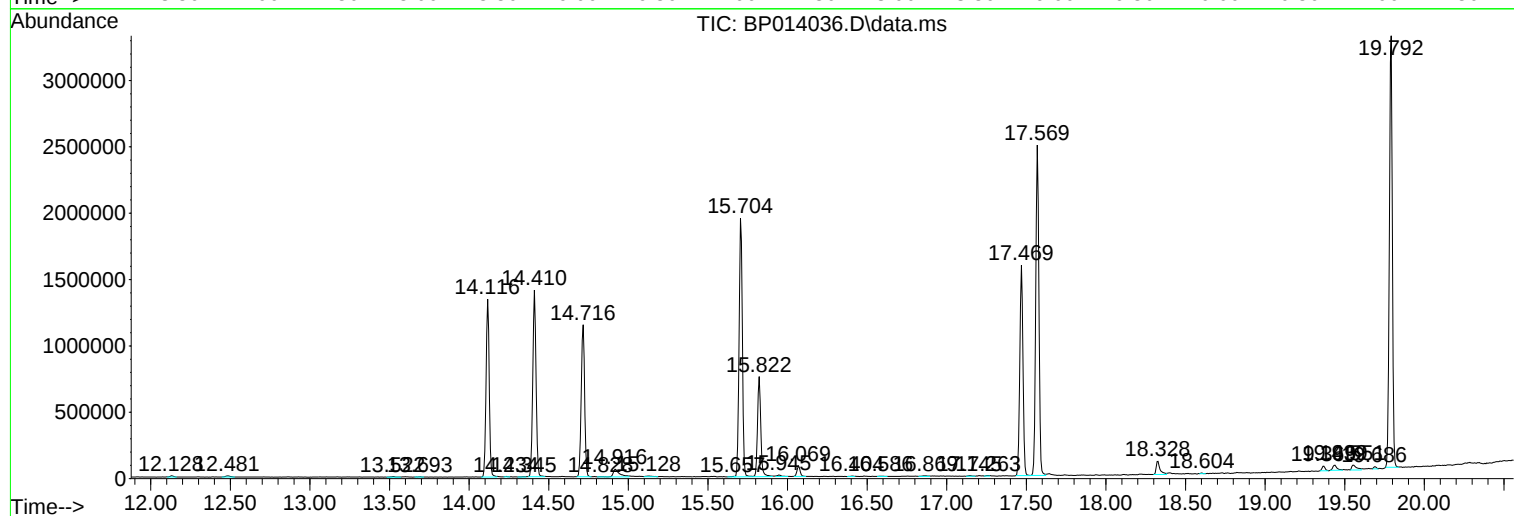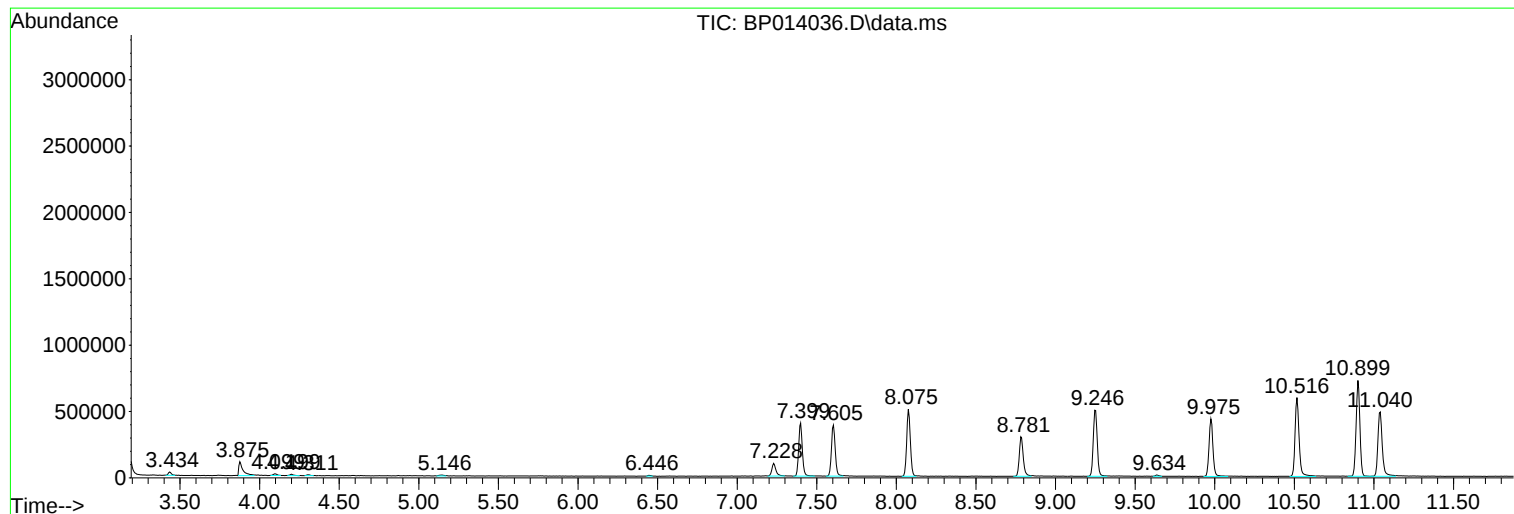

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014036.D
Acq On : 10 Mar 2023 18:22
Operator : CG/JU
Sample : 01804-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014036.D
Acq On : 10 Mar 2023 18:22
Operator : CG/JU
Sample : 01804-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------