

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014037.D
 Acq On : 10 Mar 2023 18:57
 Operator : CG/JU
 Sample : 01804-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	39	42	48	rVB	22999	31654	0.74%	0.086%
2	3.875	115	117	131	rBV	91081	155200	3.62%	0.423%
3	4.099	150	155	163	rVB2	15702	24077	0.56%	0.066%
4	4.199	168	172	177	rBV	9507	14278	0.33%	0.039%
5	4.305	186	190	197	rVB6	8594	14286	0.33%	0.039%
6	5.140	327	332	343	rVB5	8283	21720	0.51%	0.059%
7	6.446	550	554	559	rBV4	6561	9973	0.23%	0.027%
8	7.228	681	687	704	rVB	79838	145184	3.39%	0.396%
9	7.399	708	716	730	rBV	385128	623579	14.54%	1.700%
10	7.605	743	751	762	rBV	357049	594658	13.87%	1.621%
11	8.075	823	831	840	rBV	485919	773214	18.03%	2.108%
12	8.781	945	951	967	rBV	259706	465110	10.85%	1.268%
13	9.252	1022	1031	1044	rBV	497380	839399	19.58%	2.288%
14	9.640	1091	1097	1103	rVB	20074	30139	0.70%	0.082%
15	9.975	1147	1154	1166	rBV	412101	700855	16.35%	1.910%
16	10.516	1238	1246	1260	rBV	552132	979052	22.83%	2.669%
17	10.899	1302	1311	1319	rBV	688497	1165571	27.18%	3.177%
18	11.040	1327	1335	1348	rBV	456751	860253	20.06%	2.345%
19	12.134	1516	1521	1527	rVB3	14306	22533	0.53%	0.061%
20	12.481	1575	1580	1587	rVB2	9796	16387	0.38%	0.045%
21	13.522	1751	1757	1761	rBV9	2787	4821	0.11%	0.013%
22	14.116	1851	1858	1870	rBV	1325668	1801935	42.03%	4.912%
23	14.410	1901	1908	1920	rBV	1340414	1959340	45.70%	5.341%
24	14.716	1953	1960	1970	rBV	1120280	1653830	38.57%	4.508%
25	14.922	1989	1995	2011	rBV	43797	125746	2.93%	0.343%
26	15.128	2025	2030	2037	rVB	3002	7430	0.17%	0.020%
27	15.528	2094	2098	2100	rBV5	3255	5656	0.13%	0.015%
28	15.704	2114	2128	2140	rBV	1902562	2724894	63.55%	7.428%
29	15.822	2142	2148	2158	rBV	713027	995336	23.21%	2.713%
30	15.951	2166	2170	2175	rVB4	11159	16125	0.38%	0.044%
31	16.069	2185	2190	2200	rVB	55011	79815	1.86%	0.218%
32	16.404	2242	2247	2248	rBV4	3899	4366	0.10%	0.012%
33	16.645	2283	2288	2291	rBV6	2354	4570	0.11%	0.012%
34	17.145	2369	2373	2377	rBV6	3442	5267	0.12%	0.014%
35	17.198	2379	2382	2385	rBV5	3390	4430	0.10%	0.012%
36	17.257	2388	2392	2399	rVB6	5538	9559	0.22%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014037.D
 Acq On : 10 Mar 2023 18:57
 Operator : CG/JU
 Sample : 01804-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	17.469	2421	2428	2435	rBV	1532306	2170907	50.63%	5.918%
38	17.569	2438	2445	2454	rVV	2391016	3332686	77.73%	9.085%
39	17.739	2471	2474	2480	rVB8	3444	5496	0.13%	0.015%
40	18.322	2569	2573	2583	rBV	74369	132981	3.10%	0.362%
41	18.728	2640	2642	2647	rVB6	8480	10613	0.25%	0.029%
42	19.369	2747	2751	2756	rBV2	35231	50094	1.17%	0.137%
43	19.433	2758	2762	2769	rBV	35698	57471	1.34%	0.157%
44	19.551	2779	2782	2791	rBV6	41954	78110	1.82%	0.213%
45	19.792	2817	2823	2834	rBV	3136379	4230014	98.65%	11.531%
46	21.216	3062	3065	3074	rBV3	117025	181964	4.24%	0.496%
47	21.545	3116	3121	3136	rBV	2024648	2704346	63.07%	7.372%
48	23.916	3517	3524	3536	rVB2	2031735	4287768	100.00%	11.688%
49	24.086	3546	3553	3564	rVB2	1198764	2552316	59.53%	6.957%




Sum of corrected areas: 36685008

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014037.D
Acq On : 10 Mar 2023 18:57
Operator : CG/JU
Sample : 01804-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

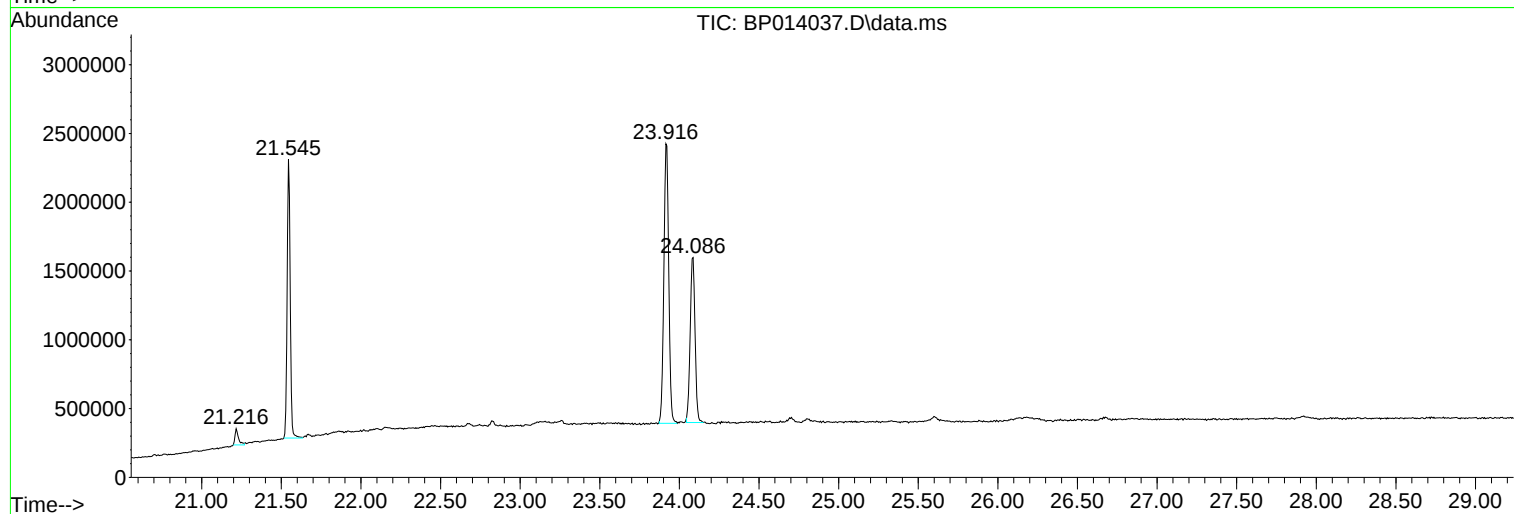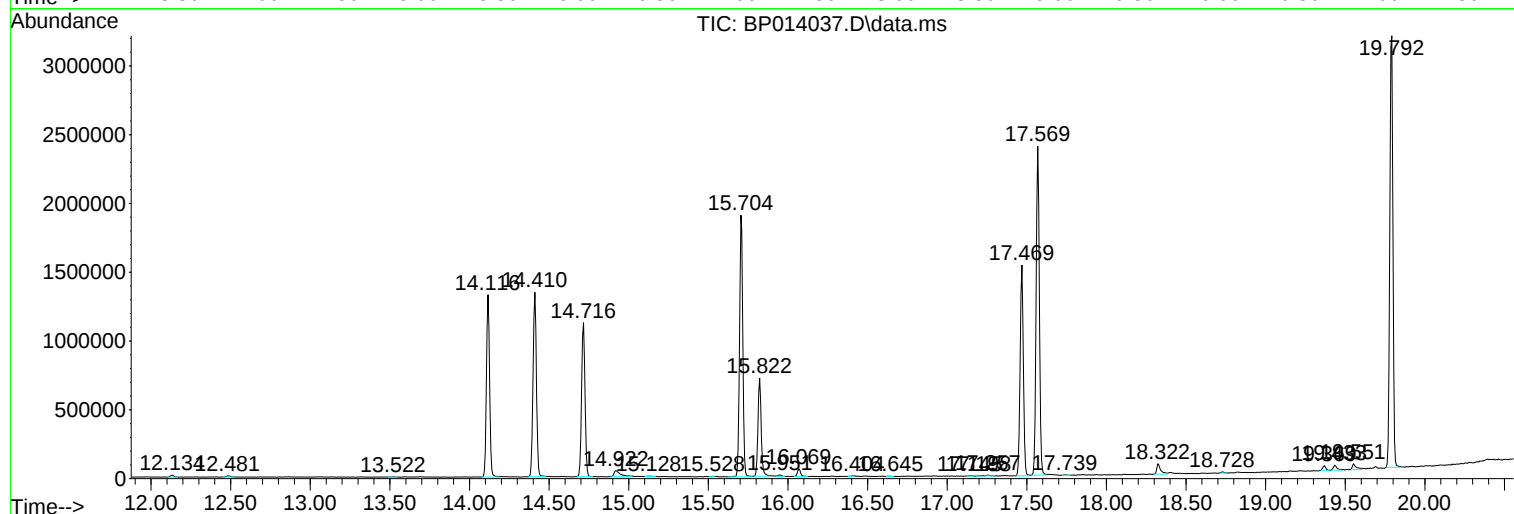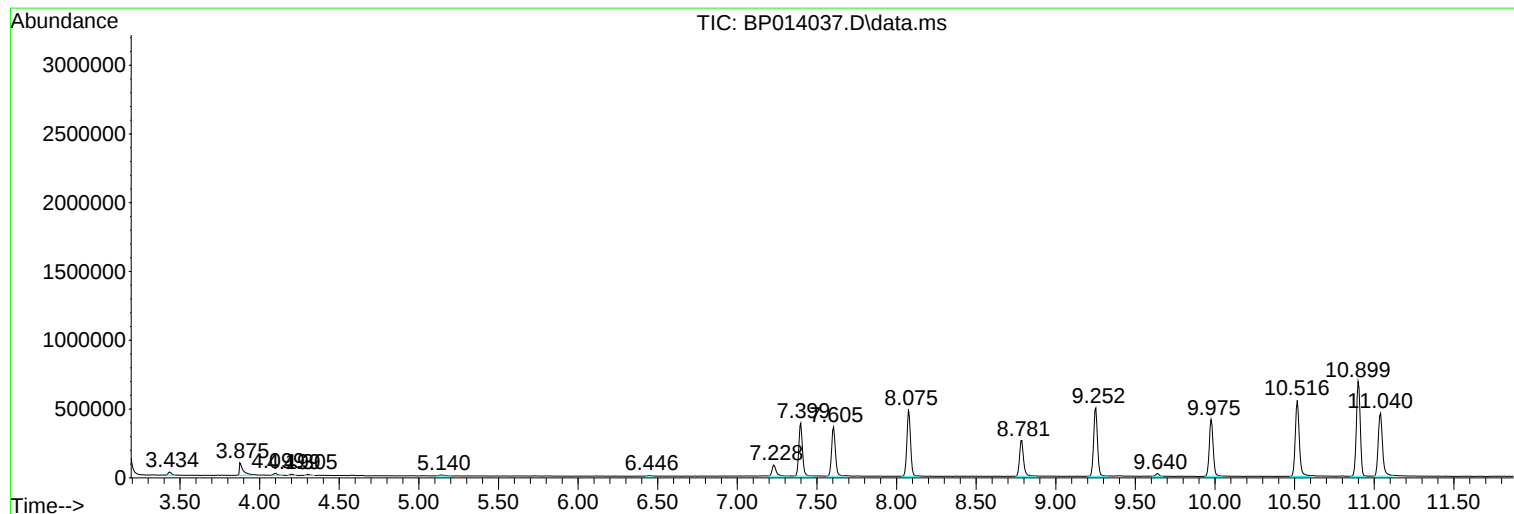

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014037.D
Acq On : 10 Mar 2023 18:57
Operator : CG/JU
Sample : 01804-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014037.D
Acq On : 10 Mar 2023 18:57
Operator : CG/JU
Sample : 01804-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------