

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014040.D
 Acq On : 10 Mar 2023 21:14
 Operator : CG/JU
 Sample : PB151258BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	53	rVB	42629	61139	1.34%	0.144%
2	3.864	112	115	129	rBV	521971	818450	17.90%	1.922%
3	4.199	167	172	177	rBV3	7768	14260	0.31%	0.033%
4	7.228	680	687	704	rBV	634248	1036242	22.66%	2.433%
5	7.399	707	716	729	rBV	468307	765394	16.74%	1.797%
6	7.599	743	750	762	rBV	600790	1006817	22.02%	2.364%
7	8.075	824	831	849	rVB	456601	740971	16.21%	1.740%
8	8.781	944	951	969	rBV	783207	1312778	28.71%	3.082%
9	9.246	1021	1030	1045	rBV	617743	1039039	22.72%	2.440%
10	9.975	1146	1154	1164	rBV	541508	900224	19.69%	2.114%
11	10.516	1239	1246	1268	rBV	771516	1372942	30.03%	3.224%
12	10.898	1303	1311	1320	rBV	643539	1066904	23.33%	2.505%
13	11.034	1327	1334	1349	rBV	726637	1316375	28.79%	3.091%
14	12.487	1575	1581	1592	rVB2	10410	23035	0.50%	0.054%
15	13.592	1765	1769	1775	rBV7	5096	9464	0.21%	0.022%
16	13.687	1782	1785	1793	rVB9	2875	5762	0.13%	0.014%
17	14.116	1850	1858	1872	rBV	1620409	2221309	48.58%	5.216%
18	14.410	1901	1908	1921	rBV	1635357	2389793	52.27%	5.611%
19	14.716	1952	1960	1973	rBV	1048789	1555969	34.03%	3.653%
20	14.904	1985	1992	2021	rBV	648537	1156880	25.30%	2.716%
21	15.122	2027	2029	2036	rVB7	3839	5779	0.13%	0.014%
22	15.704	2121	2128	2138	rBV	2254444	3134111	68.54%	7.359%
23	15.822	2142	2148	2162	rVV	813036	1145627	25.06%	2.690%
24	15.945	2166	2169	2175	rVB5	12528	18910	0.41%	0.044%
25	17.145	2370	2373	2377	rVB6	3272	4736	0.10%	0.011%
26	17.469	2422	2428	2438	rVV	1487580	2051911	44.88%	4.818%
27	17.569	2438	2445	2460	rVV	2550713	3630974	79.41%	8.526%
28	19.369	2747	2751	2756	rVB3	31543	42048	0.92%	0.099%
29	19.433	2759	2762	2769	rVB2	30964	43397	0.95%	0.102%
30	19.792	2816	2823	2834	rBV	3356651	4572438	100.00%	10.736%
31	21.545	3116	3121	3128	rBV	1857168	2467597	53.97%	5.794%
32	23.915	3517	3524	3536	rVB2	2101949	4371561	95.61%	10.264%
33	24.080	3546	3552	3563	rVB2	1078133	2286338	50.00%	5.368%




Sum of corrected areas: 42589174

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014040.D
Acq On : 10 Mar 2023 21:14
Operator : CG/JU
Sample : PB151258BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK258

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

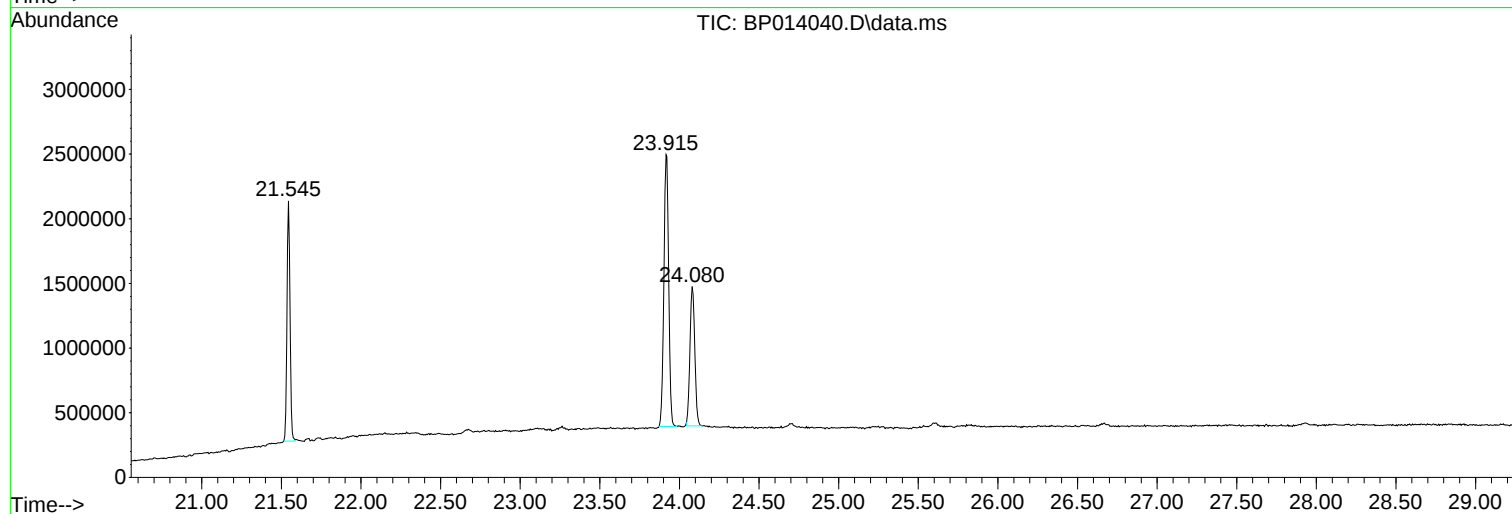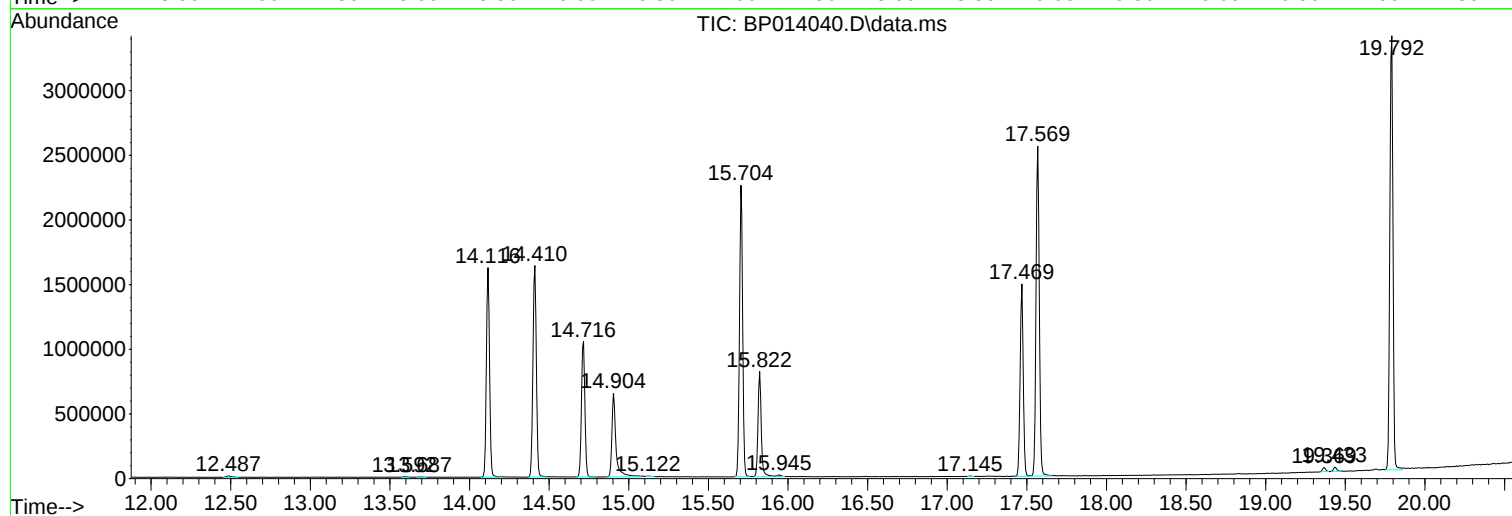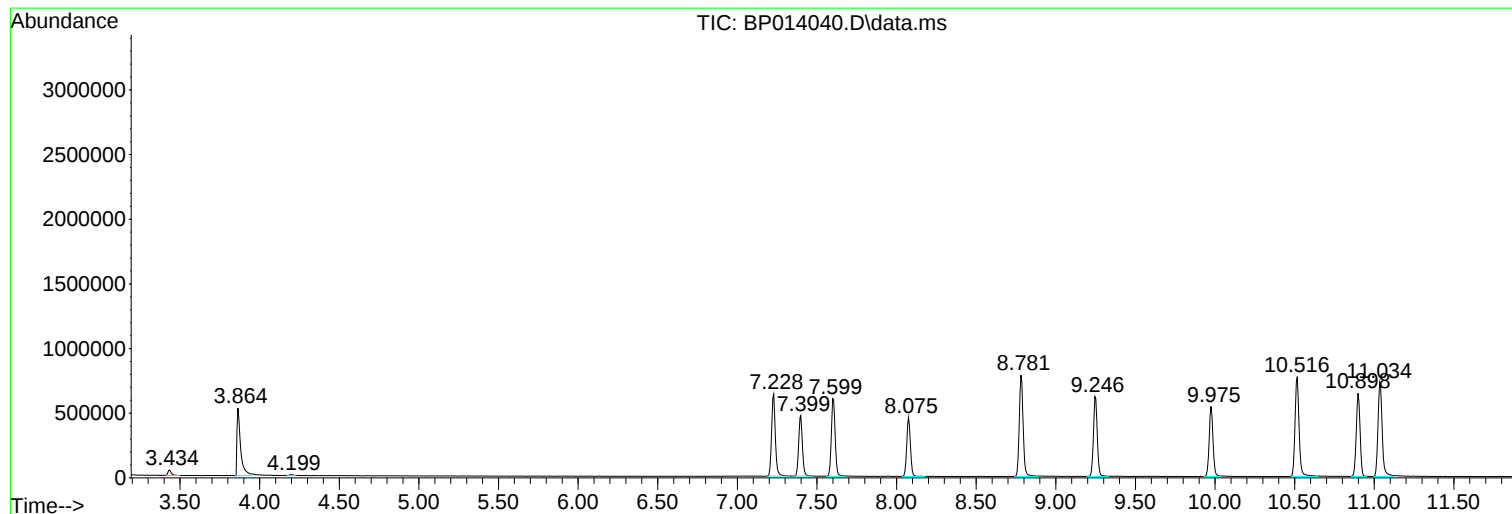

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014040.D
Acq On : 10 Mar 2023 21:14
Operator : CG/JU
Sample : PB151258BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK258

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014040.D
Acq On : 10 Mar 2023 21:14
Operator : CG/JU
Sample : PB151258BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK258

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------