

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014041.D
 Acq On : 10 Mar 2023 21:48
 Operator : CG/JU
 Sample : PB151260BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	49	rBV	32298	45634	1.25%	0.128%
2	3.863	112	115	138	rBV	403549	680274	18.57%	1.913%
3	4.199	168	172	176	rBV3	8855	11687	0.32%	0.033%
4	7.228	680	687	702	rBV	489427	809428	22.10%	2.277%
5	7.398	709	716	727	rVB	371297	598023	16.33%	1.682%
6	7.598	742	750	761	rBV	474838	789443	21.56%	2.220%
7	8.075	824	831	843	rBV	430806	685713	18.72%	1.929%
8	8.781	943	951	966	rBV	628466	1057152	28.87%	2.973%
9	9.245	1023	1030	1041	rBV	469993	802282	21.91%	2.256%
10	9.975	1146	1154	1169	rBV	425856	721370	19.70%	2.029%
11	10.516	1238	1246	1269	rBV	595097	1070155	29.22%	3.010%
12	10.898	1303	1311	1321	rBV	623691	1018252	27.80%	2.864%
13	11.039	1327	1335	1354	rBV	555504	1057874	28.89%	2.975%
14	12.492	1574	1582	1592	rBV3	8168	19220	0.52%	0.054%
15	13.592	1764	1769	1775	rBV6	7924	12193	0.33%	0.034%
16	14.116	1852	1858	1873	rBV	1258181	1754996	47.92%	4.936%
17	14.410	1901	1908	1923	rBV	1277856	1920703	52.44%	5.402%
18	14.716	1952	1960	1969	rBV	987826	1499590	40.95%	4.218%
19	14.904	1985	1992	2009	rBV	461420	863661	23.58%	2.429%
20	15.127	2027	2030	2034	rVB6	3769	4253	0.12%	0.012%
21	15.704	2122	2128	2139	rBV	1729736	2512111	68.59%	7.066%
22	15.821	2142	2148	2160	rBV	597993	852486	23.28%	2.398%
23	15.945	2165	2169	2174	rVB6	9879	15715	0.43%	0.044%
24	16.492	2257	2262	2264	rBV5	2616	4450	0.12%	0.013%
25	17.139	2369	2372	2377	rBV7	3541	4722	0.13%	0.013%
26	17.251	2390	2391	2399	rVB7	3639	5734	0.16%	0.016%
27	17.468	2421	2428	2438	rBV	1368347	1948408	53.20%	5.480%
28	17.568	2438	2445	2463	rVV	2103061	2928699	79.97%	8.237%
29	19.368	2747	2751	2756	rVB2	26779	35840	0.98%	0.101%
30	19.433	2759	2762	2768	rVV2	23052	33288	0.91%	0.094%
31	19.786	2817	2822	2832	rBV	2697224	3662335	100.00%	10.301%
32	20.704	2975	2978	2982	rBV3	52249	59269	1.62%	0.167%
33	21.545	3116	3121	3130	rBV	1765497	2399355	65.51%	6.748%
34	23.915	3517	3524	3536	rVB2	1670432	3484193	95.14%	9.800%
35	24.080	3546	3552	3564	rVB	1061723	2185825	59.68%	6.148%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014041.D
Acq On : 10 Mar 2023 21:48
Operator : CG/JU
Sample : PB151260BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 35554333

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014041.D
Acq On : 10 Mar 2023 21:48
Operator : CG/JU
Sample : PB151260BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

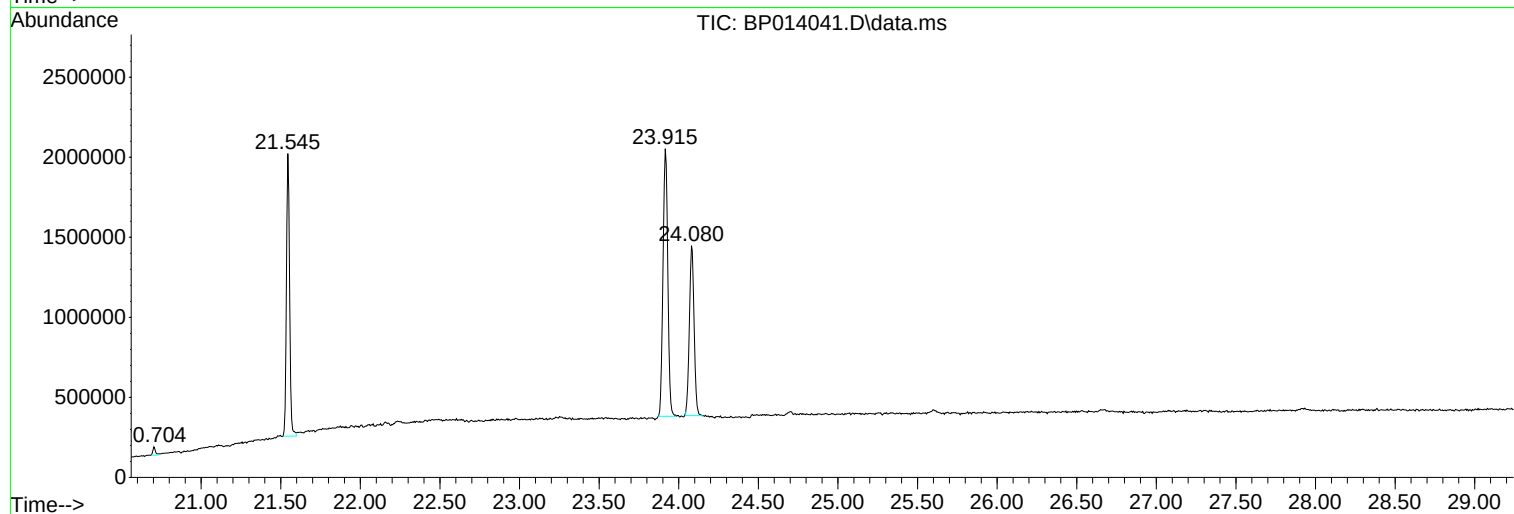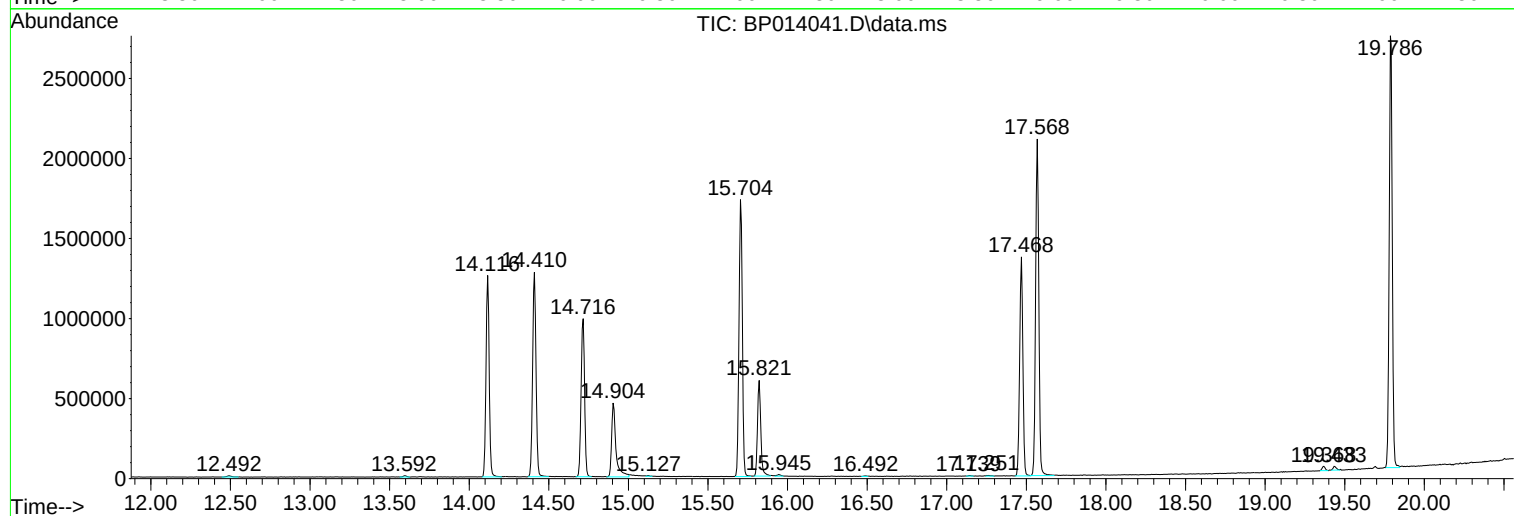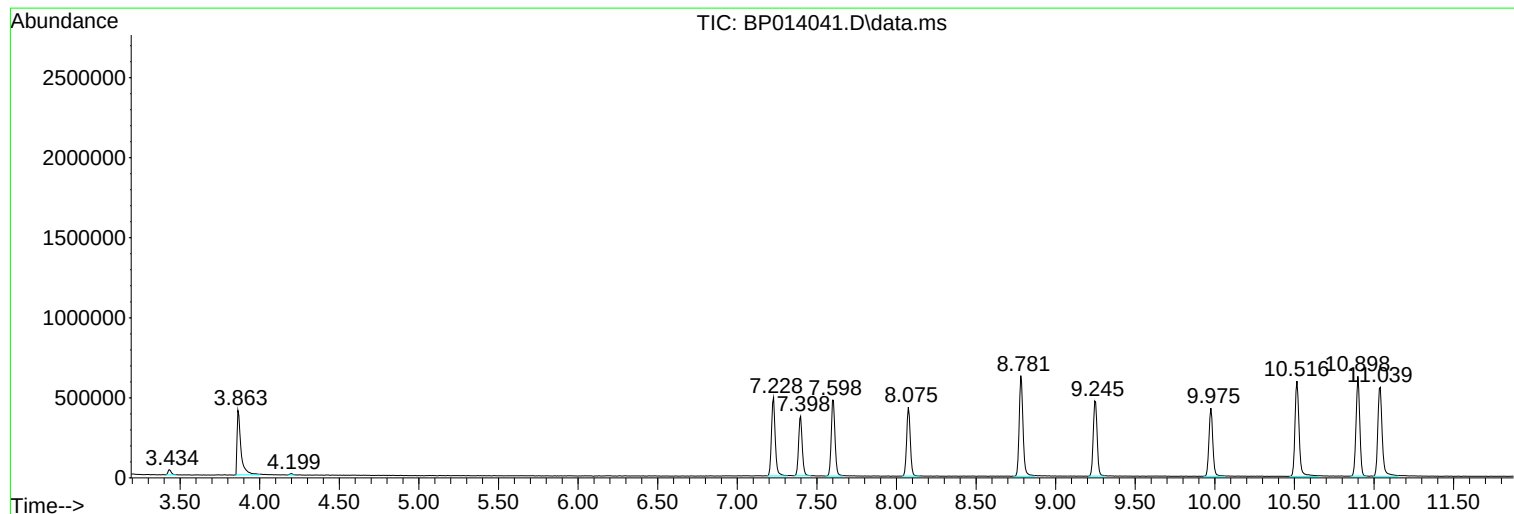

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014041.D
Acq On : 10 Mar 2023 21:48
Operator : CG/JU
Sample : PB151260BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014041.D
Acq On : 10 Mar 2023 21:48
Operator : CG/JU
Sample : PB151260BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------