

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014043.D
 Acq On : 10 Mar 2023 22:57
 Operator : CG/JU
 Sample : PB151297BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK297

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	53	rVB	39172	57815	1.25%	0.133%
2	3.864	112	115	139	rBV	483741	833075	17.98%	1.916%
3	4.199	168	172	177	rVB	8849	12355	0.27%	0.028%
4	7.228	680	687	701	rBV	581429	997511	21.53%	2.294%
5	7.393	709	715	725	rBV	447490	721766	15.58%	1.660%
6	7.599	743	750	763	rBV	596617	986830	21.30%	2.270%
7	8.075	823	831	840	rBV	474253	774551	16.72%	1.781%
8	8.781	944	951	967	rBV	750825	1255316	27.09%	2.887%
9	9.246	1021	1030	1044	rBV	602954	1000190	21.58%	2.300%
10	9.975	1144	1154	1167	rBV	529239	892754	19.27%	2.053%
11	10.516	1238	1246	1268	rBV	732900	1322074	28.53%	3.041%
12	10.899	1302	1311	1321	rVB	683075	1150143	24.82%	2.645%
13	11.034	1327	1334	1354	rBV	709378	1303813	28.14%	2.999%
14	12.487	1575	1581	1589	rBV2	11519	21010	0.45%	0.048%
15	14.116	1852	1858	1871	rBV	1650009	2212290	47.74%	5.088%
16	14.410	1898	1908	1920	rBV	1622116	2391823	51.62%	5.501%
17	14.710	1949	1959	1968	rBV	1121824	1718576	37.09%	3.952%
18	14.904	1986	1992	2014	rBV	630746	1120118	24.17%	2.576%
19	15.704	2121	2128	2137	rBV	2182827	3083231	66.54%	7.091%
20	15.822	2142	2148	2162	rVV	802709	1154282	24.91%	2.655%
21	15.945	2165	2169	2177	rVB6	10667	20239	0.44%	0.047%
22	17.257	2389	2392	2398	rVB7	3935	5671	0.12%	0.013%
23	17.469	2420	2428	2438	rBV	1586168	2265884	48.90%	5.211%
24	17.569	2438	2445	2457	rVV	2542967	3621616	78.16%	8.329%
25	19.369	2746	2751	2756	rBV2	39476	57809	1.25%	0.133%
26	19.433	2759	2762	2768	rVB2	30651	43835	0.95%	0.101%
27	19.786	2816	2822	2833	rBV	3425684	4578938	98.82%	10.531%
28	21.545	3116	3121	3129	rVB	1972500	2611706	56.36%	6.007%
29	23.916	3517	3524	3540	rVB	2310808	4633803	100.00%	10.657%
30	24.080	3546	3552	3566	rVB2	1266572	2632290	56.81%	6.054%




Sum of corrected areas: 43481314

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014043.D
Acq On : 10 Mar 2023 22:57
Operator : CG/JU
Sample : PB151297BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

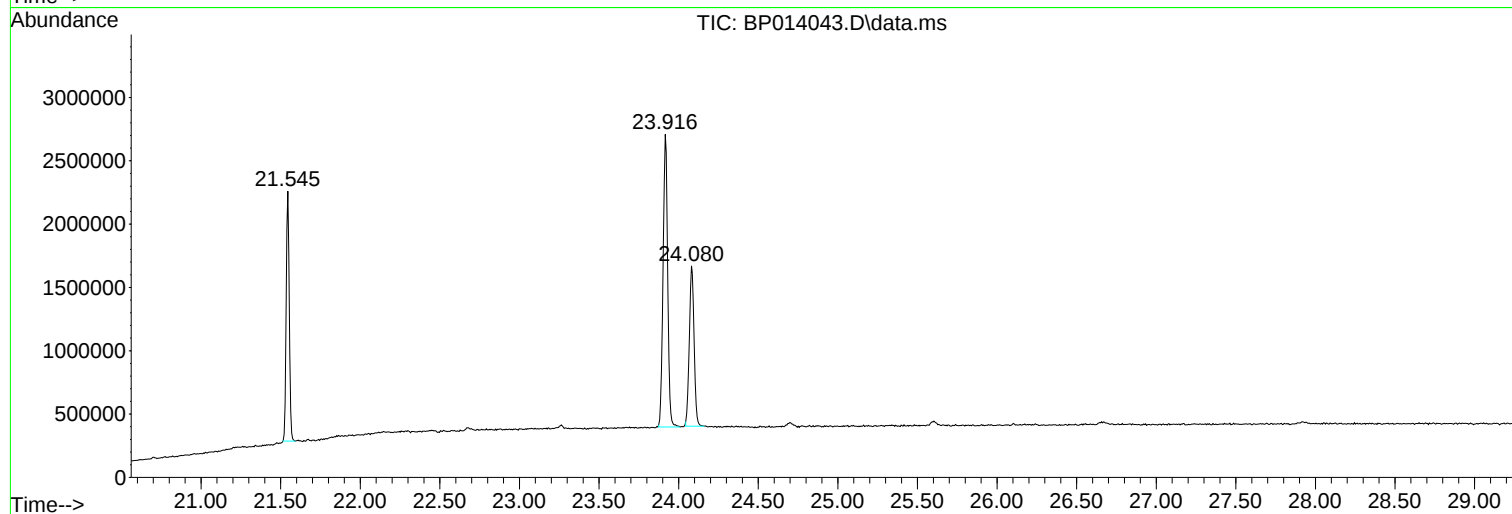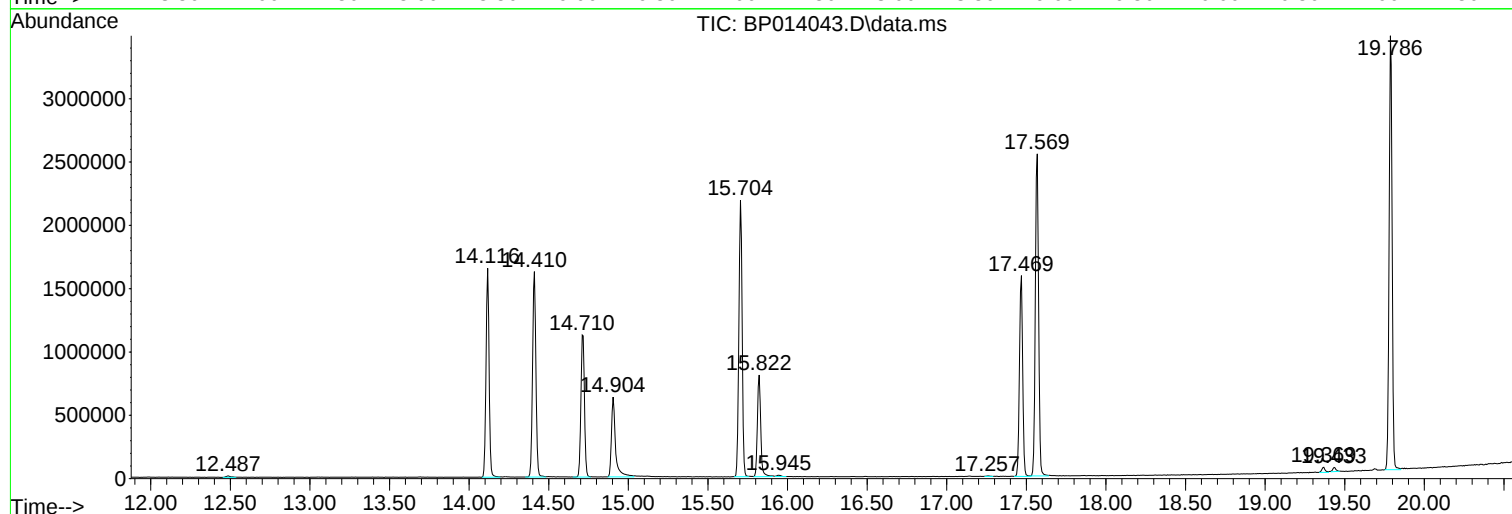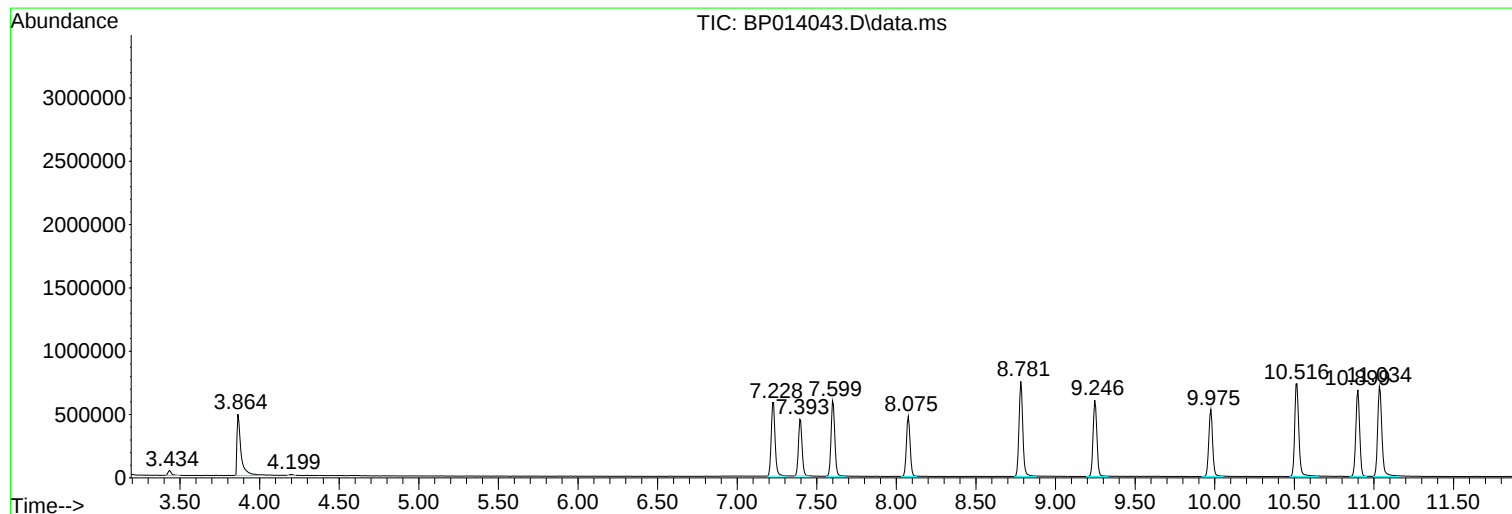

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014043.D
Acq On : 10 Mar 2023 22:57
Operator : CG/JU
Sample : PB151297BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014043.D
Acq On : 10 Mar 2023 22:57
Operator : CG/JU
Sample : PB151297BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc