

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014050.D
 Acq On : 11 Mar 2023 02:57
 Operator : CG/JU
 Sample : 01810-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	50	rVB	30466	44259	0.81%	0.093%
2	3.876	114	117	131	rBV	114342	210772	3.86%	0.444%
3	4.099	150	155	159	rVB	17119	25556	0.47%	0.054%
4	4.199	167	172	178	rVB	10779	18390	0.34%	0.039%
5	4.299	186	189	195	rVB5	8575	12376	0.23%	0.026%
6	5.134	327	331	337	rBV	8628	14439	0.26%	0.030%
7	6.446	549	554	561	rVB3	9887	18725	0.34%	0.039%
8	7.175	673	678	681	rBV7	3481	6453	0.12%	0.014%
9	7.228	681	687	700	rVV	118088	213845	3.92%	0.450%
10	7.393	708	715	732	rBV	546619	865299	15.86%	1.821%
11	7.599	742	750	761	rBV	505664	831415	15.24%	1.750%
12	8.075	821	831	848	rBV	551935	928681	17.03%	1.955%
13	8.781	942	951	964	rBV	399188	674717	12.37%	1.420%
14	9.246	1022	1030	1042	rBV	726015	1205339	22.10%	2.537%
15	9.352	1044	1048	1056	rBV3	12667	24833	0.46%	0.052%
16	9.634	1090	1096	1104	rVB	15517	25652	0.47%	0.054%
17	9.975	1146	1154	1163	rBV	576461	986266	18.08%	2.076%
18	10.510	1238	1245	1260	rBV	777190	1357445	24.89%	2.857%
19	10.899	1300	1311	1319	rBV	805595	1371619	25.15%	2.887%
20	11.034	1325	1334	1351	rBV	687710	1239008	22.72%	2.608%
21	11.752	1446	1456	1457	rBV9	2778	6075	0.11%	0.013%
22	12.128	1512	1520	1527	rBV2	9615	15007	0.28%	0.032%
23	12.481	1575	1580	1586	rVB3	11837	20734	0.38%	0.044%
24	12.610	1598	1602	1606	rVB7	3526	5997	0.11%	0.013%
25	13.351	1722	1728	1733	rVB8	3168	6249	0.11%	0.013%
26	13.516	1750	1756	1762	rBV5	6899	12525	0.23%	0.026%
27	14.116	1850	1858	1871	rBV	1805604	2505264	45.93%	5.274%
28	14.410	1900	1908	1917	rBV	1836918	2797754	51.29%	5.889%
29	14.593	1934	1939	1942	rVB6	4918	6879	0.13%	0.014%
30	14.710	1952	1959	1969	rBV	1337503	2028613	37.19%	4.270%
31	14.916	1989	1994	2007	rBV	69505	171011	3.14%	0.360%
32	15.128	2026	2030	2035	rVB7	5524	8852	0.16%	0.019%
33	15.534	2095	2099	2103	rBV6	4631	7645	0.14%	0.016%
34	15.657	2116	2120	2122	rBV5	4055	6026	0.11%	0.013%
35	15.704	2122	2128	2141	rVV	2591154	3717260	68.15%	7.825%
36	15.822	2141	2148	2163	rVV	935837	1326317	24.32%	2.792%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014050.D
 Acq On : 11 Mar 2023 02:57
 Operator : CG/JU
 Sample : 01810-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCAF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	15.945	2165	2169	2174	rVB3	12855	21415	0.39%	0.045%
38	16.069	2184	2190	2199	rVB	137043	195938	3.59%	0.412%
39	16.410	2242	2248	2250	rBV7	5066	9958	0.18%	0.021%
40	16.640	2282	2287	2293	rVB7	8609	14434	0.26%	0.030%
41	17.140	2367	2372	2378	rBV9	4546	8676	0.16%	0.018%
42	17.469	2421	2428	2436	rBV	1814470	2640764	48.42%	5.559%
43	17.569	2438	2445	2456	rVV	3102143	4377428	80.25%	9.214%
44	17.651	2456	2459	2466	rVB9	12993	21946	0.40%	0.046%
45	18.116	2533	2538	2542	rBV7	8724	12991	0.24%	0.027%
46	18.322	2569	2573	2581	rBV	98244	144963	2.66%	0.305%
47	18.728	2639	2642	2646	rVB6	11906	13568	0.25%	0.029%
48	19.363	2746	2750	2757	rBV3	45359	64927	1.19%	0.137%
49	19.434	2758	2762	2771	rVV	45284	78036	1.43%	0.164%
50	19.551	2779	2782	2794	rBV7	30696	59683	1.09%	0.126%
51	19.686	2803	2805	2809	rVB5	15766	17539	0.32%	0.037%
52	19.786	2816	2822	2830	rBV	4144951	5454426	100.00%	11.481%
53	21.216	3060	3065	3080	rBV2	329543	599127	10.98%	1.261%
54	21.545	3116	3121	3127	rBV	2129883	2864158	52.51%	6.029%
55	23.916	3516	3524	3539	rVB	2594823	5281549	96.83%	11.118%
56	24.080	3545	3552	3562	rVB2	1374781	2907779	53.31%	6.121%




Sum of corrected areas: 47506602

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014050.D
Acq On : 11 Mar 2023 02:57
Operator : CG/JU
Sample : 01810-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

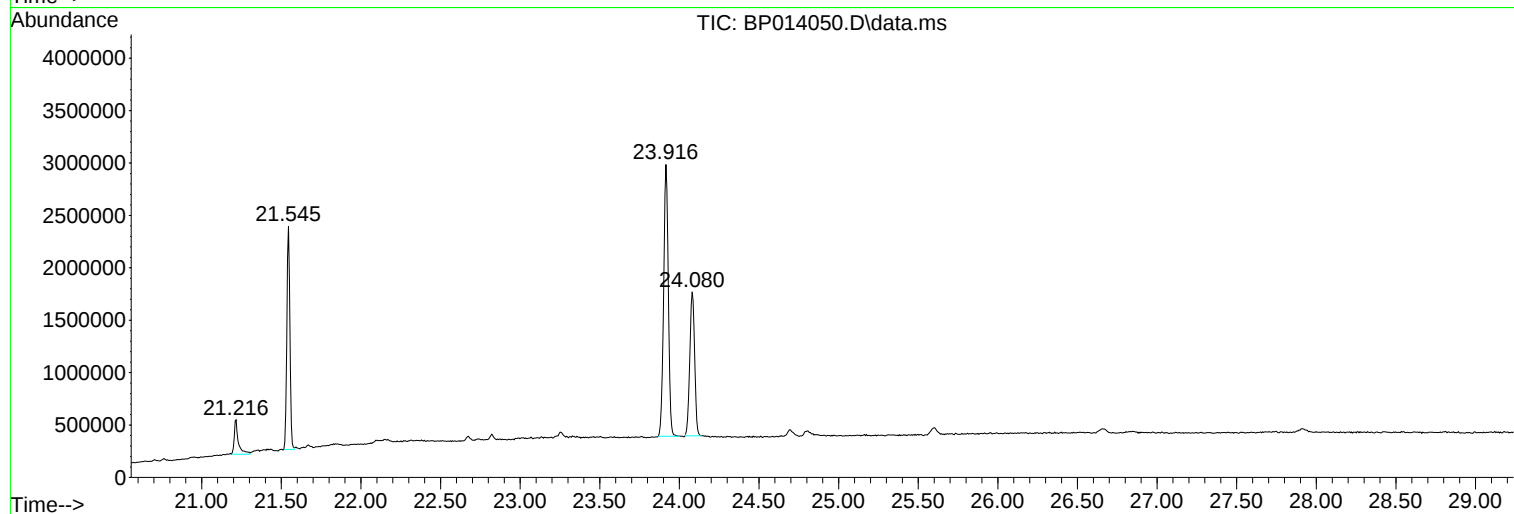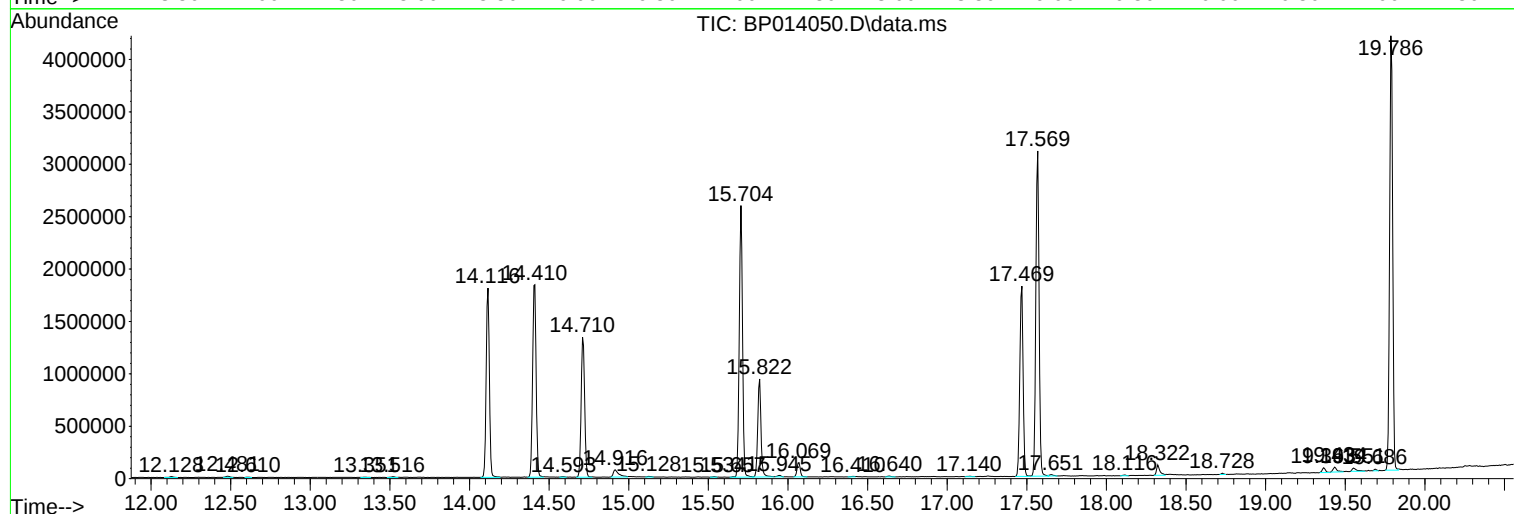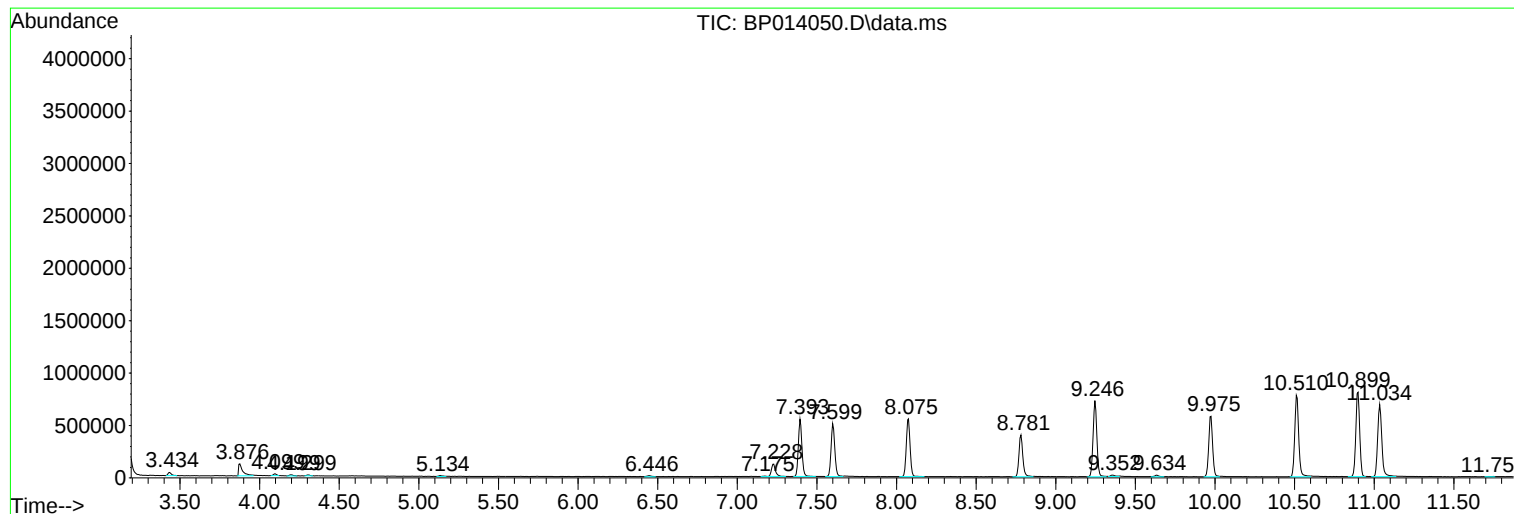

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014050.D
Acq On : 11 Mar 2023 02:57
Operator : CG/JU
Sample : 01810-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAF7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.216	4.18 ng/ul	599127	Chrysene-d12	21.545

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentacos-1-ene	350	C25H50	016980-85-1	94
2			1-Heneicosyl formate	340	C22H44O2	077899-03-7	94
3			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	94
4			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
5			n-Nonadecanol-1	284	C19H40O	001454-84-8	94

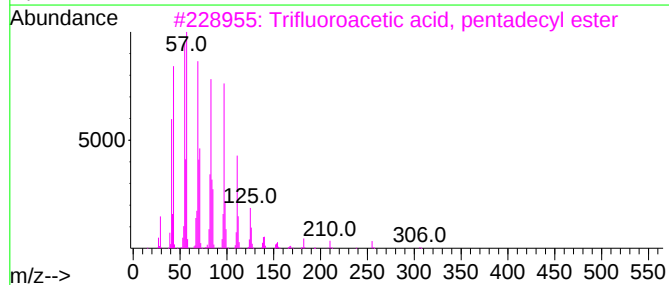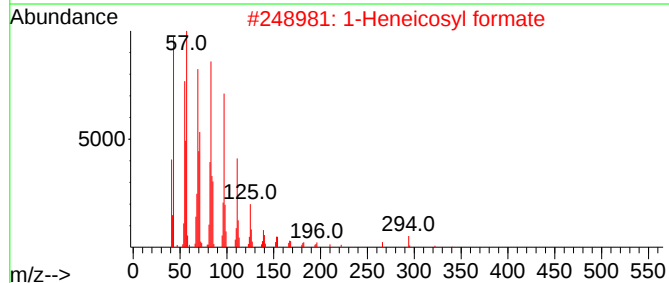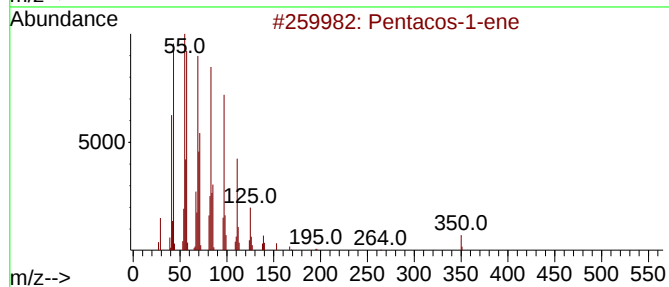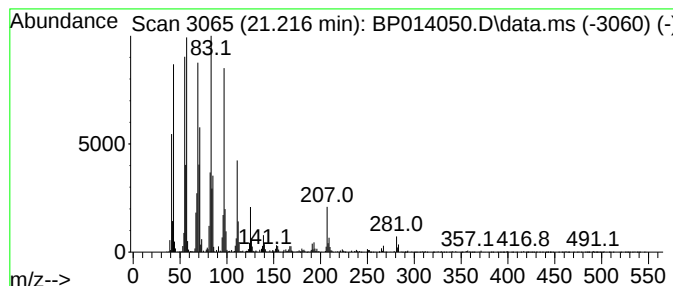

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014050.D
Acq On : 11 Mar 2023 02:57
Operator : CG/JU
Sample : 01810-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCAF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.216	4.2	ng/u1	599127	5	21.545	2864160	20.0