

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014054.D
 Acq On : 11 Mar 2023 05:14
 Operator : CG/JU
 Sample : 01804-12
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	49	rVB	32505	44674	0.87%	0.101%
2	3.875	114	117	133	rBV	115259	217105	4.24%	0.492%
3	4.093	149	154	160	rBV2	16385	26487	0.52%	0.060%
4	4.199	167	172	181	rVB	48862	77678	1.52%	0.176%
5	4.305	186	190	195	rVB5	8461	11700	0.23%	0.027%
6	5.134	327	331	340	rBV	9342	15146	0.30%	0.034%
7	6.446	549	554	559	rBV2	7547	12825	0.25%	0.029%
8	7.222	681	686	697	rBV	122091	216040	4.22%	0.490%
9	7.393	708	715	731	rBV	488336	776042	15.15%	1.760%
10	7.599	743	750	760	rBV	483847	778496	15.19%	1.765%
11	8.069	823	830	839	rBV	550741	908498	17.73%	2.060%
12	8.781	941	951	968	rBV	381191	658315	12.85%	1.493%
13	9.246	1022	1030	1044	rBV	626672	1047450	20.44%	2.375%
14	9.358	1044	1049	1055	rBV2	16024	30565	0.60%	0.069%
15	9.634	1091	1096	1101	rBV2	12286	19387	0.38%	0.044%
16	9.969	1146	1153	1168	rBV	509923	885718	17.29%	2.008%
17	10.510	1238	1245	1261	rBV	705919	1246960	24.34%	2.827%
18	10.893	1301	1310	1323	rVB	774165	1352142	26.39%	3.066%
19	11.034	1326	1334	1352	rBV	567041	1066224	20.81%	2.417%
20	12.134	1515	1521	1527	rBV4	6582	10842	0.21%	0.025%
21	12.481	1574	1580	1586	rBV3	9992	18896	0.37%	0.043%
22	12.604	1595	1601	1609	rVB3	2327	5644	0.11%	0.013%
23	13.334	1721	1725	1730	rBV3	7067	11791	0.23%	0.027%
24	13.522	1751	1757	1760	rBV5	4992	8286	0.16%	0.019%
25	13.593	1763	1769	1774	rVB3	9172	16806	0.33%	0.038%
26	14.116	1849	1858	1871	rBV	1633857	2255791	44.03%	5.115%
27	14.228	1871	1877	1884	rVB	3433	8136	0.16%	0.018%
28	14.404	1900	1907	1920	rBV	1622239	2484405	48.49%	5.633%
29	14.710	1952	1959	1967	rBV	1375408	1995284	38.94%	4.524%
30	14.910	1987	1993	2016	rBV	76854	219323	4.28%	0.497%
31	15.128	2025	2030	2036	rBV10	5617	12071	0.24%	0.027%
32	15.704	2121	2128	2136	rBV	2423527	3357454	65.53%	7.612%
33	15.822	2142	2148	2164	rBV	922110	1294238	25.26%	2.934%
34	15.945	2164	2169	2174	rVB4	13194	20855	0.41%	0.047%
35	16.069	2184	2190	2195	rBV	85255	116541	2.27%	0.264%
36	17.145	2368	2373	2376	rBV6	4843	9288	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014054.D
 Acq On : 11 Mar 2023 05:14
 Operator : CG/JU
 Sample : 01804-12
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	17.251	2389	2391	2397	rVB5	4228	6701	0.13%	0.015%
38	17.463	2420	2427	2436	rBV	1747600	2598452	50.72%	5.891%
39	17.569	2438	2445	2454	rVV	2778876	4123796	80.49%	9.350%
40	17.639	2455	2457	2465	rVB8	11806	21481	0.42%	0.049%
41	18.116	2533	2538	2541	rBV7	6537	9819	0.19%	0.022%
42	18.322	2569	2573	2584	rBV2	89273	144571	2.82%	0.328%
43	19.363	2746	2750	2756	rBV3	42237	62236	1.21%	0.141%
44	19.433	2758	2762	2769	rVB	42647	67890	1.33%	0.154%
45	19.551	2779	2782	2788	rBV6	30737	47971	0.94%	0.109%
46	19.686	2803	2805	2810	rVB5	15783	14837	0.29%	0.034%
47	19.786	2816	2822	2833	rBV	3847192	5123488	100.00%	11.617%
48	21.216	3061	3065	3073	rBV2	145406	248692	4.85%	0.564%
49	21.545	3115	3121	3131	rBV	2199427	3045035	59.43%	6.904%
50	23.916	3517	3524	3536	rVB	2349918	4701239	91.76%	10.659%
51	24.080	3545	3552	3561	rVB	1325540	2651844	51.76%	6.013%




Sum of corrected areas: 44105155

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014054.D
Acq On : 11 Mar 2023 05:14
Operator : CG/JU
Sample : 01804-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

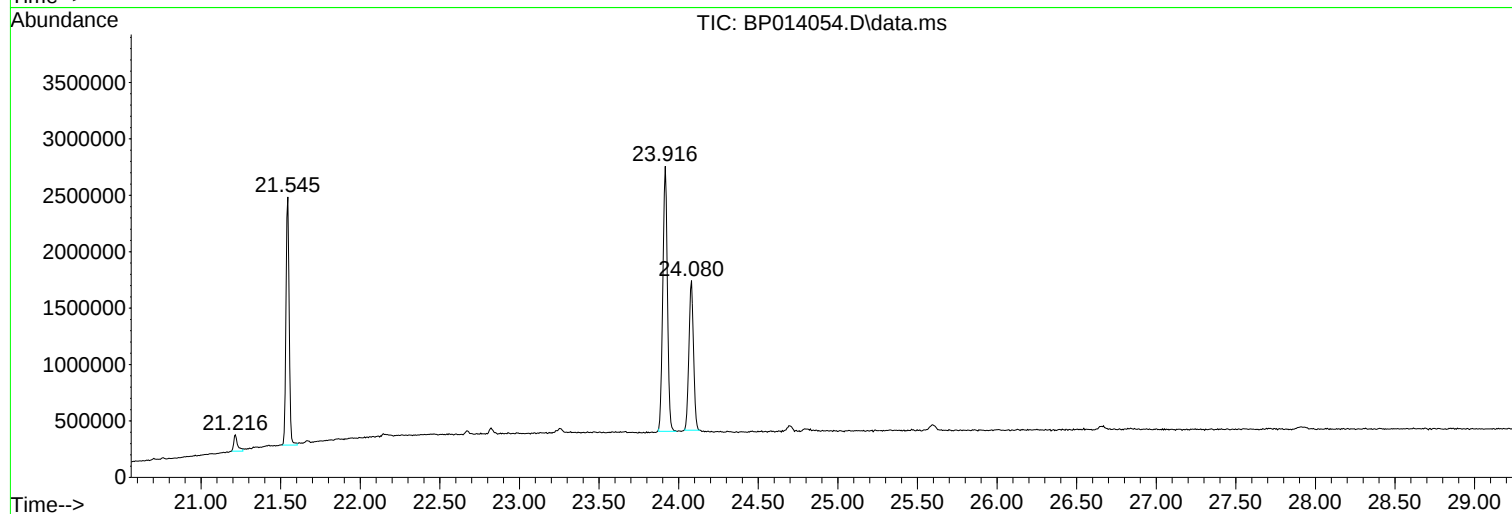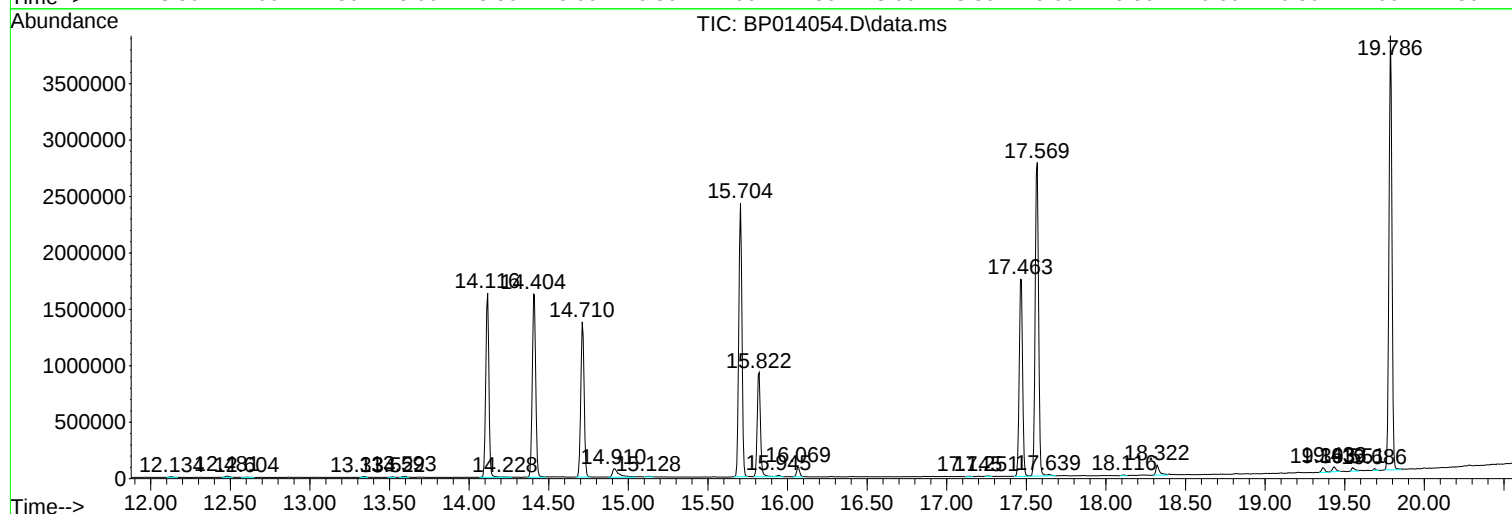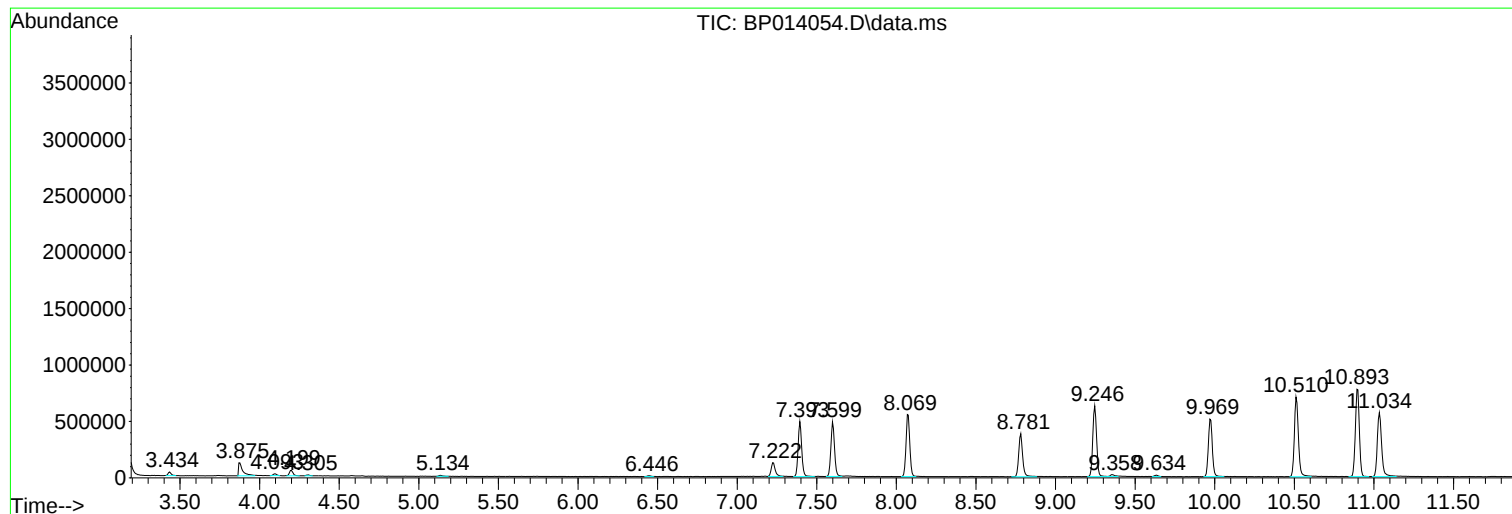

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014054.D
Acq On : 11 Mar 2023 05:14
Operator : CG/JU
Sample : 01804-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014054.D
Acq On : 11 Mar 2023 05:14
Operator : CG/JU
Sample : 01804-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc