

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
 Data File : BP014057.D
 Acq On : 11 Mar 2023 07:30
 Operator : CG/JU
 Sample : PB151314BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK314

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	50	rBV	47567	67903	1.28%	0.133%
2	3.864	112	115	142	rBV	609382	990226	18.65%	1.944%
3	4.193	168	171	179	rVB3	10204	16926	0.32%	0.033%
4	7.222	679	686	703	rBV	766872	1236490	23.28%	2.428%
5	7.393	709	715	727	rBV	574683	891459	16.79%	1.750%
6	7.599	742	750	763	rBV	758266	1229292	23.15%	2.414%
7	8.069	823	830	841	rBV	573631	949933	17.89%	1.865%
8	8.781	943	951	966	rBV	896880	1504780	28.34%	2.955%
9	9.246	1021	1030	1045	rBV	743338	1240192	23.35%	2.435%
10	9.969	1146	1153	1169	rBV	646479	1112381	20.95%	2.184%
11	10.510	1237	1245	1260	rBV	918413	1599666	30.12%	3.141%
12	10.893	1301	1310	1324	rBV	798514	1377187	25.93%	2.704%
13	11.034	1326	1334	1353	rBV	838188	1514449	28.52%	2.974%
14	12.481	1575	1580	1590	rBV2	12604	25757	0.49%	0.051%
15	13.598	1760	1770	1775	rBV7	4993	10276	0.19%	0.020%
16	14.116	1850	1858	1868	rBV	1797208	2564553	48.29%	5.036%
17	14.404	1900	1907	1923	rBV	1895889	2857517	53.81%	5.611%
18	14.710	1952	1959	1970	rVB	1379660	2027255	38.18%	3.981%
19	14.904	1985	1992	2009	rBV	734431	1274284	24.00%	2.502%
20	15.704	2121	2128	2141	rBV	2499442	3625653	68.28%	7.119%
21	15.822	2141	2148	2159	rBV	955058	1342808	25.29%	2.637%
22	15.945	2165	2169	2175	rVB3	14927	23406	0.44%	0.046%
23	17.145	2368	2373	2379	rBV8	4233	7663	0.14%	0.015%
24	17.251	2388	2391	2394	rBV5	4505	5388	0.10%	0.011%
25	17.469	2421	2428	2437	rBV	1868646	2753534	51.85%	5.407%
26	17.563	2438	2444	2455	rBV	2874684	4269488	80.40%	8.383%
27	19.363	2746	2750	2756	rBV3	40753	60358	1.14%	0.119%
28	19.433	2758	2762	2770	rVB	43075	60670	1.14%	0.119%
29	19.686	2803	2805	2812	rVB7	13356	14436	0.27%	0.028%
30	19.786	2816	2822	2832	rBV	4149364	5310358	100.00%	10.427%
31	21.545	3116	3121	3129	rBV	2315175	3161762	59.54%	6.208%
32	23.916	3517	3524	3540	rVB2	2402376	4908495	92.43%	9.638%
33	24.080	3545	3552	3563	rVB2	1358830	2893760	54.49%	5.682%




Sum of corrected areas: 50928305

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014057.D
Acq On : 11 Mar 2023 07:30
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

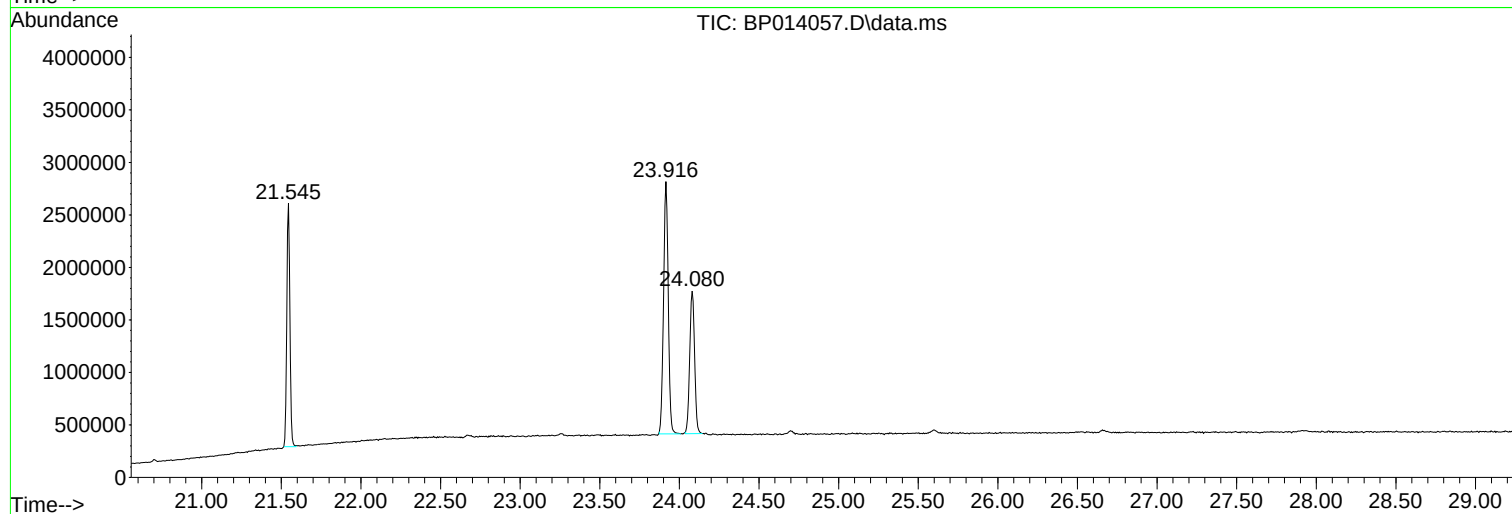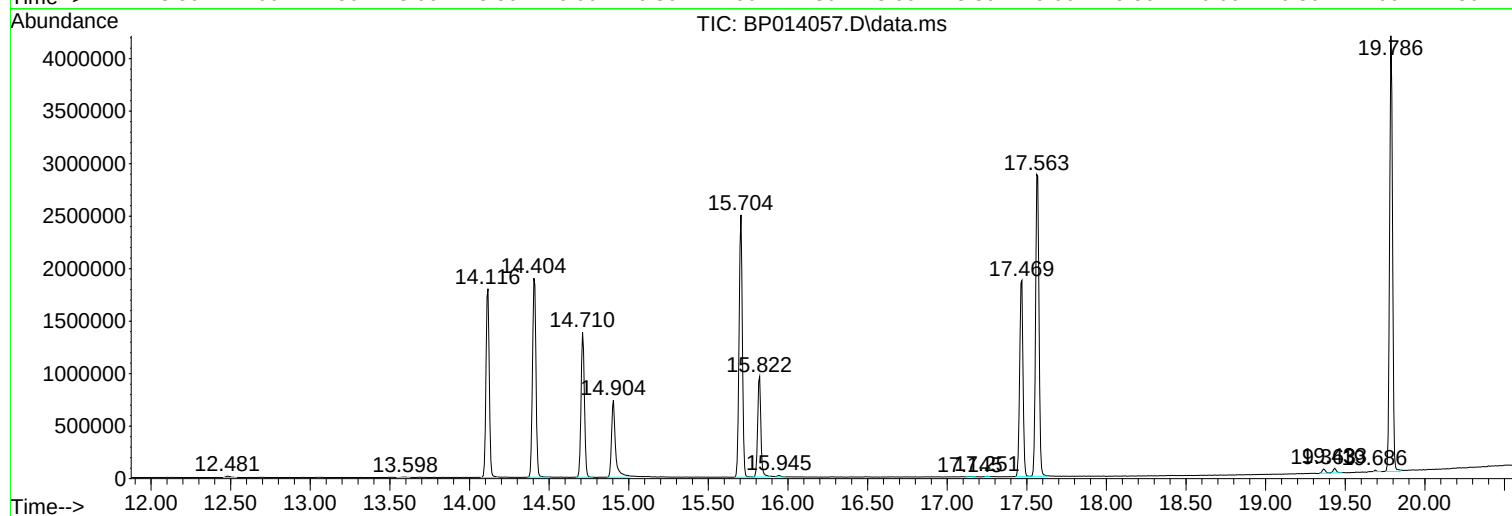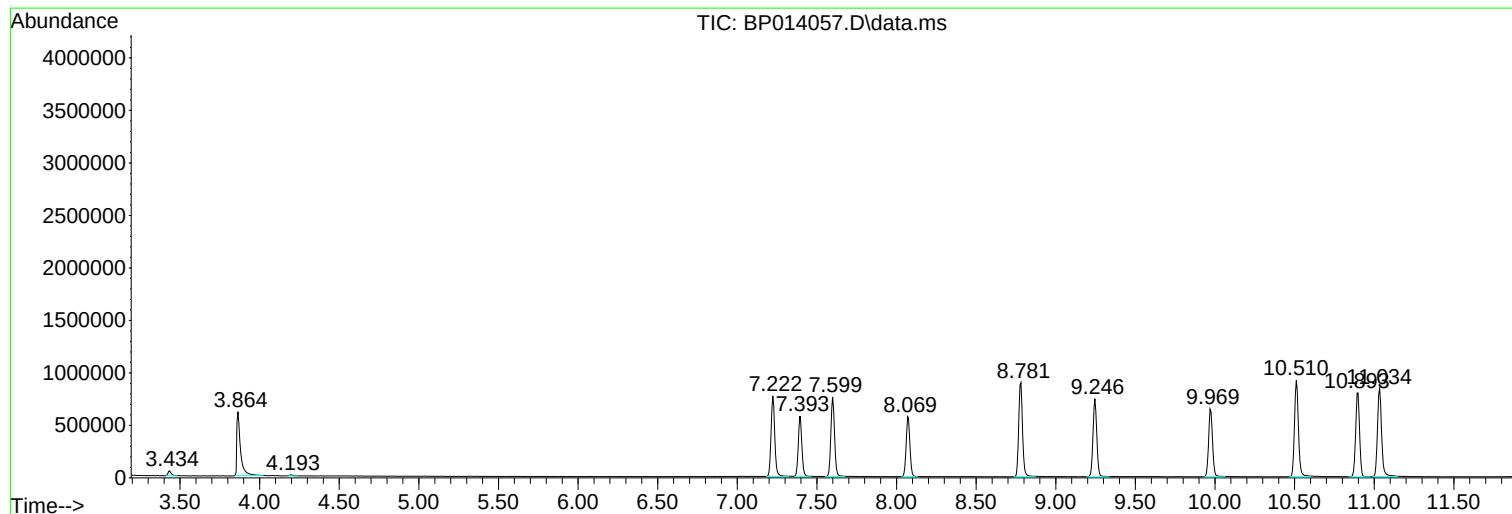

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014057.D
Acq On : 11 Mar 2023 07:30
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031023\
Data File : BP014057.D
Acq On : 11 Mar 2023 07:30
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------