

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031121\
 Data File : BP004969.D
 Acq On : 11 Mar 2021 12:18
 Operator : CG/JU
 Sample : PB134982BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP030821.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	7	9	14	rVB6	1544	1649	0.15%	0.016%
2	3.228	21	24	29	rBV	10367	14016	1.24%	0.133%
3	3.552	76	79	80	rBV3	1717	1703	0.15%	0.016%
4	3.640	92	94	118	rVV	105482	187439	16.60%	1.781%
5	3.946	144	146	150	rBV5	2022	3020	0.27%	0.029%
6	4.299	204	206	213	rVB5	1306	2018	0.18%	0.019%
7	5.575	421	423	427	rVV4	793	1213	0.11%	0.012%
8	5.622	428	431	435	rVB4	1050	1513	0.13%	0.014%
9	5.887	474	476	481	rVB6	1094	1808	0.16%	0.017%
10	6.252	536	538	540	rBV3	1316	1339	0.12%	0.013%
11	6.305	543	547	548	rBV3	1192	1303	0.12%	0.012%
12	6.481	574	577	582	rVB7	880	1704	0.15%	0.016%
13	6.905	642	649	660	rBV	170237	264988	23.46%	2.518%
14	7.069	671	677	687	rBV	114736	183786	16.27%	1.746%
15	7.263	704	710	718	rBV	169480	275192	24.36%	2.615%
16	7.469	743	745	748	rBV4	931	1356	0.12%	0.013%
17	7.734	783	790	797	rBV	121044	188394	16.68%	1.790%
18	8.169	859	864	869	rVB8	905	1626	0.14%	0.015%
19	8.440	901	910	920	rBV	205475	332249	29.42%	3.157%
20	8.893	978	987	997	rVV	164715	276965	24.52%	2.631%
21	8.975	999	1001	1004	rVB4	947	1201	0.11%	0.011%
22	9.610	1101	1109	1118	rBV	147740	242622	21.48%	2.305%
23	9.675	1118	1120	1125	rVB5	1047	1403	0.12%	0.013%
24	10.146	1193	1200	1213	rBV	206257	347247	30.74%	3.299%
25	10.522	1257	1264	1272	rBV	157810	266107	23.56%	2.528%
26	10.663	1280	1288	1300	rBV	186960	342237	30.30%	3.252%
27	12.134	1530	1538	1545	rVB7	2460	5641	0.50%	0.054%
28	13.798	1814	1821	1830	rBV	402962	567765	50.27%	5.394%
29	14.075	1861	1868	1880	rBV	438632	618539	54.76%	5.877%
30	14.163	1881	1883	1888	rVB6	870	1176	0.10%	0.011%
31	14.387	1913	1921	1932	rBV	252076	374058	33.12%	3.554%
32	14.592	1949	1956	1968	rBV	165129	272959	24.17%	2.593%
33	15.381	2084	2090	2099	rBV	538068	766520	67.87%	7.283%
34	15.504	2103	2111	2125	rVV	211508	295831	26.19%	2.811%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031121\
 Data File : BP004969.D
 Acq On : 11 Mar 2021 12:18
 Operator : CG/JU
 Sample : PB134982BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP030821.M
 Title : SVOA CALIBRATION

35	15.628	2127	2132	2136	rVB2	6590	9641	0.85%	0.092%
36	15.816	2160	2164	2167	rBV6	758	1230	0.11%	0.012%
37	16.169	2219	2224	2229	rVB8	2130	3477	0.31%	0.033%
38	16.539	2285	2287	2292	rVB5	863	1165	0.10%	0.011%
39	16.922	2350	2352	2354	rBV2	1150	1154	0.10%	0.011%
40	17.139	2382	2389	2396	rBV	330290	452155	40.03%	4.296%
41	17.239	2400	2406	2421	rBV	628609	895859	79.32%	8.511%
42	17.816	2500	2504	2506	rBV5	857	1370	0.12%	0.013%
43	18.345	2592	2594	2596	rBV3	1199	1240	0.11%	0.012%
44	18.433	2607	2609	2612	rBV3	1249	1327	0.12%	0.013%
45	18.586	2633	2635	2638	rBV3	1413	1503	0.13%	0.014%
46	19.051	2712	2714	2716	rBV3	1299	1396	0.12%	0.013%
47	19.128	2723	2727	2731	rBV2	6214	7419	0.66%	0.070%
48	19.375	2765	2769	2774	rBV3	6336	9350	0.83%	0.089%
49	19.480	2781	2787	2797	rBV	820065	1095279	96.97%	10.406%
50	19.669	2817	2819	2821	rBV3	2917	2559	0.23%	0.024%
51	21.227	3079	3084	3090	rBV	442284	541996	47.99%	5.149%
52	23.374	3442	3449	3461	rVB	619340	1129459	100.00%	10.731%
53	23.516	3467	3473	3482	rVB2	269426	521187	46.14%	4.952%


Sum of corrected areas: 10525353

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031121\
Data File : BP004969.D
Acq On : 11 Mar 2021 12:18
Operator : CG/JU
Sample : PB134982BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP030821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

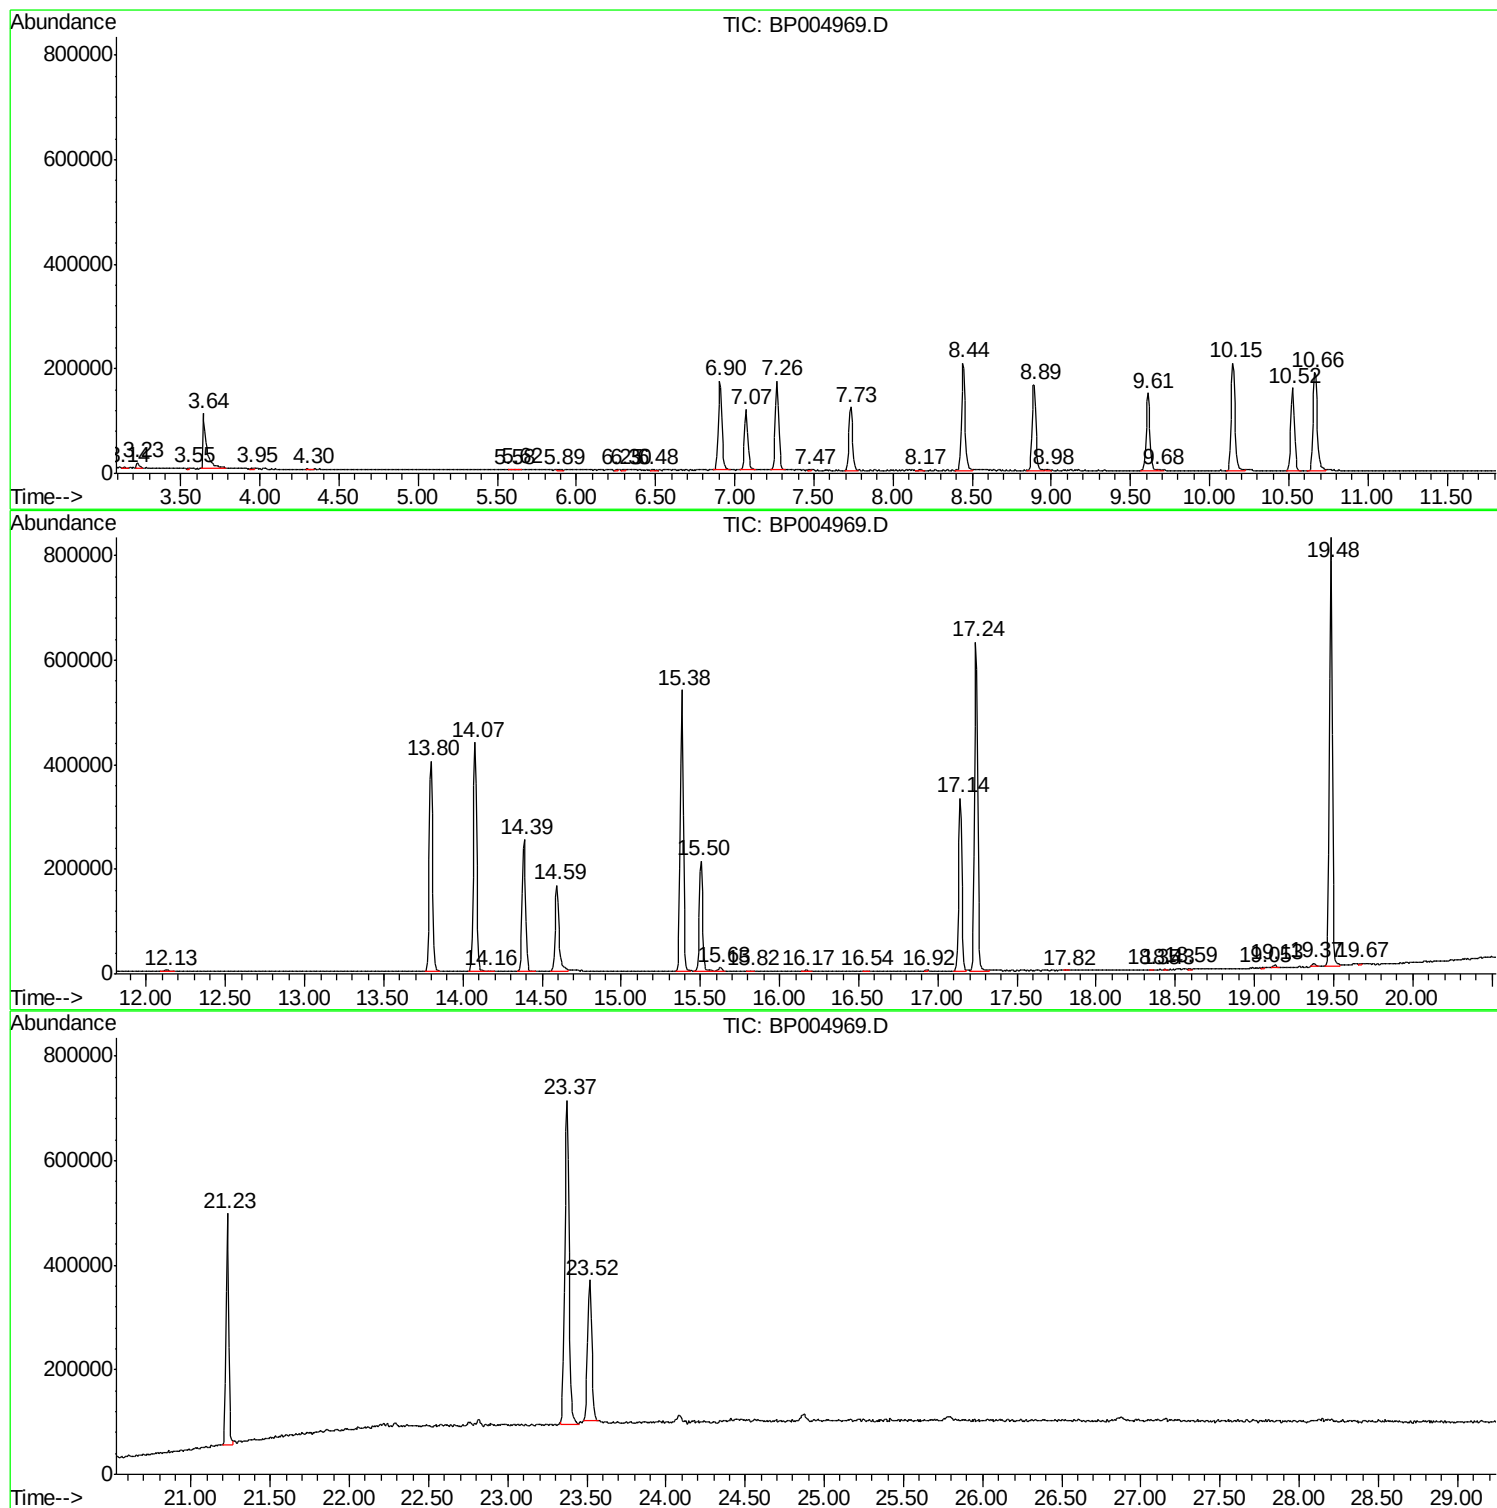

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031121\
Data File : BP004969.D
Acq On : 11 Mar 2021 12:18
Operator : CG/JU
Sample : PB134982BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP030821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031121\
Data File : BP004969.D
Acq On : 11 Mar 2021 12:18
Operator : CG/JU
Sample : PB134982BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK982

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP030821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc