
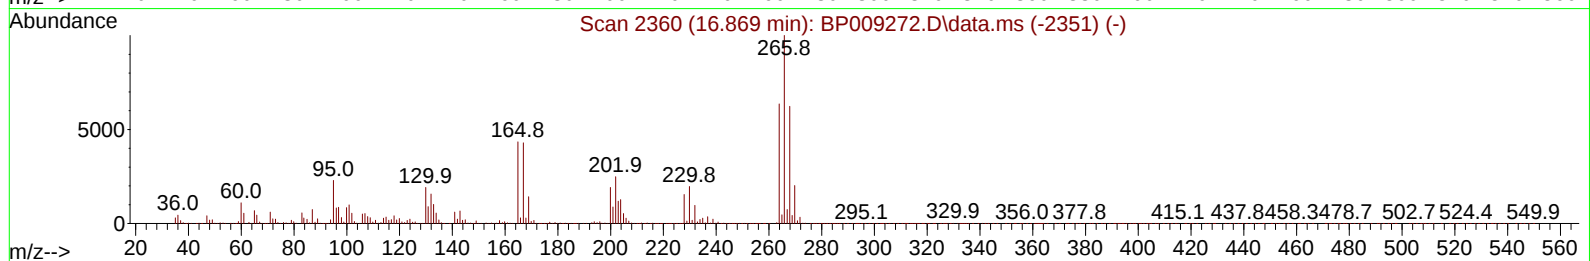
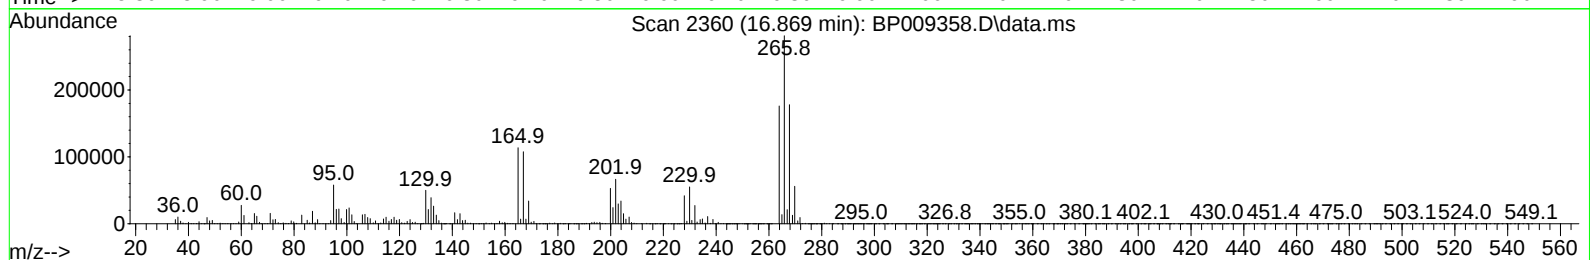


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009358.D
Acq On : 11 Mar 2022 10:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 06:04:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

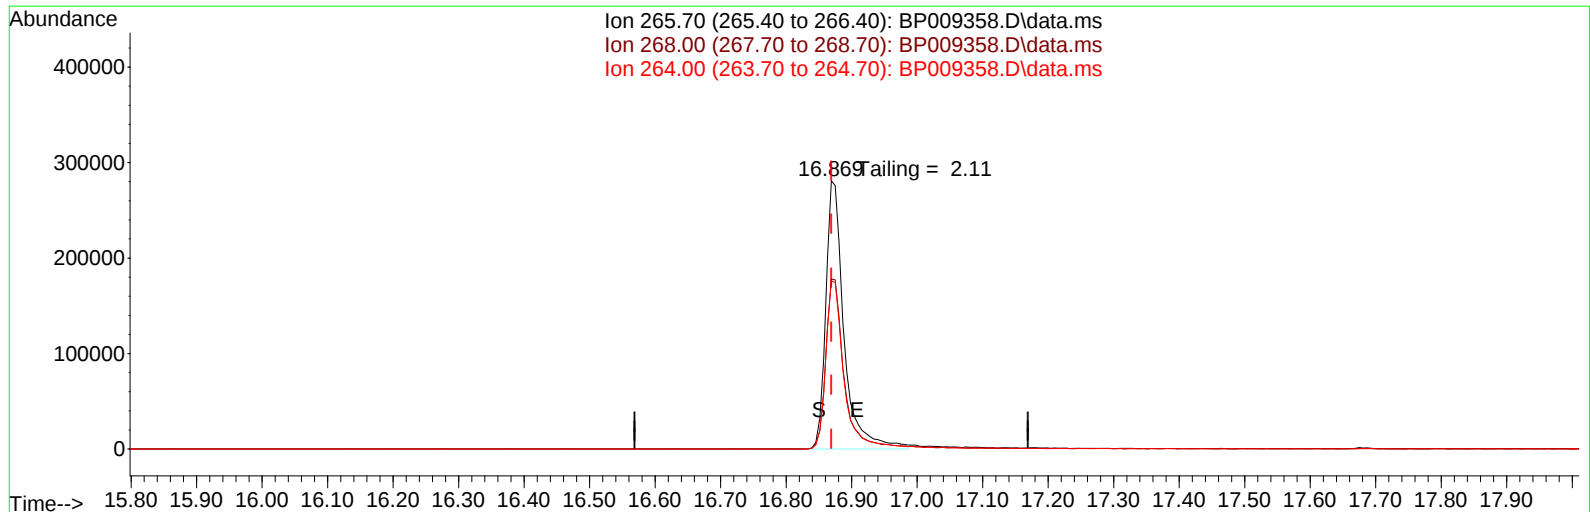

TIC: BP009358.D\data.ms

(70) Pentachlorophenol (C)




16.869min (+ 0.000) 552178.20 ng

response 550937

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.32
264.00	63.60	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
 Data File : BP009358.D
 Acq On : 11 Mar 2022 10:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 06:04:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

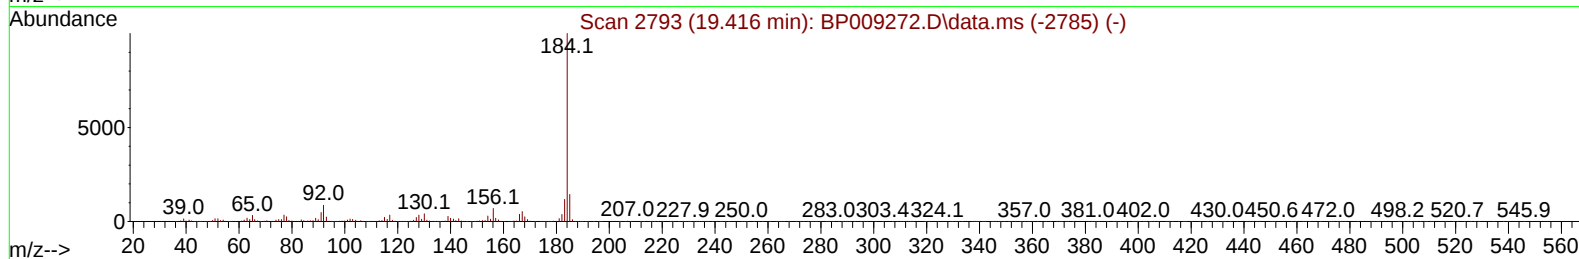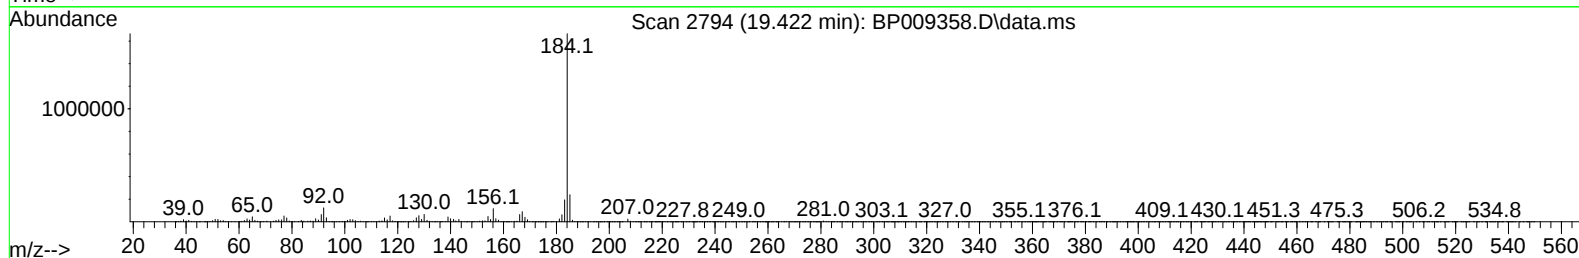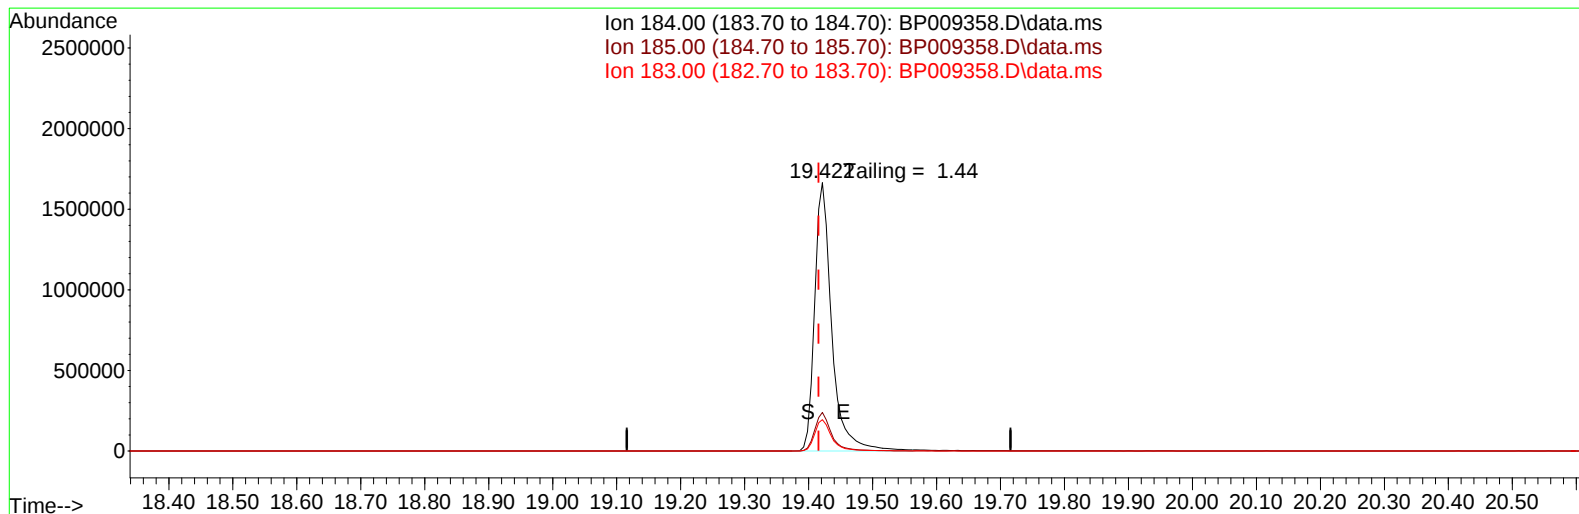

TIC: BP009358.D\data.ms

(77) Benzidine**19.422min (+ 0.006) 640828.06 ng****response 3109067**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	11.70	11.67
0.00	0.00	0.00