

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
 Data File : BP009360.D
 Acq On : 11 Mar 2022 12:10
 Operator : CG/JU
 Sample : PB143234BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143234BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	406	413	427	rBV	6041782	9870400	48.87%	10.497%
2	6.998	674	682	703	rBV	5586691	9745012	48.25%	10.364%
3	7.822	814	822	831	rBV	1153387	1944375	9.63%	2.068%
4	8.975	1009	1018	1039	rBV	3657326	6534920	32.35%	6.950%
5	10.616	1288	1297	1310	rBV	1445812	2657710	13.16%	2.826%
6	13.086	1708	1717	1741	rBV	9025728	15795668	78.20%	16.798%
7	14.463	1944	1951	1976	rBV	1882724	3504769	17.35%	3.727%
8	15.957	2197	2205	2242	rBV	6021848	11778408	58.31%	12.526%
9	17.221	2413	2420	2436	rBV	2428389	4094997	20.27%	4.355%
10	19.798	2852	2858	2879	rBV	14948010	20198346	100.00%	21.480%
11	21.339	3114	3120	3131	rBV	2411276	3981616	19.71%	4.234%
12	23.751	3524	3530	3555	rVB2	1380632	3925360	19.43%	4.175%


Sum of corrected areas: 94031581

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009360.D
Acq On : 11 Mar 2022 12:10
Operator : CG/JU
Sample : PB143234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143234BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

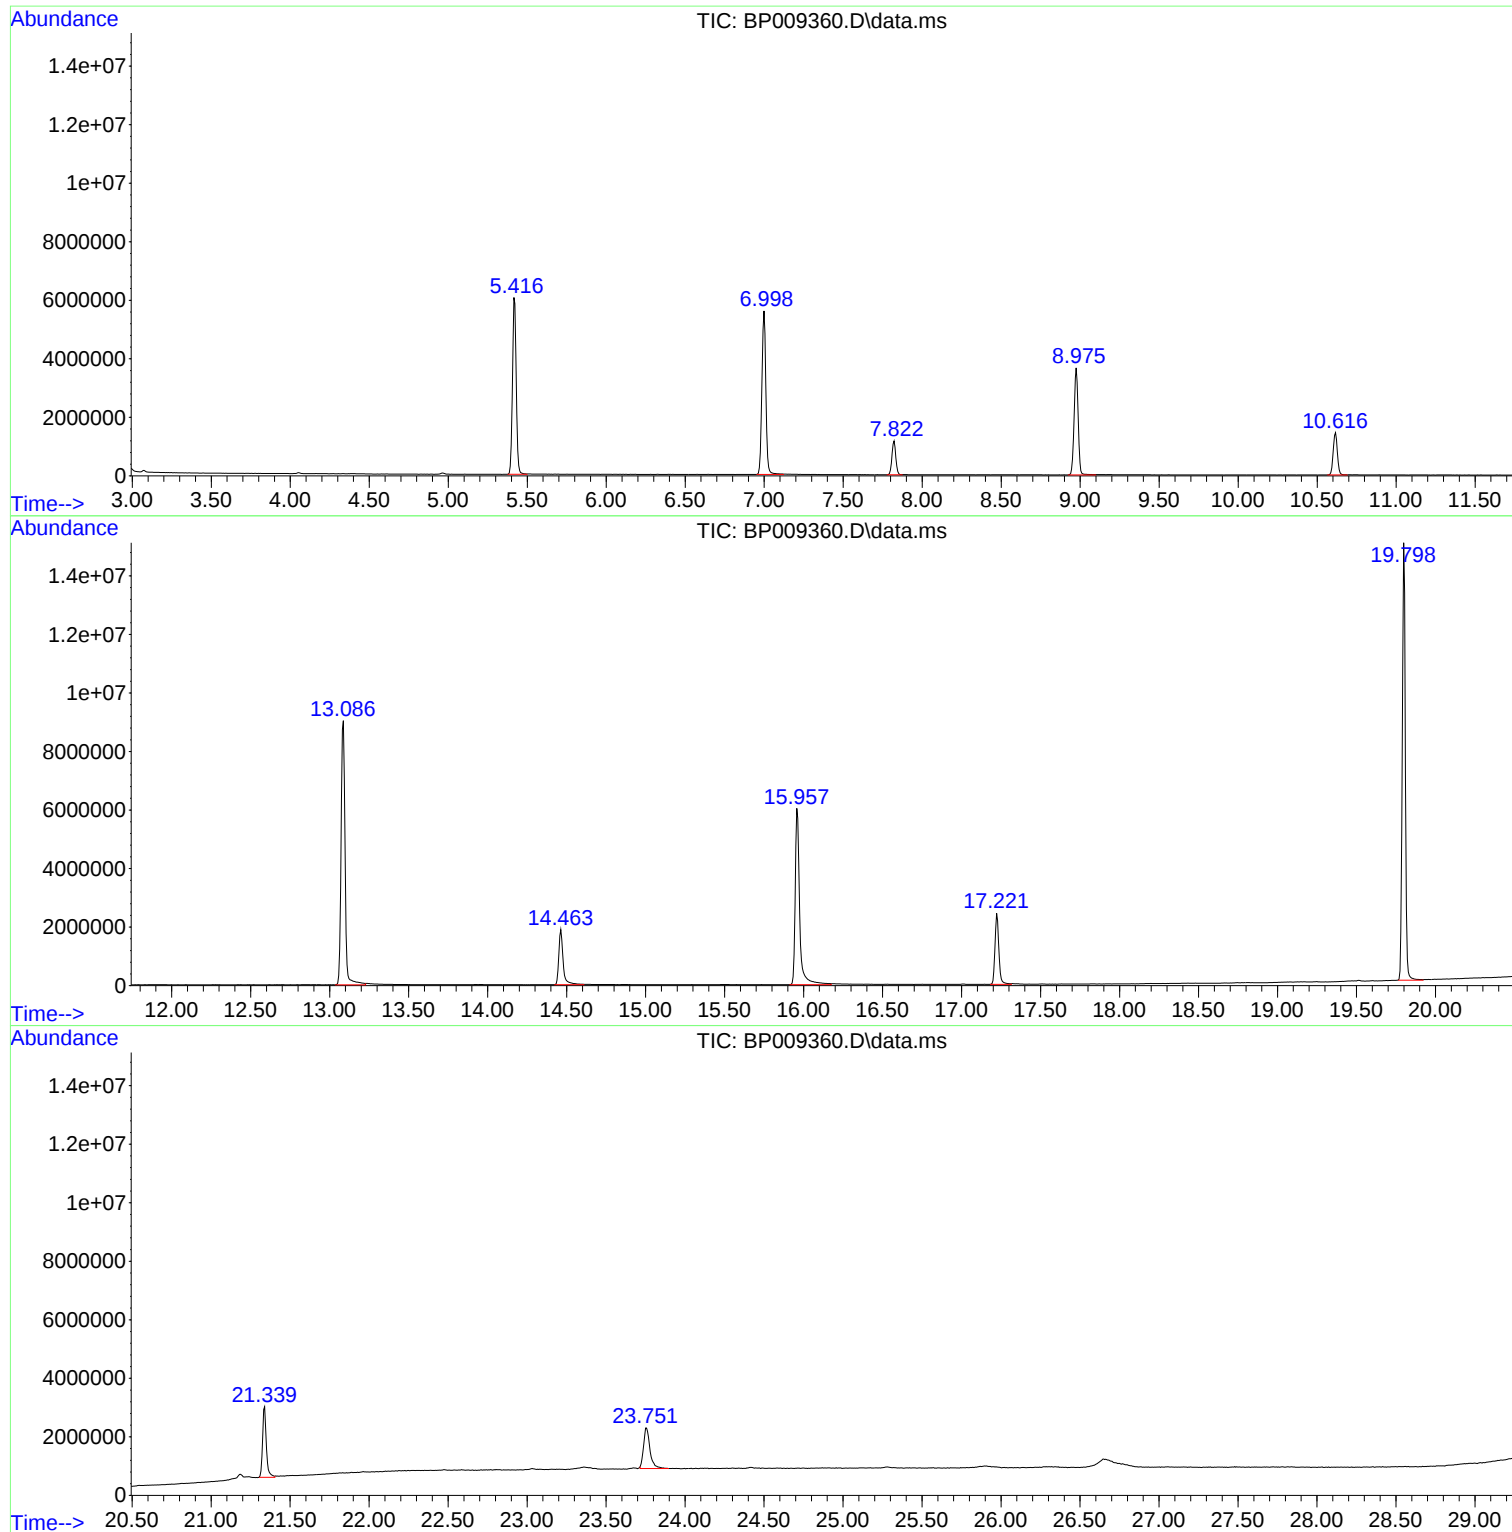

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009360.D
Acq On : 11 Mar 2022 12:10
Operator : CG/JU
Sample : PB143234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143234BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009360.D
Acq On : 11 Mar 2022 12:10
Operator : CG/JU
Sample : PB143234BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143234BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------