

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
 Data File : BP009374.D
 Acq On : 11 Mar 2022 20:20
 Operator : CG/JU
 Sample : N1884-03 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HR-04-031022

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	29	rVB	241013	409833	2.33%	0.654%
2	5.428	408	415	429	rBV	1652757	2727569	15.51%	4.354%
3	7.016	677	685	697	rBV	1477301	2670901	15.19%	4.263%
4	7.816	814	821	830	rBV	1199927	2017718	11.48%	3.221%
5	8.969	1007	1017	1027	rBV	1011298	1823578	10.37%	2.911%
6	10.610	1286	1296	1313	rBV	1512236	2836644	16.13%	4.528%
7	13.081	1708	1716	1733	rBV	2431400	4227801	24.05%	6.748%
8	14.457	1943	1950	1971	rBV	1981154	3641015	20.71%	5.812%
9	15.957	2198	2205	2214	rBV	2131089	3477647	19.78%	5.551%
10	16.775	2339	2344	2353	rBV	144042	246744	1.40%	0.394%
11	17.222	2413	2420	2426	rBV	2673618	4435319	25.23%	7.080%
12	18.128	2570	2574	2581	rBV2	201012	306601	1.74%	0.489%
13	19.592	2820	2823	2828	rBV2	229548	294286	1.67%	0.470%
14	19.792	2852	2857	2869	rVB	4653451	6209548	35.32%	9.912%
15	21.327	3114	3118	3123	rVB	3459675	4391716	24.98%	7.010%
16	21.451	3134	3139	3155	rBV	11902187	17581722	100.00%	28.064%
17	23.745	3524	3529	3537	rVB2	2509306	5350474	30.43%	8.540%




Sum of corrected areas: 62649116

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009374.D
Acq On : 11 Mar 2022 20:20
Operator : CG/JU
Sample : N1884-03 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-04-031022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

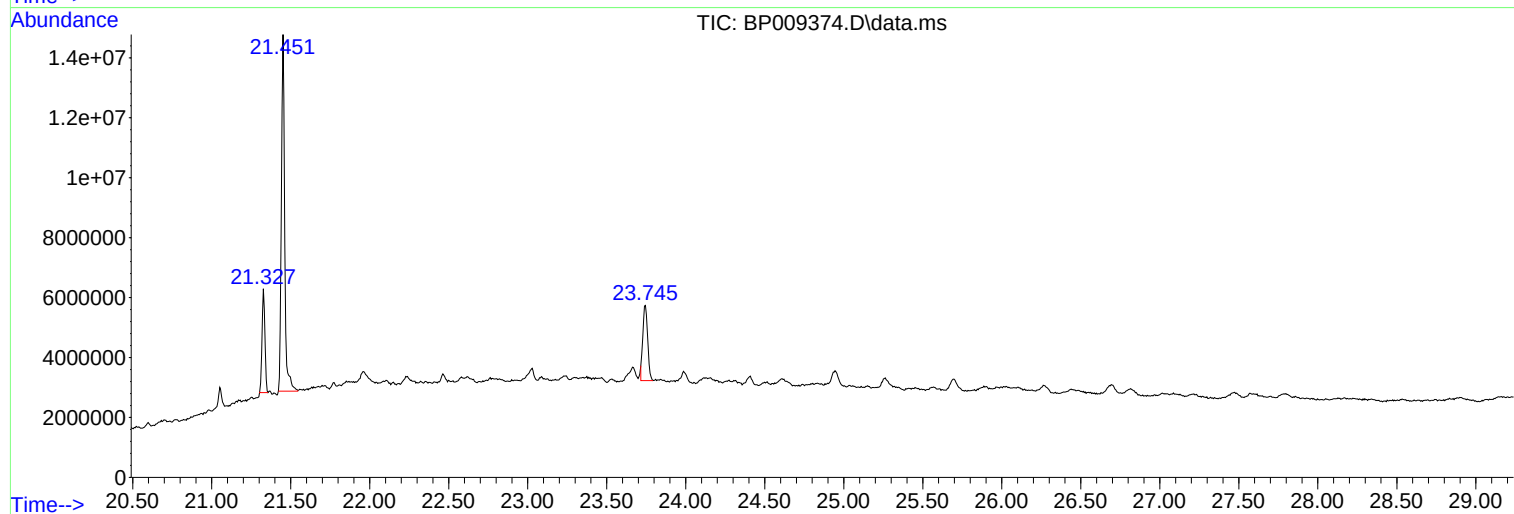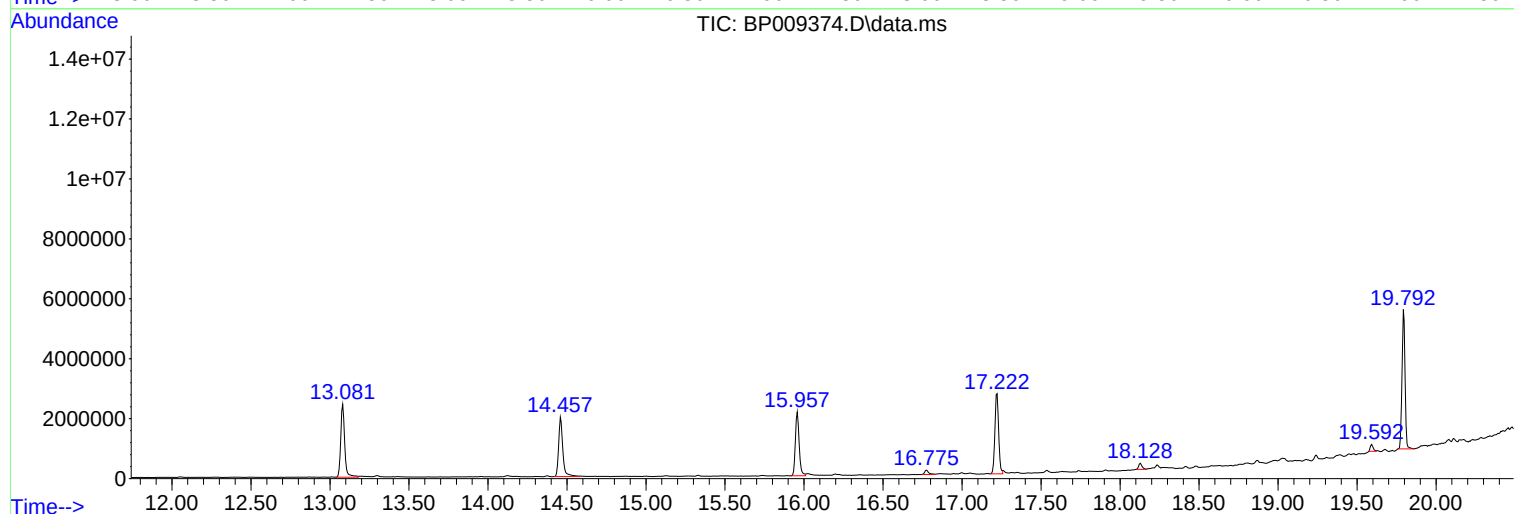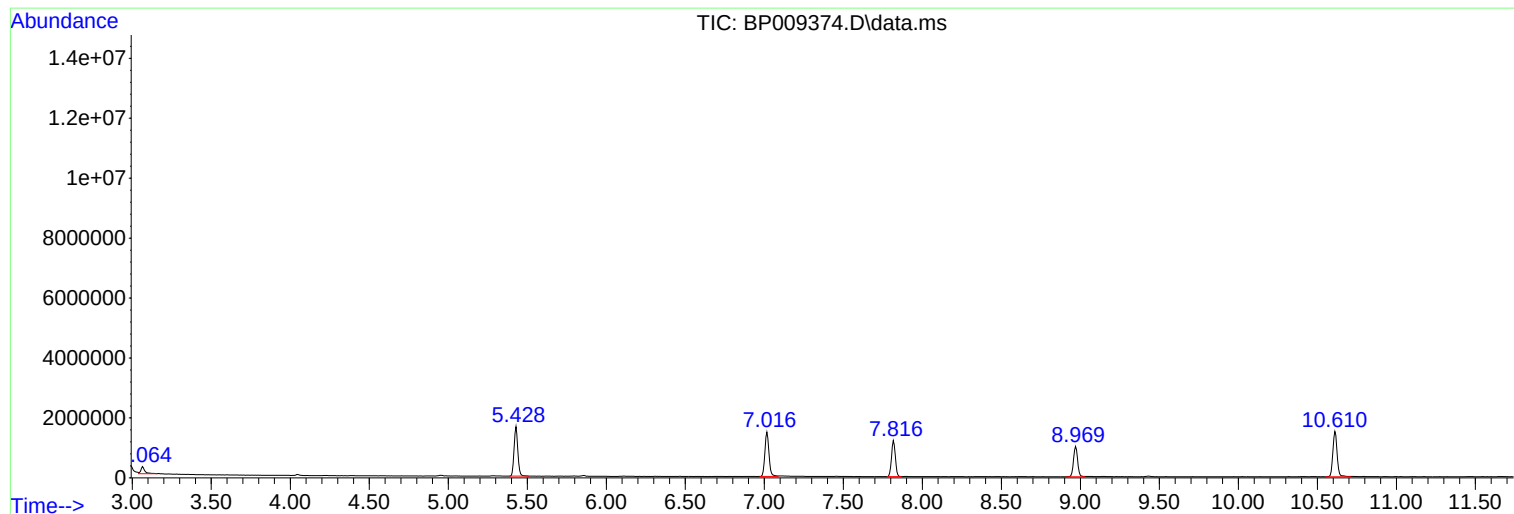

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009374.D
Acq On : 11 Mar 2022 20:20
Operator : CG/JU
Sample : N1884-03 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-04-031022










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.064	4.06 ng	409833	1,4-Dichlorobenzene-d4	7.816

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3		Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
4		Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5		N-Ethylformamide	73	C3H7NO	000627-45-2	9

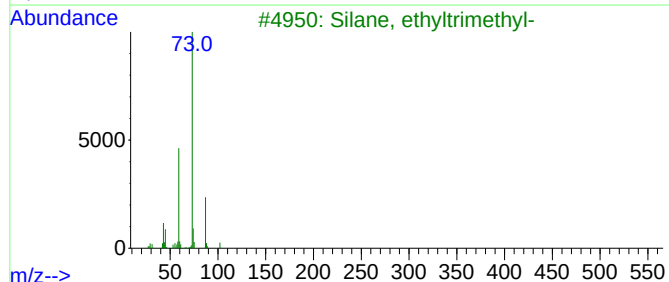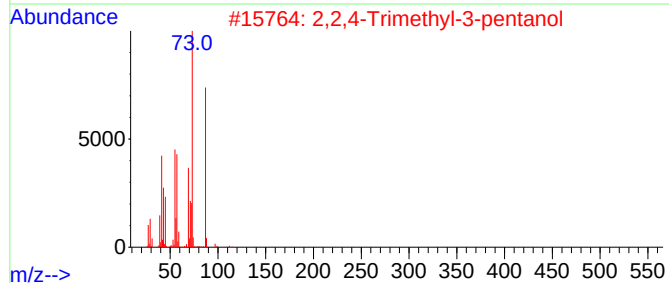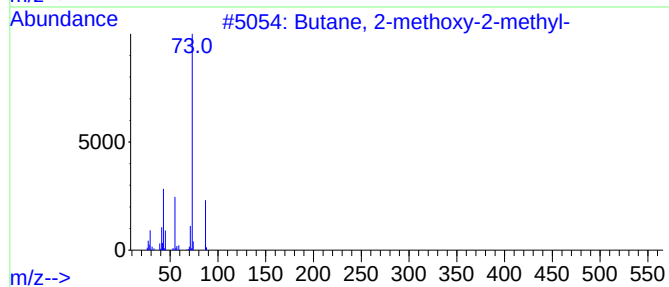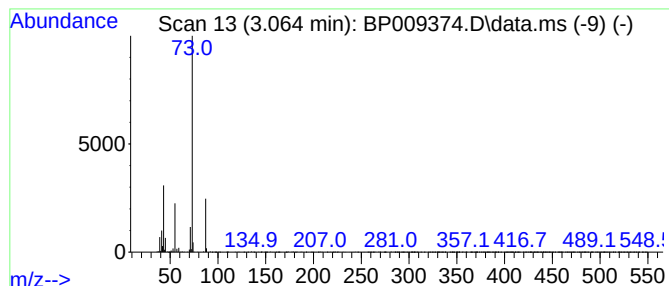

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009374.D
Acq On : 11 Mar 2022 20:20
Operator : CG/JU
Sample : N1884-03 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-04-031022










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.451	80.07 ng	17581700	Chrysene-d12	21.327

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	47
4			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28
5			Thiophene-3-carbonitrile, 4-(4-m...	277	C13H11NO2S2	1000268-75-0	9

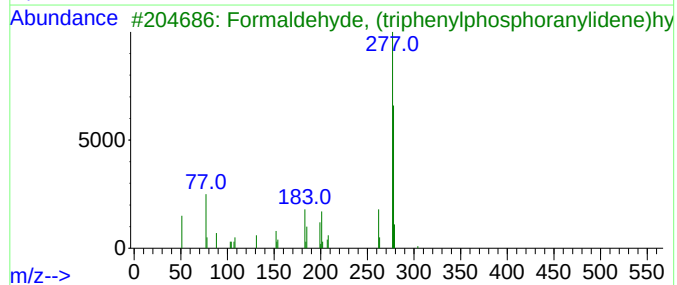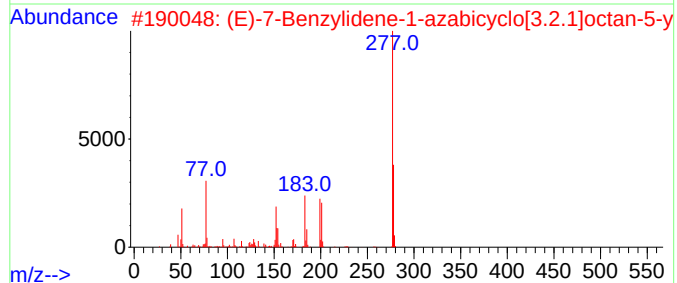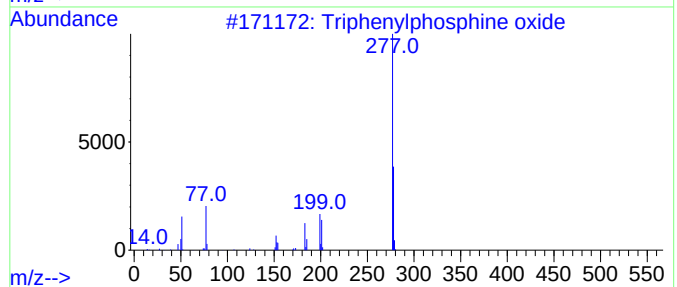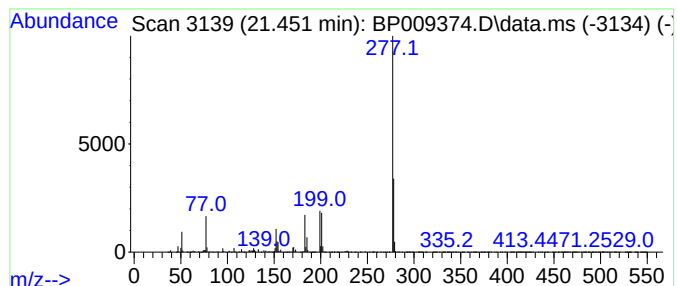

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
Data File : BP009374.D
Acq On : 11 Mar 2022 20:20
Operator : CG/JU
Sample : N1884-03 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HR-04-031022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.064	4.1	ng	409833	1	7.816	2017720	20.0
Triphenylphosph...	21.451	80.1	ng	17581700	5	21.327	4391720	20.0