
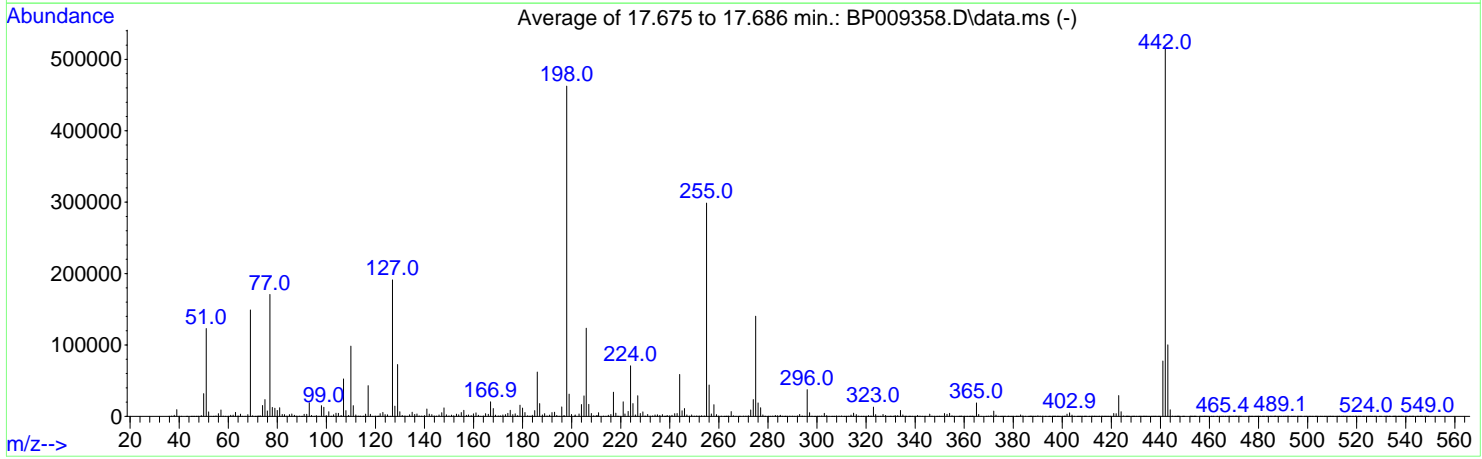


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
 Data File : BP009358.D
 Acq On : 11 Mar 2022 10:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

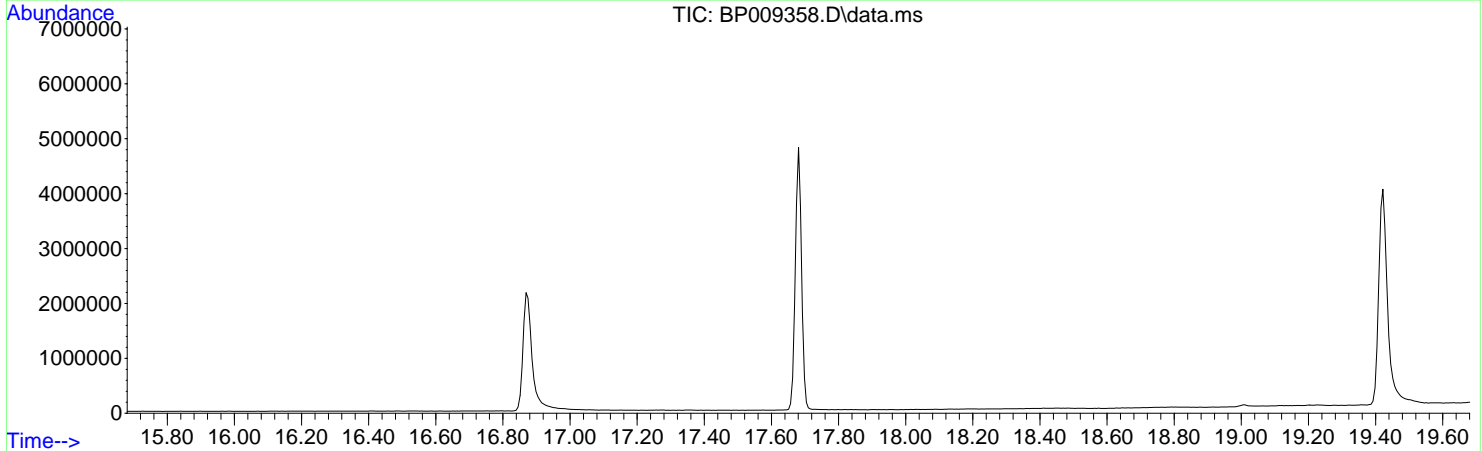




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	122946	PASS
68	69	0.00	2	1.7	2498	PASS
69	198	0.00	100	32.2	148944	PASS
70	69	0.00	2	0.5	811	PASS
127	198	10	80	41.4	191277	PASS
197	198	0.00	2	0.2	938	PASS
198	198	100	100	100.0	462485	PASS
199	198	5	9	6.7	31104	PASS
275	198	10	60	30.3	140326	PASS
365	198	1	100	4.1	18796	PASS
441	198	0.01	100	16.8	77640	PASS
442	442	100	100	100.0	515221	PASS
443	442	15	24	19.4	100127	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
 Data File : BP009358.D
 Acq On : 11 Mar 2022 10:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 12 06:04:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

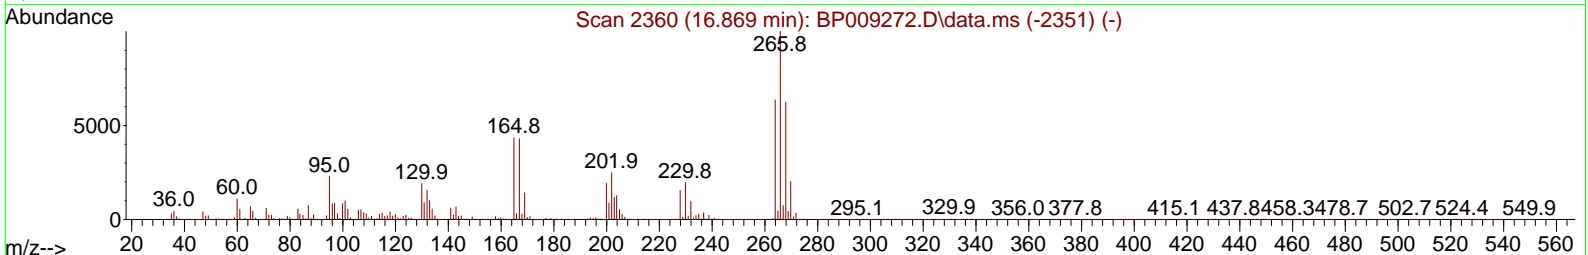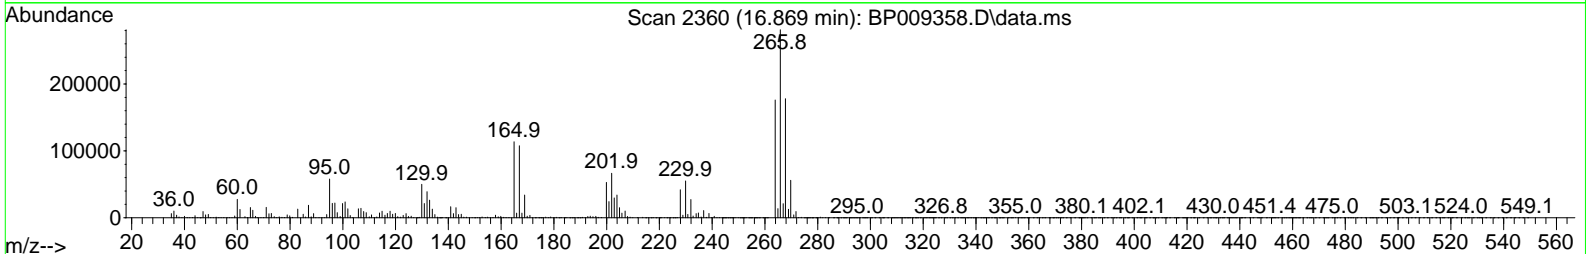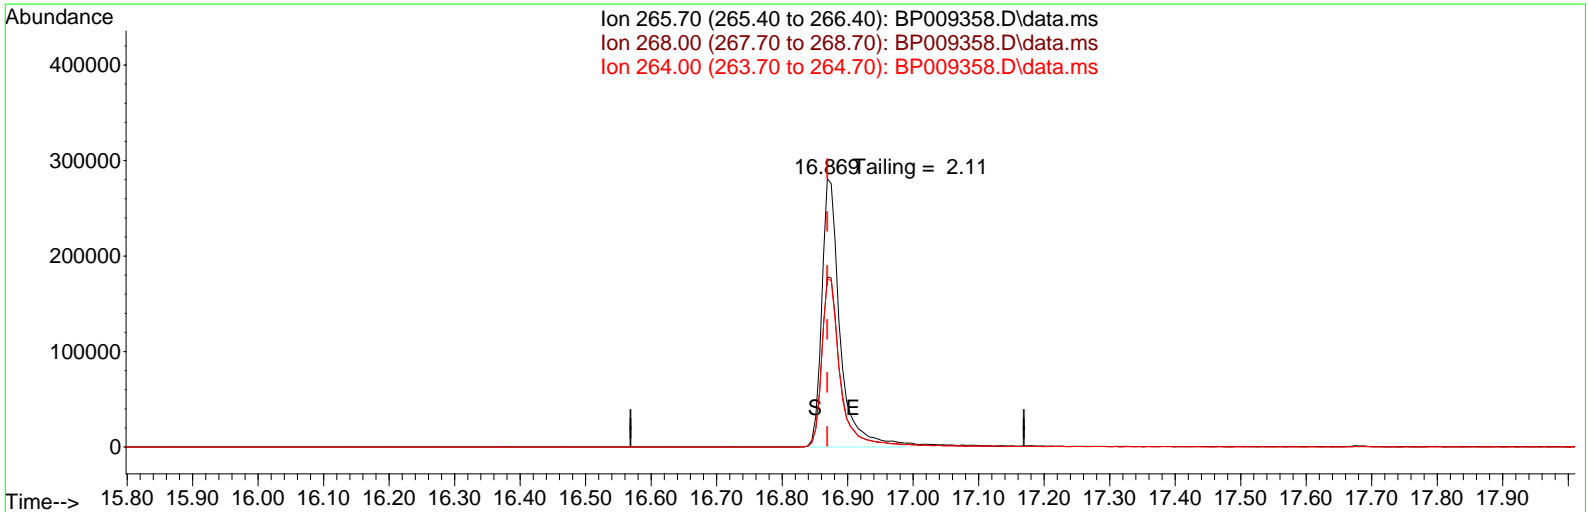

TIC: BP009358.D\data.ms

(70) Pentachlorophenol (C)

16.869min (+ 0.000) 552178.20 ng




response 550937

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.32
264.00	63.60	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031122\
 Data File : BP009358.D
 Acq On : 11 Mar 2022 10:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 12 06:04:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

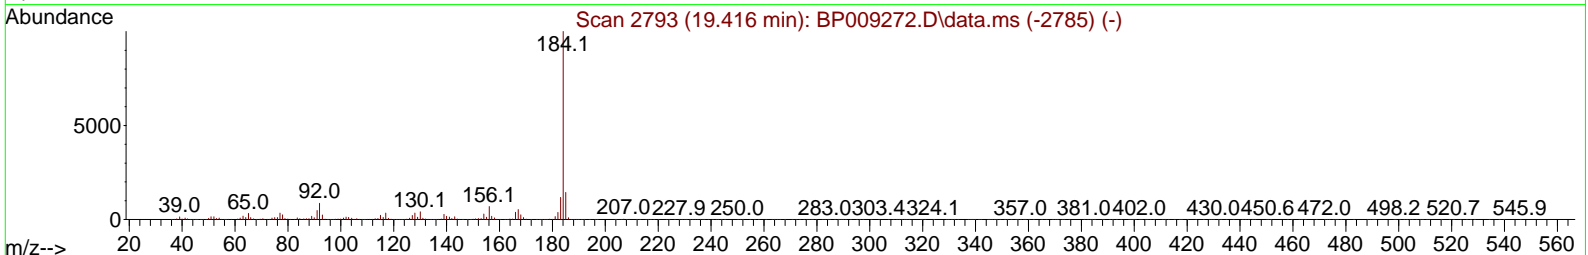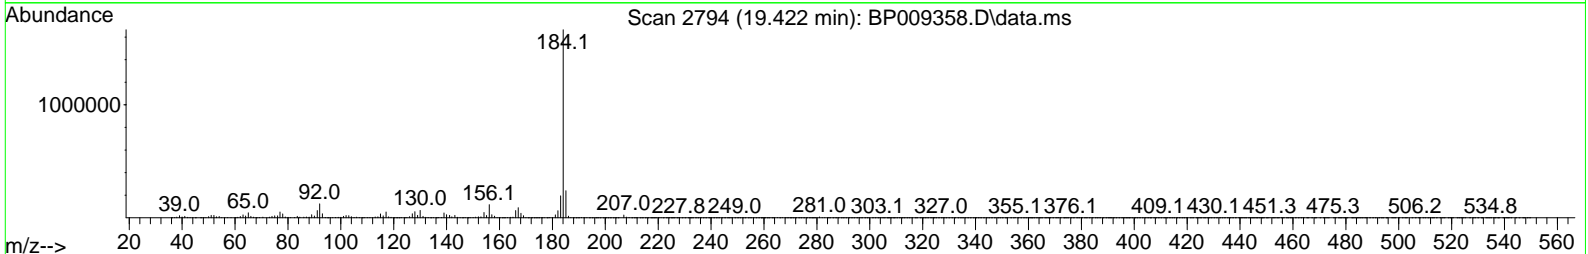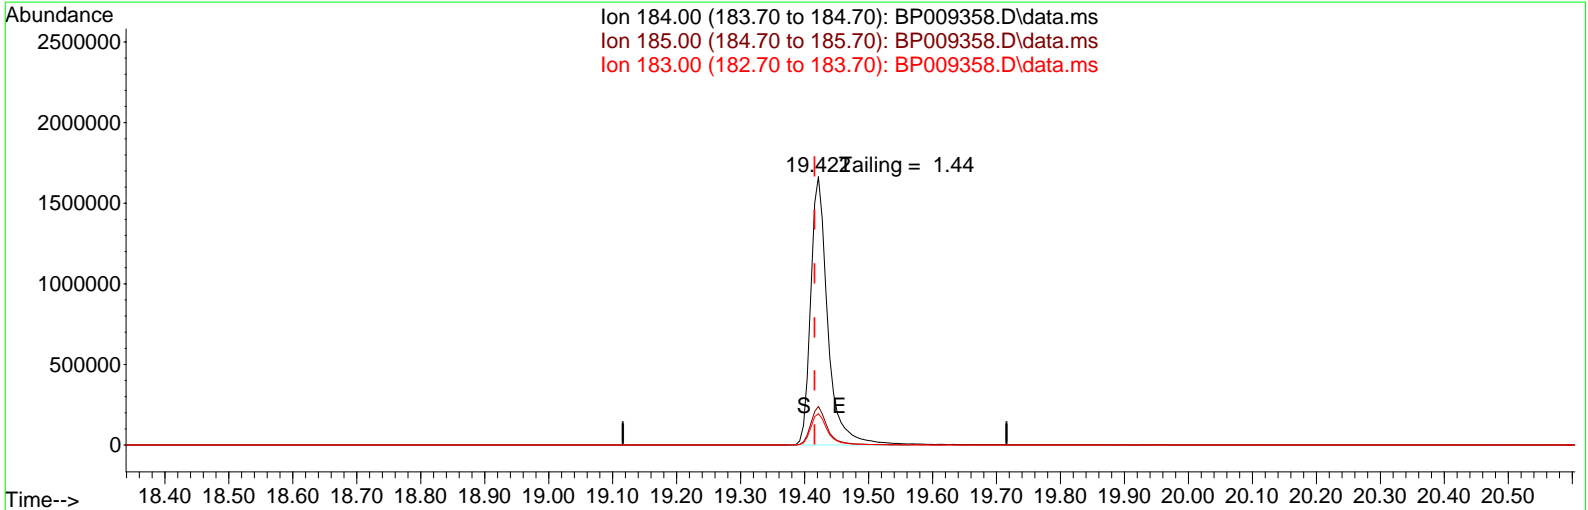

TIC: BP009358.D\data.ms

(77) Benzidine

19.422min (+ 0.006) 640828.06 ng

response 3109067

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	11.70	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/11/2022	BNA_P	<u>BP009358.D</u>
Compound Name	Response	Retention Time
DDT	1635803	20.633
DDD	35609	20.198
DDE	4187	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39796	1675599	2.38

Instrument :
 BNA_P
 ClientSampled :
 DFTPP