

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031125\
 Data File : BP024156.D
 Acq On : 11 Mar 2025 14:59
 Operator : RC/JU
 Sample : PB166629BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK629

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	38	rVB	70448	92366	1.06%	0.122%
2	3.675	96	100	124	rBV	936620	1422759	16.33%	1.879%
3	3.999	151	155	161	rVB	19677	27002	0.31%	0.036%
4	6.928	645	653	664	rBV	1164167	1841818	21.14%	2.433%
5	7.081	673	679	691	rVB	873919	1370151	15.73%	1.810%
6	7.287	707	714	726	rBV	1158781	1812851	20.81%	2.394%
7	7.752	786	793	807	rVB	883031	1336280	15.34%	1.765%
8	8.452	905	912	930	rBV	1397201	2332027	26.77%	3.080%
9	8.899	979	988	1003	rBV	947797	1605272	18.42%	2.120%
10	9.028	1004	1010	1015	rVV6	6414	12257	0.14%	0.016%
11	9.616	1102	1110	1120	rBV	839490	1241455	14.25%	1.640%
12	10.157	1194	1202	1218	rBV	1242976	2211858	25.39%	2.921%
13	10.534	1258	1266	1275	rBV	1224093	1992946	22.87%	2.632%
14	10.663	1281	1288	1308	rBV	1318068	2304383	26.45%	3.043%
15	12.122	1528	1536	1545	rBV	18868	40951	0.47%	0.054%
16	13.792	1814	1820	1832	rBV	2458691	3568506	40.96%	4.713%
17	14.081	1862	1869	1882	rBV	2770115	4142968	47.55%	5.472%
18	14.392	1915	1922	1932	rBV	1988210	2887607	33.14%	3.814%
19	14.604	1951	1958	1980	rBV	900986	1680995	19.29%	2.220%
20	15.404	2086	2094	2107	rBV	3588931	5311241	60.96%	7.015%
21	15.522	2107	2114	2127	rVV	1015261	1484386	17.04%	1.960%
22	15.645	2131	2135	2142	rVB	16412	31532	0.36%	0.042%
23	16.981	2356	2362	2369	rBV2	11129	18293	0.21%	0.024%
24	17.198	2392	2399	2409	rBV2	2539208	3761048	43.17%	4.967%
25	17.298	2409	2416	2437	rVV	4704277	6299088	72.30%	8.319%
26	18.145	2556	2560	2565	rBV8	11071	18950	0.22%	0.025%
27	19.222	2739	2743	2748	rBV	54328	80600	0.93%	0.106%
28	19.298	2752	2756	2761	rVV	46541	67125	0.77%	0.089%
29	19.669	2813	2819	2831	rBV	5435515	7921496	90.92%	10.462%
30	21.651	3150	3156	3168	rBV	3101064	4792807	55.01%	6.330%
31	24.821	3684	3695	3712	rVB	3058083	8712756	100.00%	11.507%
32	25.057	3726	3735	3751	rVB2	1910315	5292393	60.74%	6.990%




Sum of corrected areas: 75716167

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031125\
Data File : BP024156.D
Acq On : 11 Mar 2025 14:59
Operator : RC/JU
Sample : PB166629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK629

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

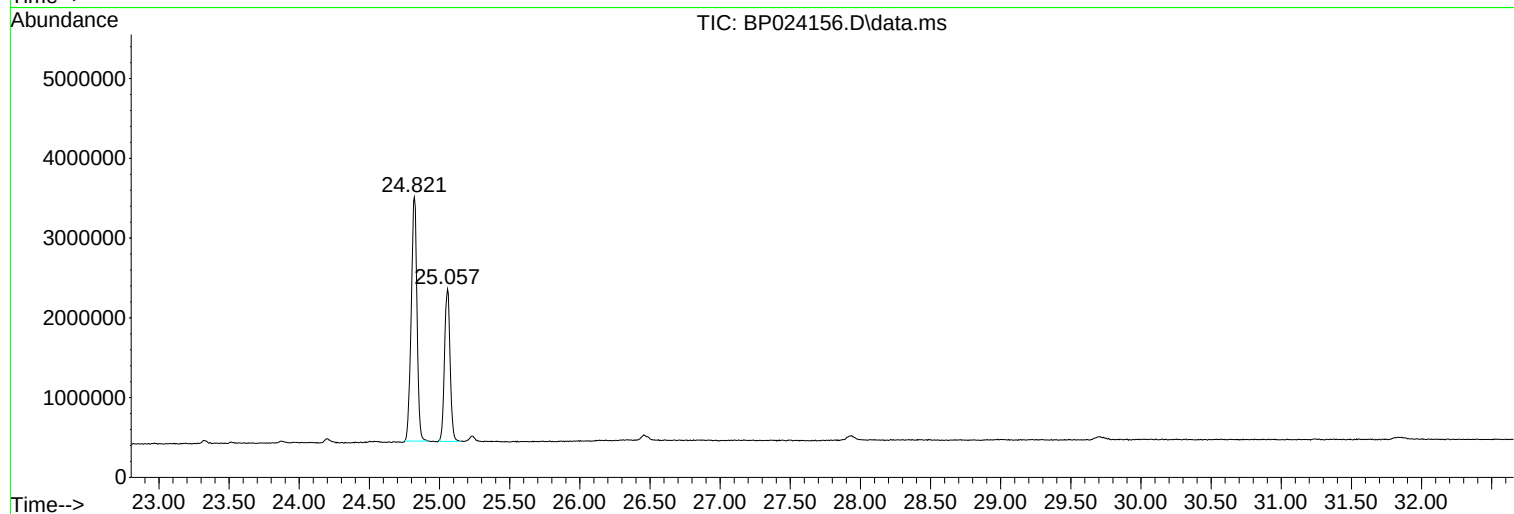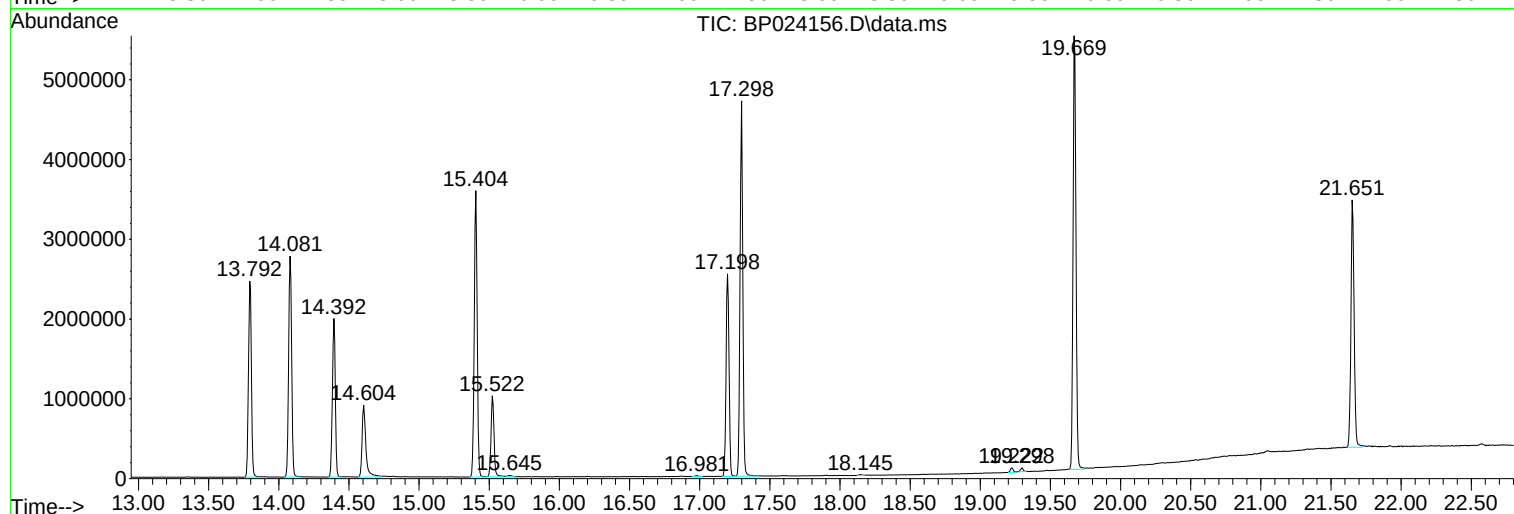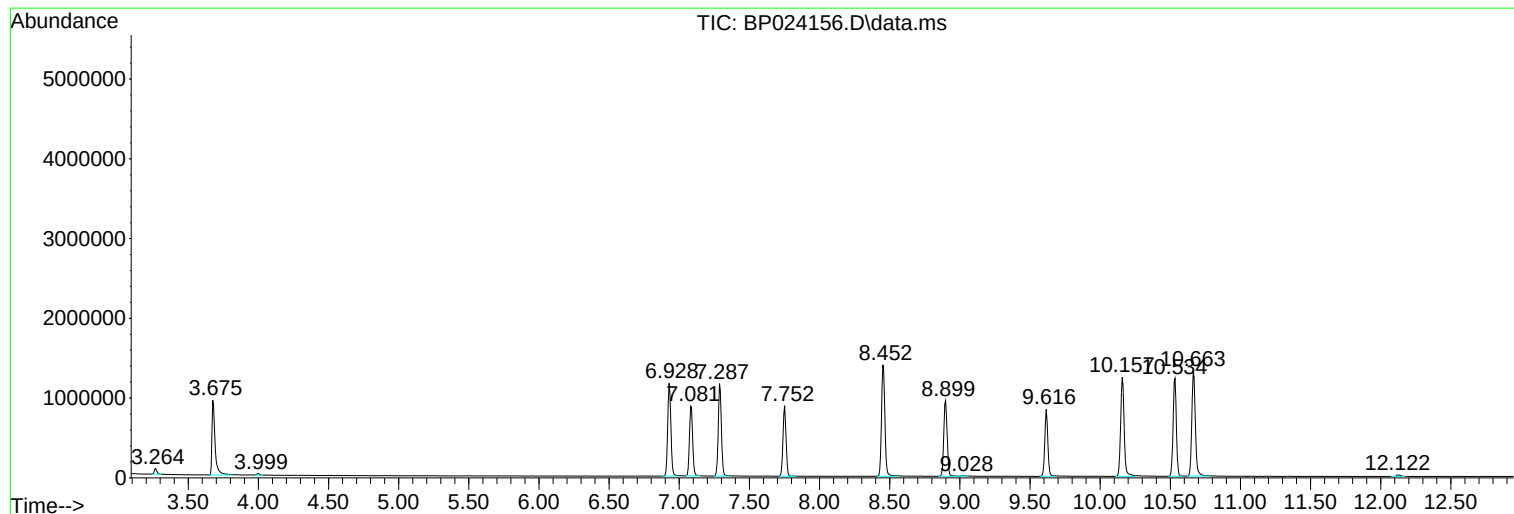

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031125\
Data File : BP024156.D
Acq On : 11 Mar 2025 14:59
Operator : RC/JU
Sample : PB166629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK629

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031125\
Data File : BP024156.D
Acq On : 11 Mar 2025 14:59
Operator : RC/JU
Sample : PB166629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK629

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc