

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
 Data File : BP002191.D
 Acq On : 12 Mar 2020 19:18
 Operator : CG/JU
 Sample : L1786-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC0

Quant Time: Mar 13 03:07:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 13 02:52:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	286720	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1189666	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	725859	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1565182	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1537490	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1784780	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	39900	5.98	ng/uL	0.00
5) Phenol-d5	6.81	99	682518	31.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	402454	34.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	598454	31.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	516504	28.74	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	273919	29.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	295924	28.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	574695	29.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	793072	36.53	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1707802	31.09	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2115293	32.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	223751	21.31	ng/ul	0.00
58) Fluorene-d10	15.26	176	1571125	33.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	162576	18.84	ng/ul	0.00
71) Anthracene-d10	17.12	188	2311460	32.86	ng/ul	0.00
79) Pyrene-d10	19.36	212	2729004	33.91	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3047481	33.37	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.73	163	387747	6.838	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002191.D
Acq On : 12 Mar 2020 19:18
Operator : CG/JU
Sample : L1786-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC0

Quant Time: Mar 13 03:07:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 13 02:52:52 2020
Response via : Initial Calibration

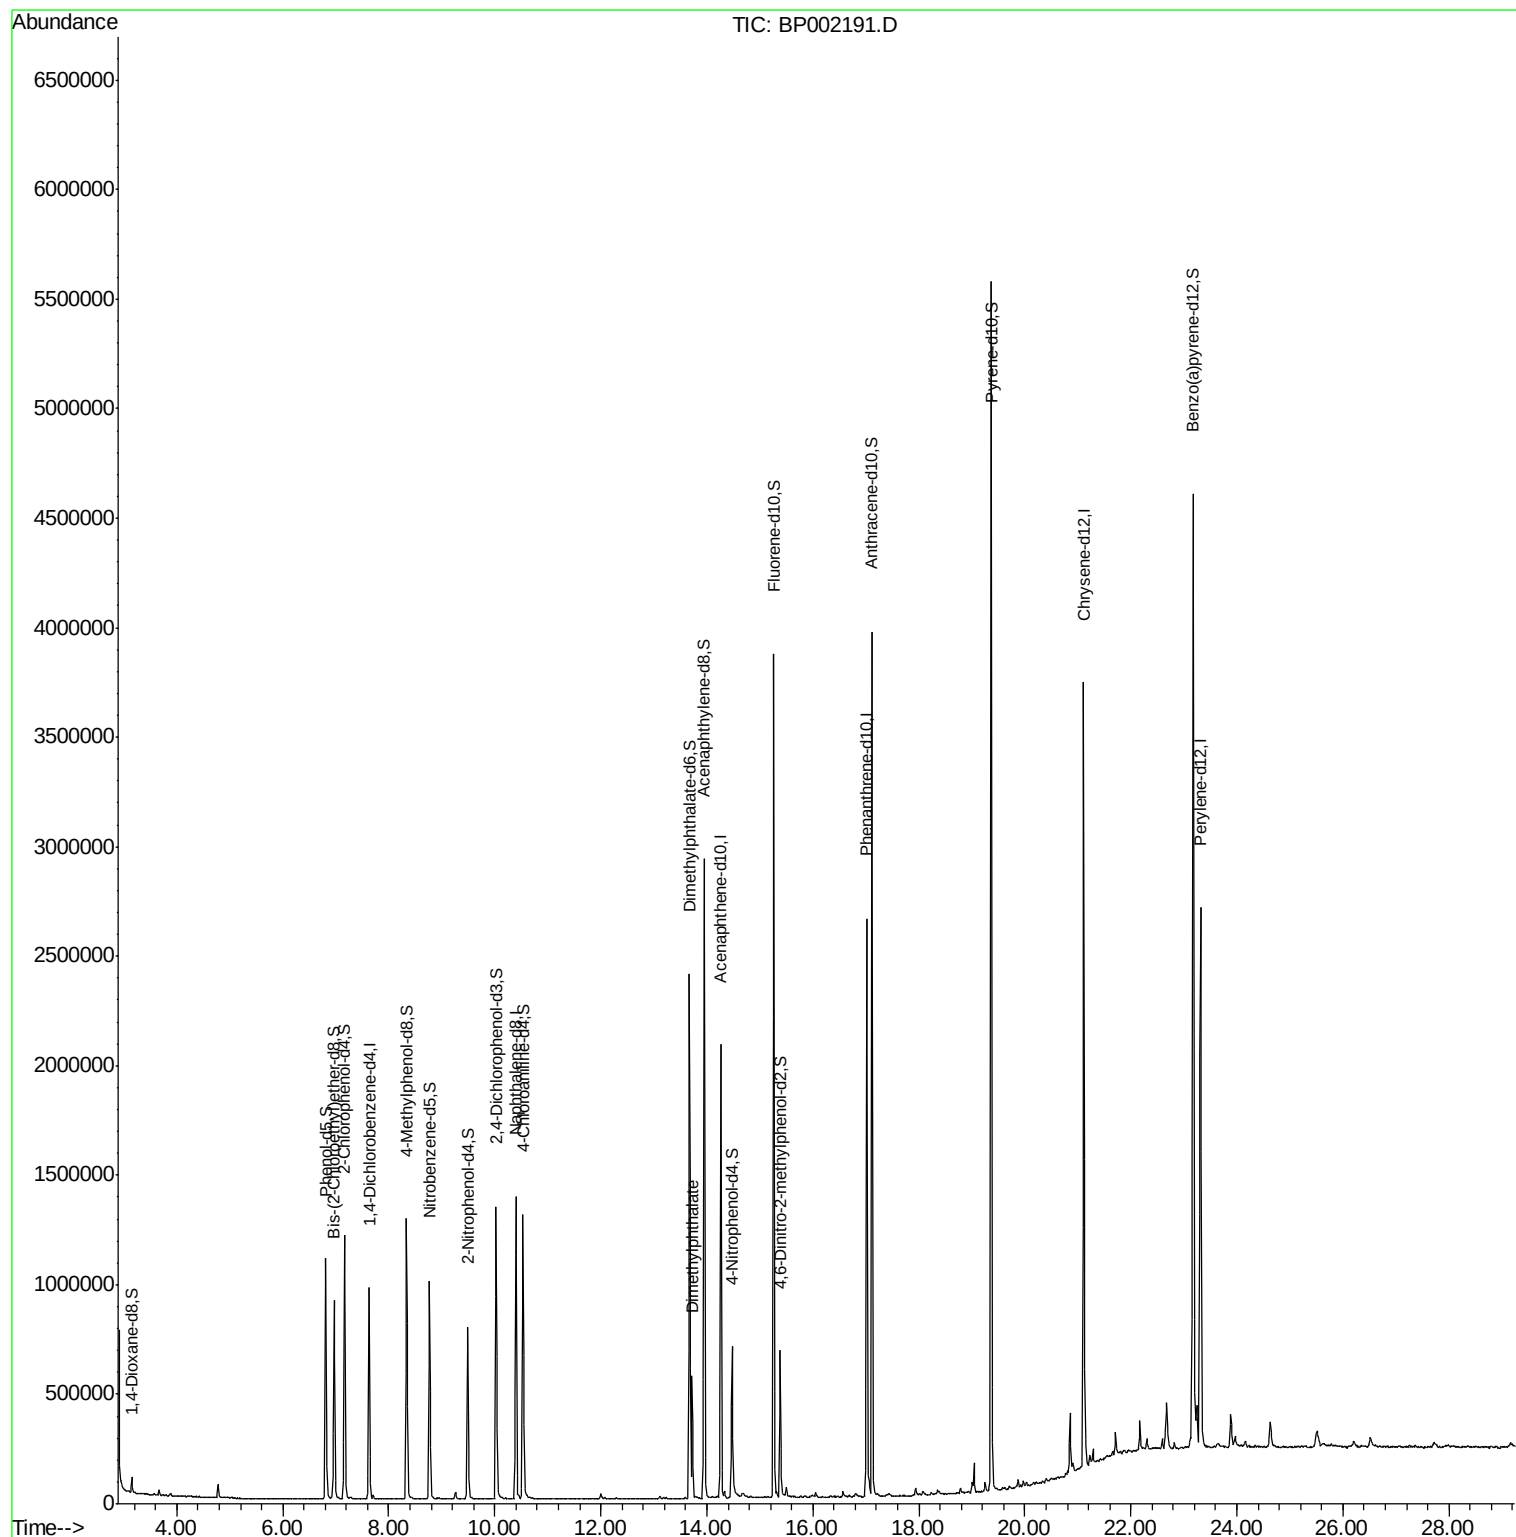

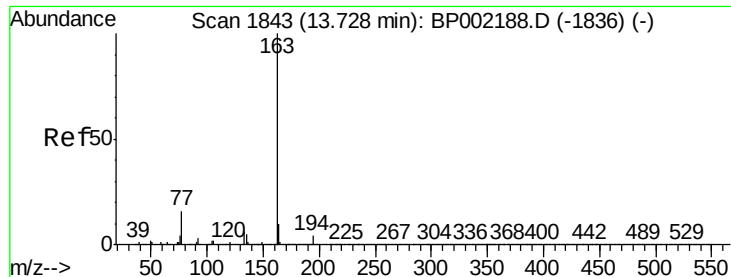

#45

Dimethylphthalate

Concen: 6.838 ng/ul

RT: 13.73 min Scan# 1843

Delta R.T. 0.00 min

Lab File: BP002191.D

Acq: 12 Mar 2020 19:18

Instrument :

BNA_P

ClientSampleId :

C0AC0


Tot Ion:163 Resp: 387747

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 9.5 8.2 12.4

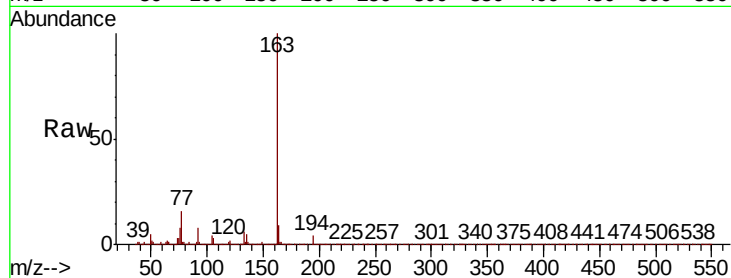

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

