

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
 Data File : BP002193.D
 Acq On : 12 Mar 2020 20:26
 Operator : CG/JU
 Sample : L1786-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB9

Quant Time: Mar 13 03:42:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 13 02:52:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	299835	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1235750	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	756243	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1622212	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1606045	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1859402	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	41791	5.99	ng/uL	0.00
5) Phenol-d5	6.81	99	734613	32.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	434746	35.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	647406	32.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	551946	29.37	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	299316	31.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	323496	30.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	609301	29.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	841448	37.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	1799128	31.44	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2261746	33.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	245378	22.43	ng/ul	0.00
58) Fluorene-d10	15.26	176	1657127	33.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	178071	19.91	ng/ul	0.00
71) Anthracene-d10	17.12	188	2434630	33.39	ng/ul	0.00
79) Pyrene-d10	19.36	212	2915526	34.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3215239	33.80	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.72	163	352895	5.973	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002193.D
Acq On : 12 Mar 2020 20:26
Operator : CG/JU
Sample : L1786-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB9

Quant Time: Mar 13 03:42:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 13 02:52:52 2020
Response via : Initial Calibration

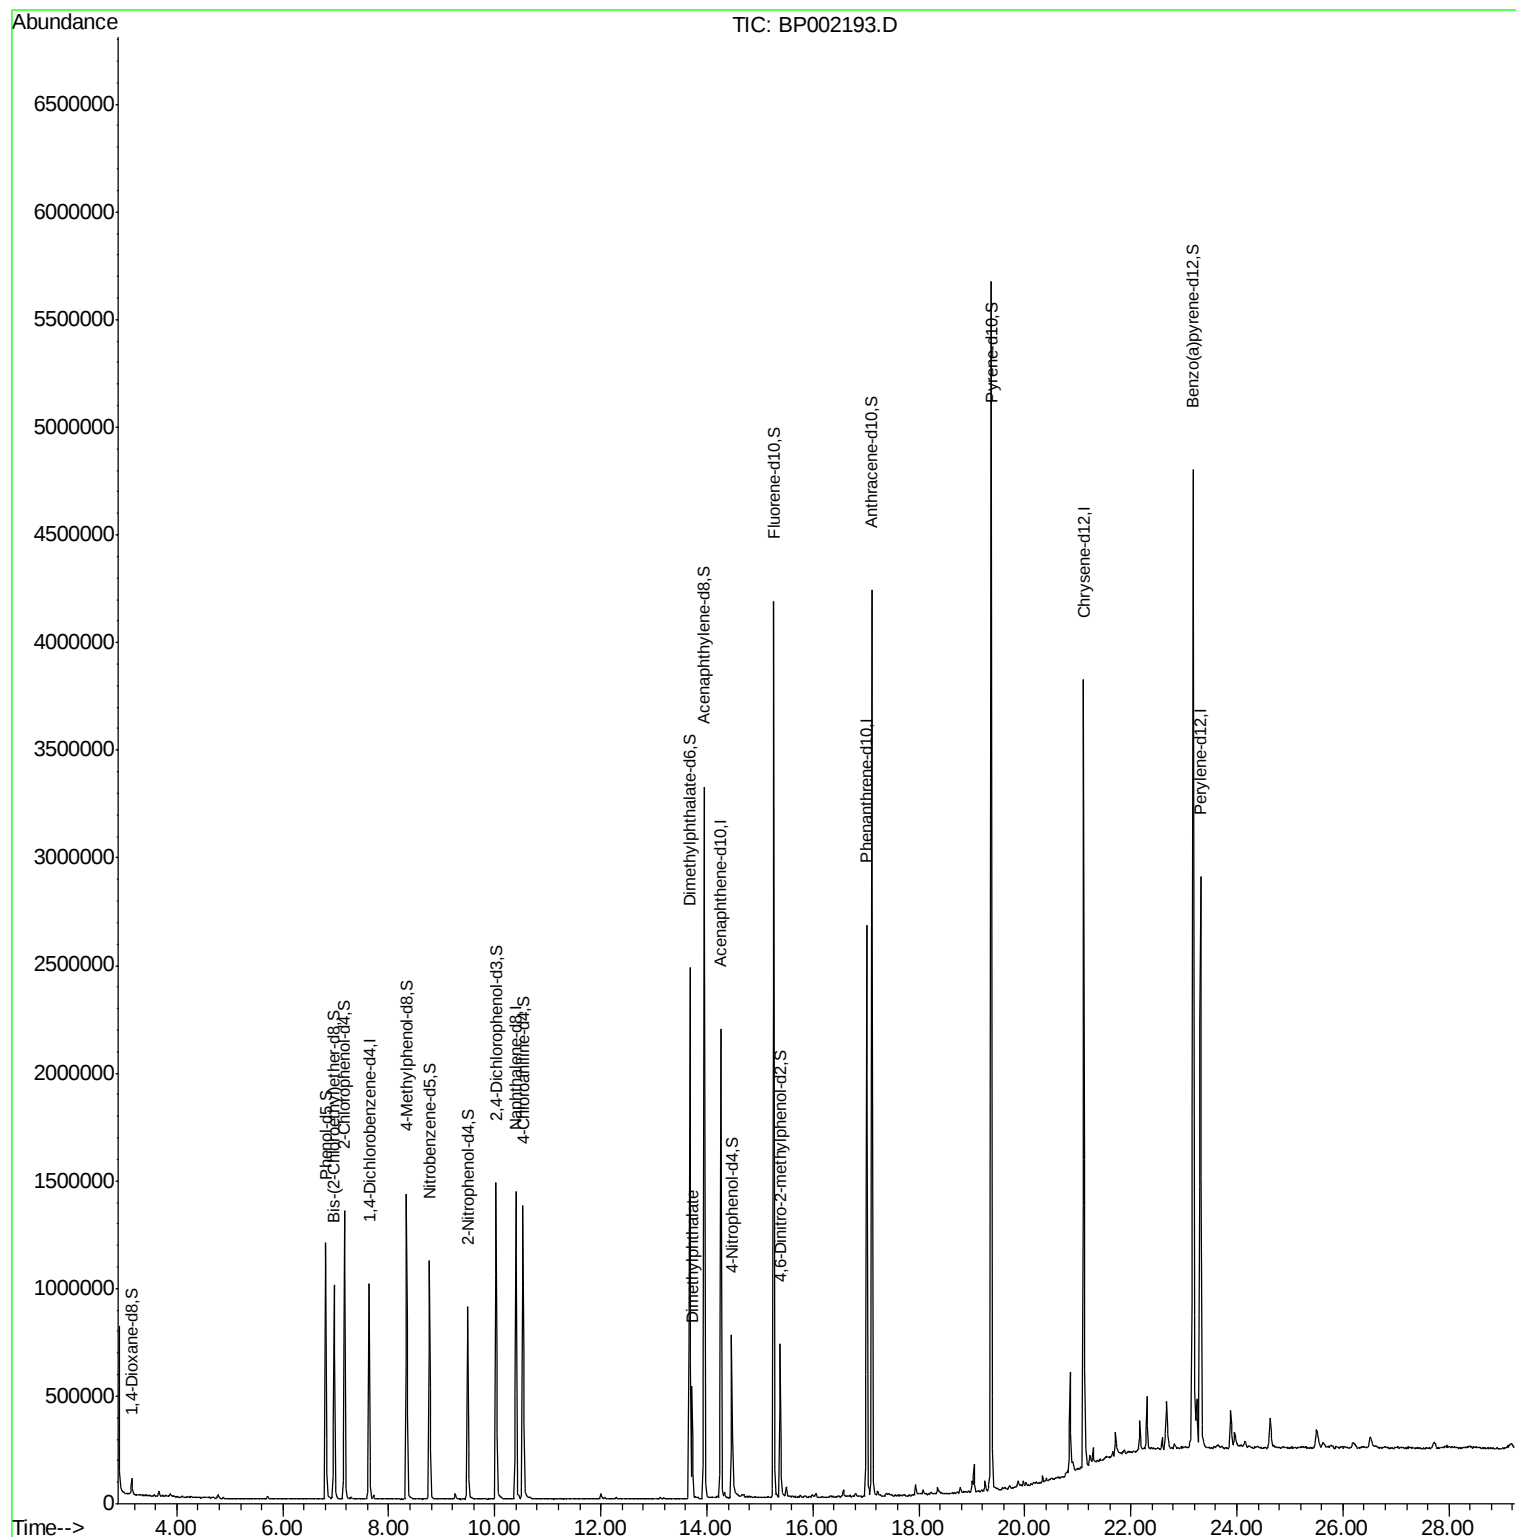

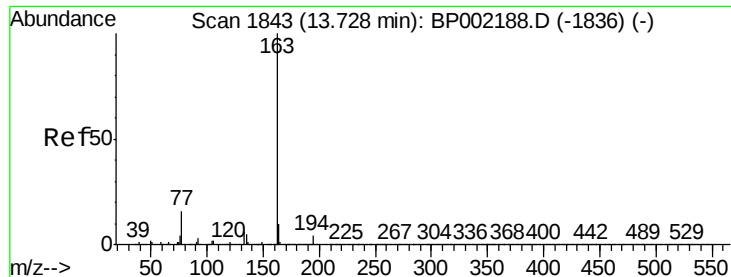

#45

Dimethylphthalate

Concen: 5.973 ng/ul

RT: 13.72 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BP002193.D

Acq: 12 Mar 2020 20:26

Instrument :

BNA_P

ClientSampleId :

C0AB9


Tot Ion:163 Resp: 352895

Ion Ratio Lower Upper

163 100

194 4.2 3.6 5.4

164 10.3 8.2 12.4

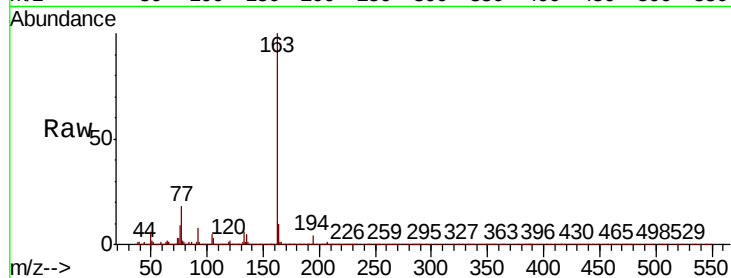

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

