

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
 Data File : BP002196.D
 Acq On : 12 Mar 2020 22:08
 Operator : CG/JU
 Sample : L1899-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0EP7

Quant Time: Mar 13 03:47:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 13 02:52:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	524351	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	2141326	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	1301694	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	2743186	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	2703778	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	3376431	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	32289	2.65	ng/uL	0.00
5) Phenol-d5	6.81	99	121509	3.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	305896	14.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	389671	11.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	223455	6.80	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	217172	13.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	231037	12.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	427878	12.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	30223	0.77	ng/ul	0.01
44) Dimethylphthalate-d6	13.67	166	1462778	14.85	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	1683682	14.29	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	37989	2.02	ng/ul	0.00
58) Fluorene-d10	15.26	176	1344387	15.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	183232	12.12	ng/ul	0.00
71) Anthracene-d10	17.12	188	2330275	18.90	ng/ul	0.00
79) Pyrene-d10	19.36	212	2759457	19.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3303754	19.12	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.72	163	157663	1.550	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002196.D
Acq On : 12 Mar 2020 22:08
Operator : CG/JU
Sample : L1899-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EP7

Quant Time: Mar 13 03:47:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 13 02:52:52 2020
Response via : Initial Calibration

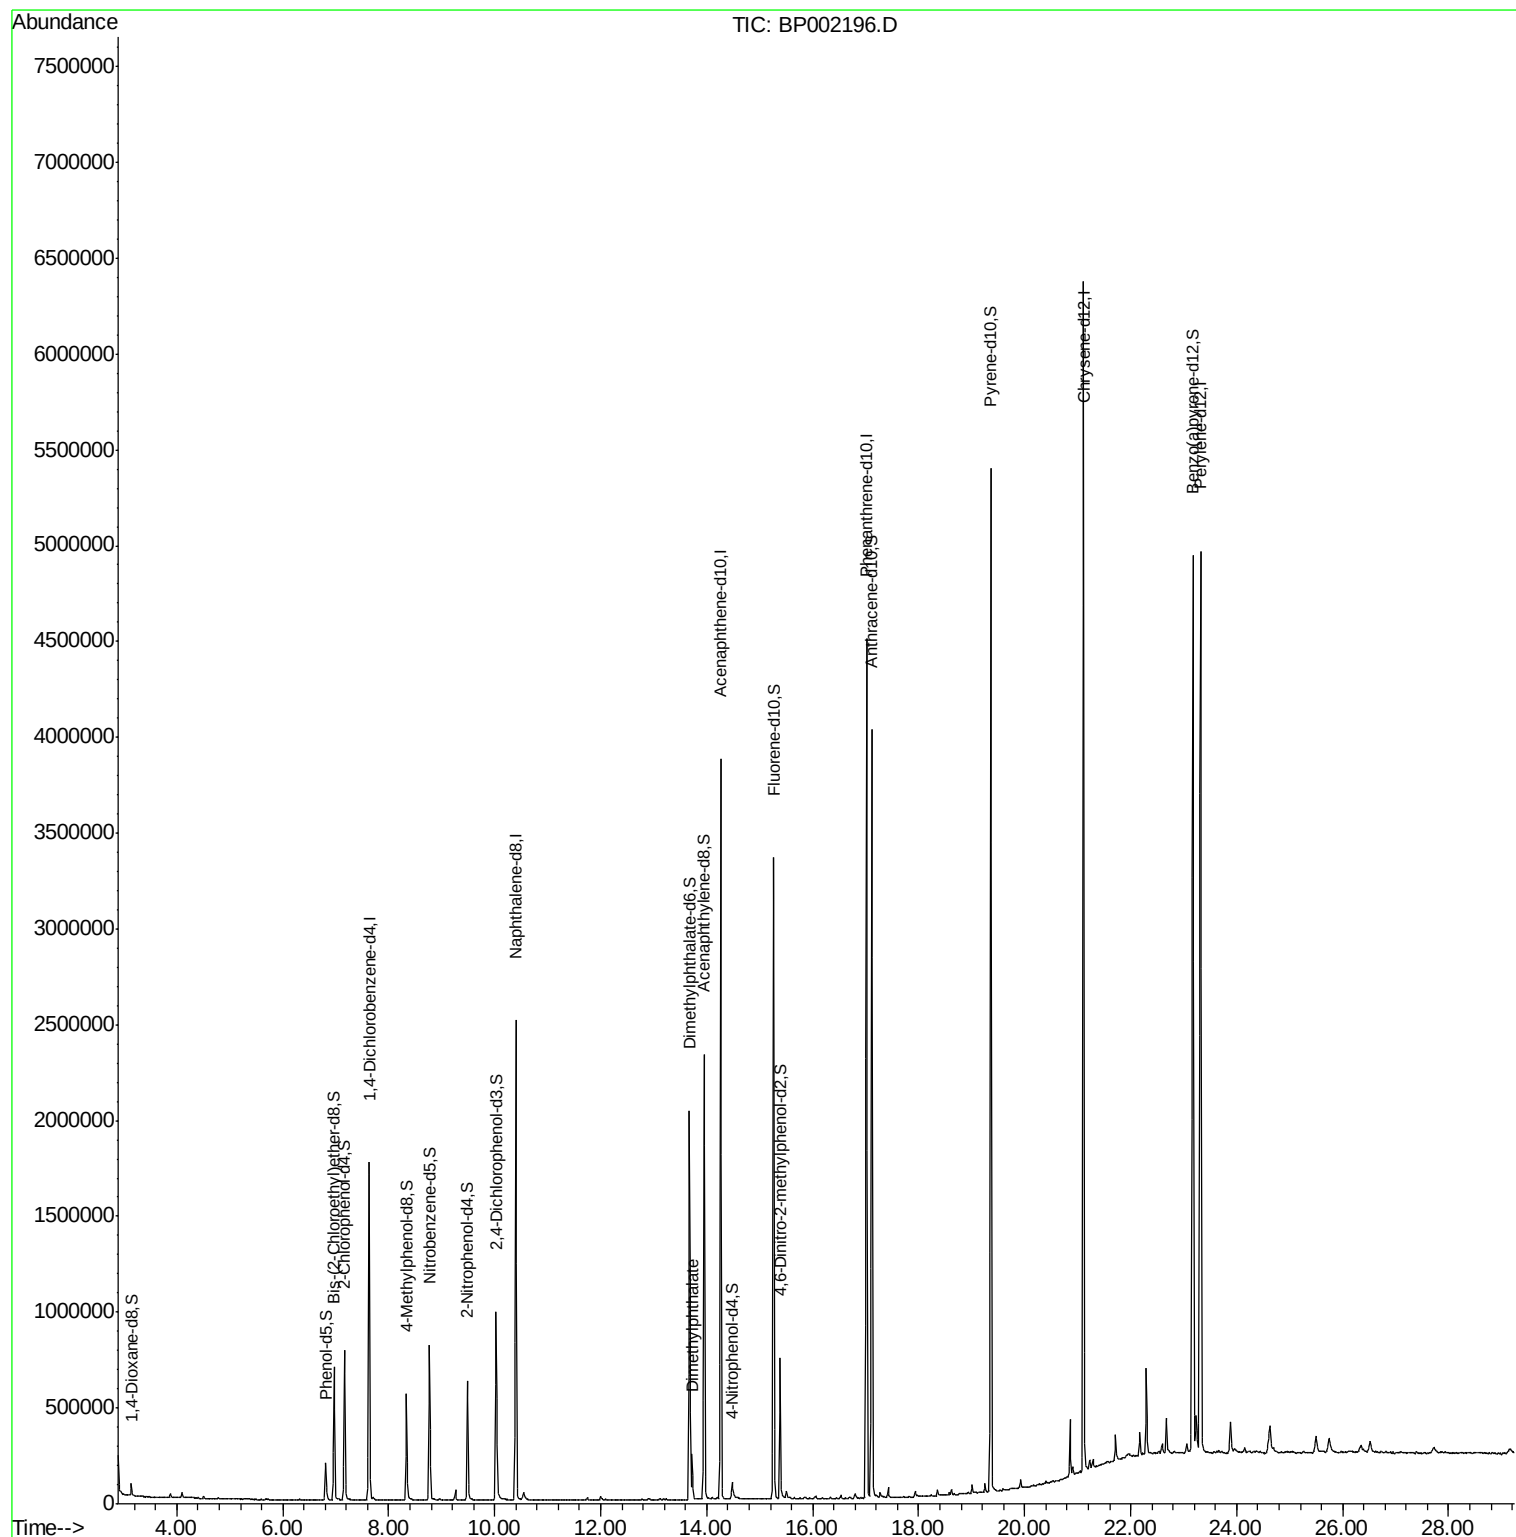

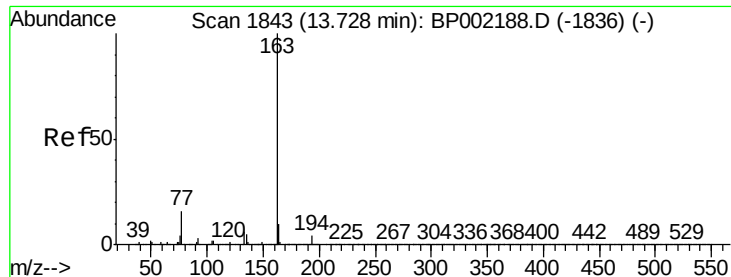

#45

Dimethylphthalate

Concen: 1.550 ng/ul

RT: 13.72 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BP002196.D

Acq: 12 Mar 2020 22:08

Instrument :

BNA_P

ClientSampleId :

C0EP7


Tot Ion:163 Resp: 157663

Ion Ratio Lower Upper

163 100

194 4.5 3.6 5.4

164 10.5 8.2 12.4

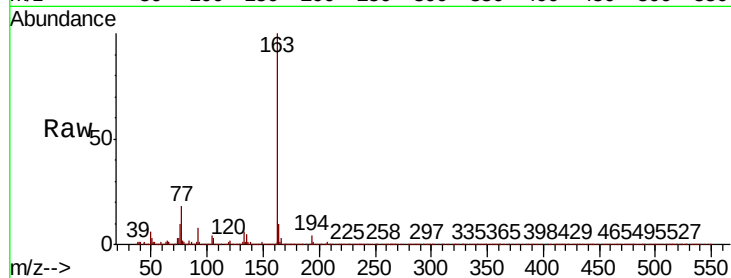

Abundance Ion 163.00 (162.70 to 163.70): E

150000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

