

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
 Data File : BP002198.D
 Acq On : 12 Mar 2020 23:16
 Operator : CG/JU
 Sample : L1899-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0EP3

Quant Time: Mar 13 03:51:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 13 02:52:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	269984	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1109843	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	677434	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1447131	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1418102	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1701439	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	31260	4.98	ng/uL	0.00
5) Phenol-d5	6.81	99	112190	5.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	281546	25.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	356537	20.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	207004	12.23	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	193673	22.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	210719	21.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	394575	21.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	24793	1.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1270418	24.78	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	1541688	25.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	24177	2.47	ng/ul	0.00
58) Fluorene-d10	15.26	176	1163036	26.22	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	127416	15.97	ng/ul	0.00
71) Anthracene-d10	17.12	188	1808583	27.81	ng/ul	0.00
79) Pyrene-d10	19.36	212	2092314	28.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2400911	27.58	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.72	163	215981	4.081	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002198.D
Acq On : 12 Mar 2020 23:16
Operator : CG/JU
Sample : L1899-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EP3

Quant Time: Mar 13 03:51:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 13 02:52:52 2020
Response via : Initial Calibration

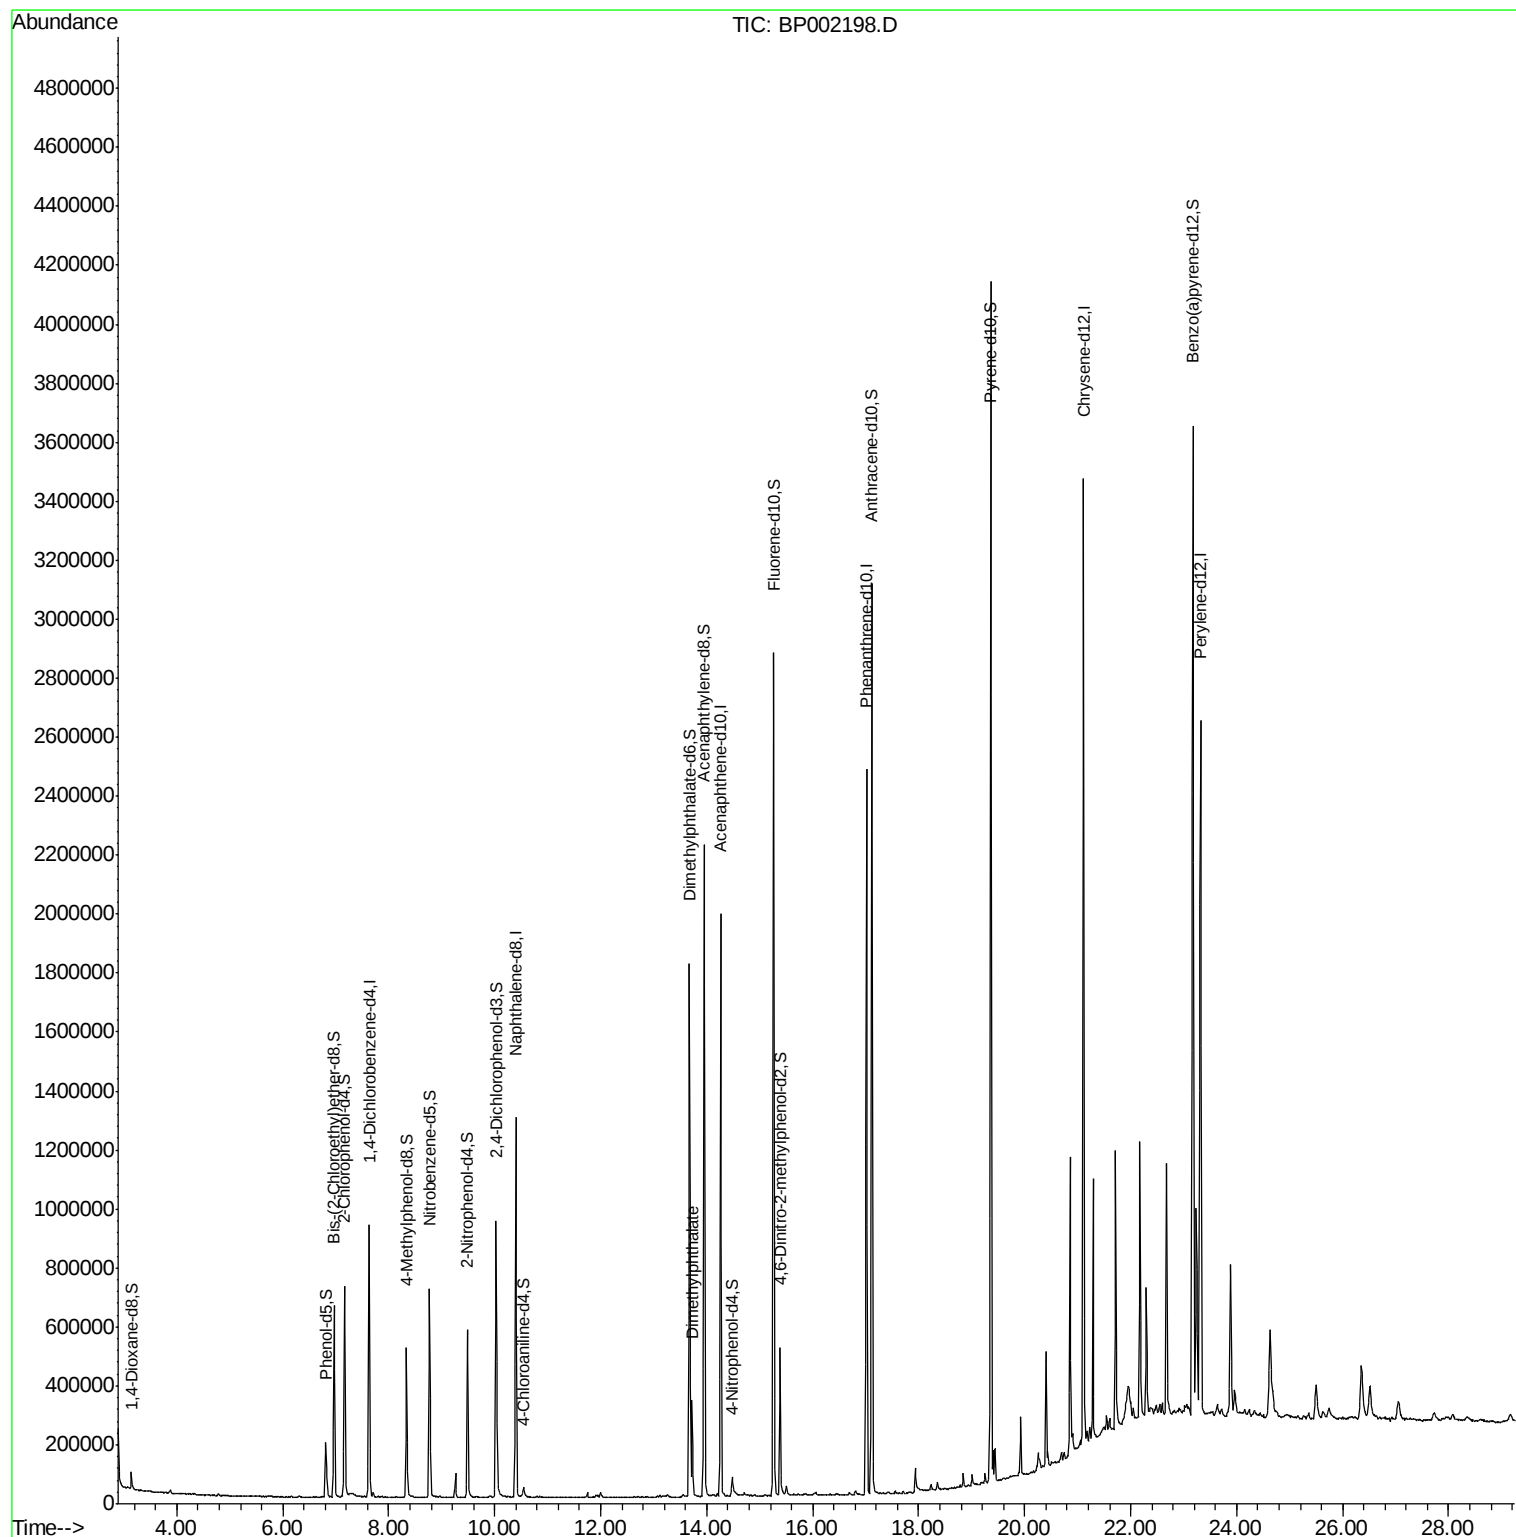

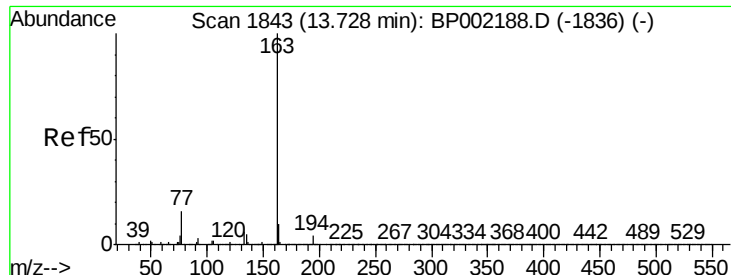

#45

Dimethylphthalate

Concen: 4.081 ng/ul

RT: 13.72 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BP002198.D

Acq: 12 Mar 2020 23:16

Instrument :

BNA_P

ClientSampleId :

C0EP3


Tot Ion:163 Resp: 215981

Ion Ratio Lower Upper

163 100

194 4.8 3.6 5.4

164 10.4 8.2 12.4

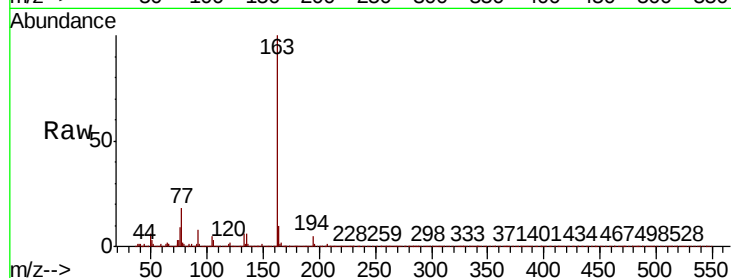

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

