

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
 Data File : BP002199.D
 Acq On : 12 Mar 2020 23:50
 Operator : CG/JU
 Sample : L1899-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0EQ2

Quant Time: Mar 13 03:54:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 13 02:52:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	276824	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1139294	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	687334	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1454731	20.00	ng/ul	0.00
78) Chrysene-d12	21.11	240	1416610	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1778628	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	33498	5.20	ng/uL	0.00
5) Phenol-d5	6.81	99	141929	6.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	361047	32.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	454800	24.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	265967	15.33	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	255752	29.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	275256	27.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	497621	26.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	34694	1.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1595907	30.68	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	1974115	31.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	30072	3.02	ng/ul	0.00
58) Fluorene-d10	15.26	176	1484674	32.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	170018	21.20	ng/ul	0.00
71) Anthracene-d10	17.12	188	2366789	36.20	ng/ul	0.00
79) Pyrene-d10	19.36	212	2705130	36.48	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3228302	35.48	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.72	163	103385	1.925	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002199.D
Acq On : 12 Mar 2020 23:50
Operator : CG/JU
Sample : L1899-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EQ2

Quant Time: Mar 13 03:54:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 13 02:52:52 2020
Response via : Initial Calibration

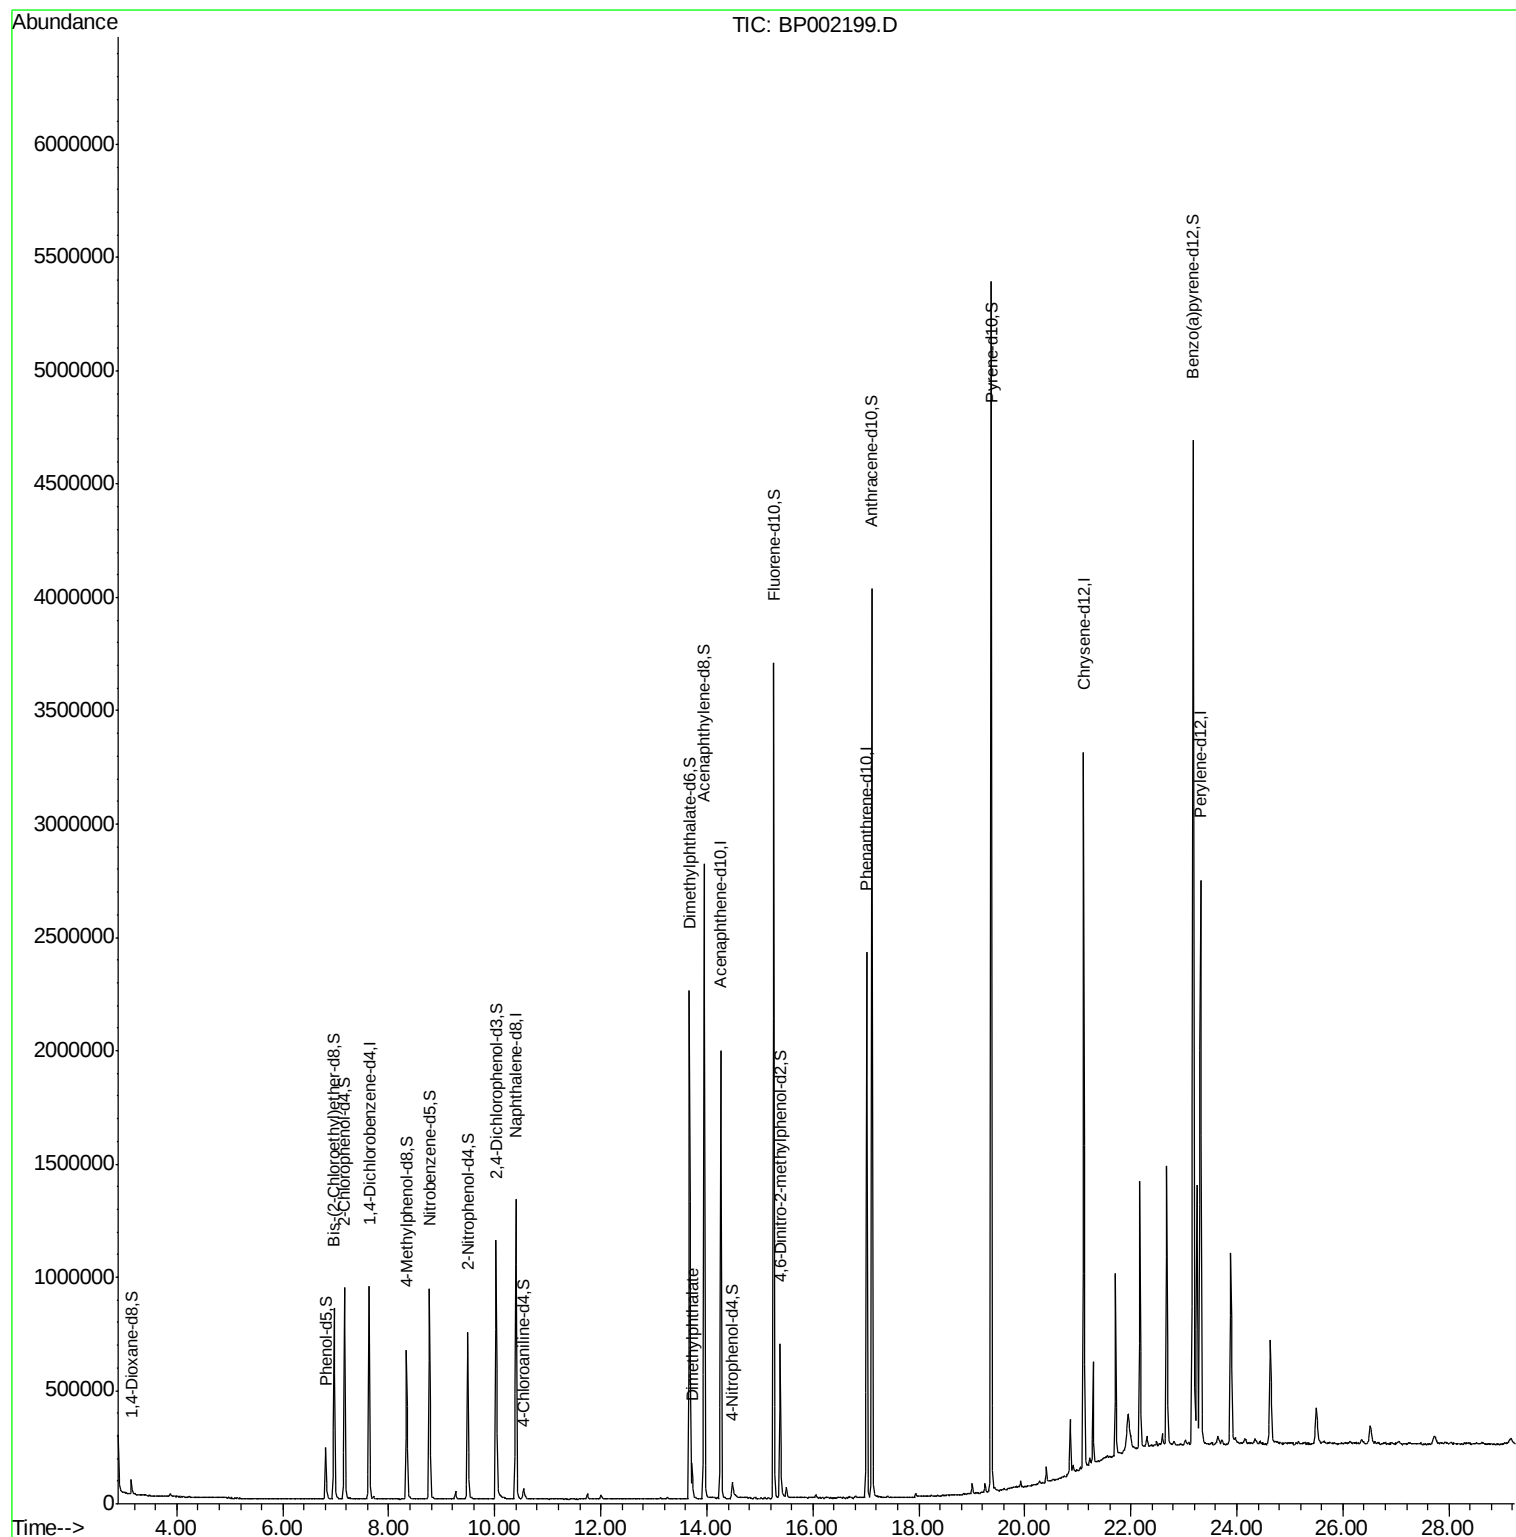

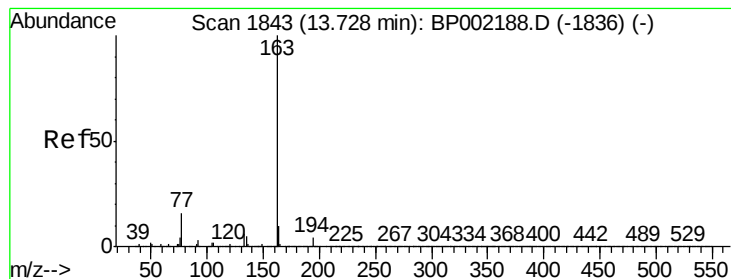

#45

Dimethylphthalate

Concen: 1.925 ng/ul

RT: 13.72 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BP002199.D

Acq: 12 Mar 2020 23:50

Instrument :

BNA_P

ClientSampleId :

C0EQ2


Tot Ion:163 Resp: 103385

Ion Ratio Lower Upper

163 100

194 4.2 3.6 5.4

164 11.1 8.2 12.4

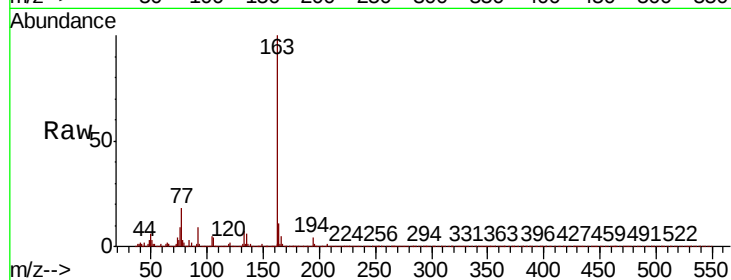

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

