

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
 Data File : BP002177.D
 Acq On : 12 Mar 2020 10:47
 Operator : CG/JU
 Sample : TESTBL-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TESTBL-01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	41	45	54	rVB	59919	87910	1.33%	0.156%
2	3.793	149	154	159	rVB	17435	27028	0.41%	0.048%
3	3.881	165	169	173	rVB2	9140	12969	0.20%	0.023%
4	4.369	247	252	256	rBV4	6533	10971	0.17%	0.020%
5	4.417	256	260	265	rVB2	4995	7200	0.11%	0.013%
6	4.775	316	321	326	rBV	35210	51076	0.77%	0.091%
7	6.811	656	667	679	rBV	839839	1301292	19.63%	2.315%
8	6.969	687	694	708	rVB	677442	1102511	16.63%	1.962%
9	7.163	717	727	743	rBV	927973	1447058	21.82%	2.575%
10	7.281	743	747	752	rVB7	5001	7381	0.11%	0.013%
11	7.628	799	806	817	rBV	705898	1123112	16.94%	1.998%
12	8.334	919	926	939	rBV	1019969	1647348	24.85%	2.931%
13	8.769	992	1000	1010	rBV	738032	1214939	18.32%	2.162%
14	9.487	1114	1122	1139	rBV	592684	987154	14.89%	1.756%
15	10.028	1206	1214	1227	rBV	1013514	1709202	25.78%	3.041%
16	10.399	1268	1277	1290	rBV	968595	1604864	24.21%	2.855%
17	10.534	1292	1300	1318	rBV	956361	1731987	26.12%	3.082%
18	12.004	1545	1550	1560	rBV2	13792	29908	0.45%	0.053%
19	13.681	1827	1835	1849	rBV	1820872	2667955	40.24%	4.747%
20	13.951	1873	1881	1896	rBV	2287368	3317701	50.04%	5.903%
21	14.092	1900	1905	1922	rVB2	22770	68848	1.04%	0.122%
22	14.263	1927	1934	1945	rVB	1515618	2242843	33.83%	3.990%
23	14.475	1961	1970	1993	rBV	530852	1012048	15.26%	1.801%
24	14.692	2004	2007	2014	rVB8	6623	10916	0.16%	0.019%
25	15.263	2097	2104	2117	rBV	3078553	4326407	65.25%	7.697%
26	15.387	2119	2125	2139	rVV	624670	930347	14.03%	1.655%
27	15.504	2141	2145	2159	rVB	37234	60979	0.92%	0.108%
28	16.051	2233	2238	2243	rVB5	11984	17678	0.27%	0.031%
29	16.704	2344	2349	2353	rVB8	6208	8935	0.13%	0.016%
30	16.810	2363	2367	2374	rVB3	8153	12974	0.20%	0.023%
31	17.016	2395	2402	2412	rBV	1945694	2689140	40.56%	4.784%
32	17.116	2412	2419	2437	rVV2	3359737	4850199	73.15%	8.629%
33	19.010	2737	2741	2747	rBV	34757	48995	0.74%	0.087%
34	19.251	2778	2782	2787	rBV	31233	44884	0.68%	0.080%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002177.D
Acq On : 12 Mar 2020 10:47
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TESTBL-01

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Title : SVOA CALIBRATION

35	19.363	2795	2801	2812	rBV	4630118	6027172	90.90%	10.723%
36	21.110	3093	3098	3113	rBV	2529472	3292843	49.66%	5.859%
37	21.716	3199	3201	3205	rVB	59441	57949	0.87%	0.103%
38	22.174	3276	3279	3285	rVB	81480	100627	1.52%	0.179%
39	22.680	3362	3365	3370	rVB	85859	119487	1.80%	0.213%
40	23.174	3442	3449	3457	rBV	3783311	6630299	100.00%	11.797%
41	23.316	3466	3473	3489	rVB	1906993	3562367	53.73%	6.338%


Sum of corrected areas: 56205503

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002177.D
Acq On : 12 Mar 2020 10:47
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TESTBL-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

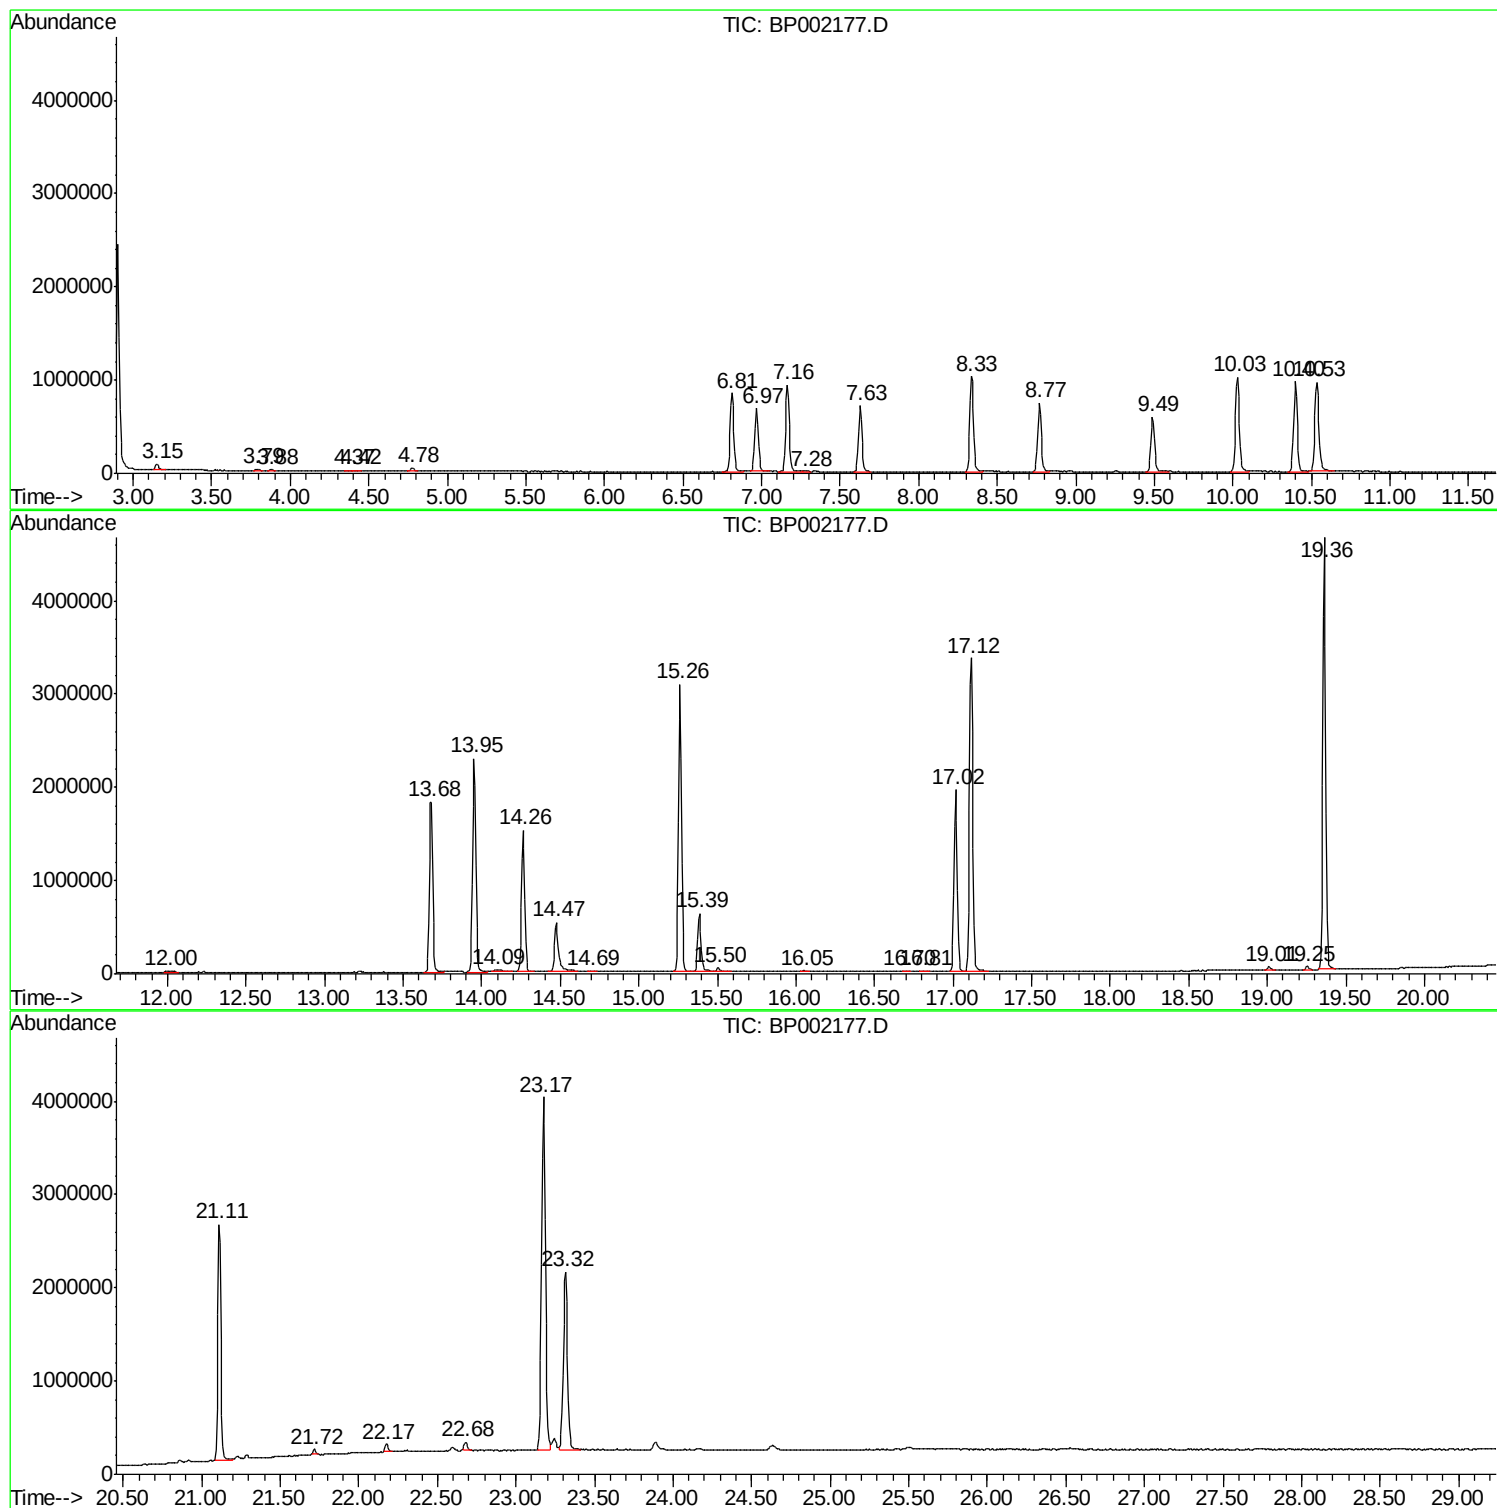

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002177.D
Acq On : 12 Mar 2020 10:47
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TESTBL-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002177.D
Acq On : 12 Mar 2020 10:47
Operator : CG/JU
Sample : TESTBL-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TESTBL-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc