

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
 Data File : BP002193.D
 Acq On : 12 Mar 2020 20:26
 Operator : CG/JU
 Sample : L1786-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	41	45	55	rVB	79129	111786	1.41%	0.141%
2	3.570	112	116	120	rVB5	5772	8772	0.11%	0.011%
3	3.658	127	131	139	rVV	26263	37379	0.47%	0.047%
4	3.793	150	154	158	rVB2	6712	8939	0.11%	0.011%
5	3.876	164	168	174	rVB	14933	22495	0.28%	0.028%
6	4.776	316	321	328	rVB	17750	27721	0.35%	0.035%
7	5.717	475	481	487	rVB	12044	19781	0.25%	0.025%
8	6.311	577	582	591	rVB	3899	9110	0.11%	0.011%
9	6.811	660	667	680	rBV	1192215	1904859	23.99%	2.404%
10	6.964	682	693	707	rVV	991945	1604425	20.21%	2.024%
11	7.164	719	727	737	rBV	1336092	2079731	26.19%	2.624%
12	7.628	798	806	815	rBV	1001881	1631660	20.55%	2.059%
13	7.711	815	820	827	rVB	16522	26589	0.33%	0.034%
14	8.334	919	926	943	rBV	1418369	2254614	28.40%	2.845%
15	8.769	992	1000	1013	rBV	1104917	1795702	22.62%	2.266%
16	9.252	1077	1082	1089	rVB	24161	38333	0.48%	0.048%
17	9.487	1114	1122	1132	rBV	894241	1432983	18.05%	1.808%
18	10.028	1206	1214	1227	rBV	1470045	2526641	31.82%	3.188%
19	10.399	1268	1277	1283	rBV	1426995	2375432	29.92%	2.997%
20	10.446	1283	1285	1292	rVV	24585	34199	0.43%	0.043%
21	10.534	1292	1300	1326	rVV	1359906	2487790	31.33%	3.139%
22	11.999	1543	1549	1557	rBV2	23470	44805	0.56%	0.057%
23	12.069	1557	1561	1568	rVB2	5772	10045	0.13%	0.013%
24	12.287	1593	1598	1607	rVB6	6447	12708	0.16%	0.016%
25	13.116	1732	1739	1744	rBV8	9476	17762	0.22%	0.022%
26	13.181	1744	1750	1754	rBV5	5668	10097	0.13%	0.013%
27	13.681	1824	1835	1839	rBV	2466492	3542380	44.62%	4.470%
28	13.722	1839	1842	1850	rVB	518887	704949	8.88%	0.890%
29	13.951	1874	1881	1894	rBV	3304894	4723162	59.49%	5.960%
30	14.199	1919	1923	1927	rBV5	8120	10936	0.14%	0.014%
31	14.263	1927	1934	1941	rVV2	2178625	3209737	40.43%	4.050%
32	14.328	1941	1945	1954	rVB2	24712	42692	0.54%	0.054%
33	14.469	1963	1969	1992	rBV	757730	1329077	16.74%	1.677%
34	15.263	2097	2104	2111	rBV	4162247	5867597	73.90%	7.404%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
 Data File : BP002193.D
 Acq On : 12 Mar 2020 20:26
 Operator : CG/JU
 Sample : L1786-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

35	15.316	2111	2113	2119	rVB	16546	21057	0.27%	0.027%
36	15.387	2119	2125	2138	rBV	709308	1048738	13.21%	1.323%
37	15.504	2140	2145	2150	rVB2	42869	66443	0.84%	0.084%
38	15.763	2185	2189	2197	rVB5	7573	13032	0.16%	0.016%
39	15.987	2224	2227	2230	rBV2	7378	9803	0.12%	0.012%
40	16.051	2234	2238	2244	rVB3	19062	30395	0.38%	0.038%
41	16.575	2321	2327	2336	rBV	30107	48814	0.61%	0.062%
42	16.698	2346	2348	2352	rVB5	9398	10340	0.13%	0.013%
43	16.804	2362	2366	2375	rVB3	14384	27492	0.35%	0.035%
44	17.016	2395	2402	2407	rBV	2655937	3776199	47.56%	4.765%
45	17.051	2407	2408	2412	rVV	45864	52223	0.66%	0.066%
46	17.116	2412	2419	2430	rVV	4206254	6023270	75.86%	7.600%
47	17.222	2433	2437	2444	rVB8	18513	32761	0.41%	0.041%
48	17.381	2460	2464	2469	rBV6	10256	24611	0.31%	0.031%
49	17.428	2470	2472	2477	rVB6	10635	15243	0.19%	0.019%
50	17.934	2554	2558	2566	rBV3	49727	83464	1.05%	0.105%
51	18.081	2579	2583	2588	rBV	16340	25300	0.32%	0.032%
52	18.234	2605	2609	2613	rBV7	9073	14767	0.19%	0.019%
53	18.357	2626	2630	2632	rBV2	28802	35109	0.44%	0.044%
54	18.781	2698	2702	2707	rBV7	26553	44675	0.56%	0.056%
55	19.004	2736	2740	2742	rBV	51517	66224	0.83%	0.084%
56	19.039	2742	2746	2752	rVB	130572	176688	2.23%	0.223%
57	19.251	2778	2782	2790	rVB	46807	66449	0.84%	0.084%
58	19.322	2790	2794	2795	rBV2	49526	47430	0.60%	0.060%
59	19.363	2795	2801	2816	rVB	5609017	7818222	98.47%	9.865%
60	19.881	2885	2889	2894	rVB3	25622	33180	0.42%	0.042%
61	19.975	2902	2905	2908	rVB2	22083	25189	0.32%	0.032%
62	20.339	2964	2967	2971	rBV3	32121	34073	0.43%	0.043%
63	20.851	3049	3054	3061	rBV	472234	730051	9.19%	0.921%
64	21.110	3092	3098	3103	rBV	3662542	4644175	58.49%	5.860%
65	21.286	3125	3128	3132	rVB	64498	66937	0.84%	0.084%
66	21.716	3197	3201	3211	rBV4	103260	177778	2.24%	0.224%
67	22.175	3276	3279	3284	rVB	128058	149644	1.88%	0.189%
68	22.298	3296	3300	3306	rVB	238689	306624	3.86%	0.387%
69	22.675	3360	3364	3377	rVB2	219426	446160	5.62%	0.563%
70	23.175	3442	3449	3457	rBV	4496243	7939668	100.00%	10.018%
71	23.316	3466	3473	3488	rVB	2648383	4862792	61.25%	6.136%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002193.D
Acq On : 12 Mar 2020 20:26
Operator : CG/JU
Sample : L1786-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Title : SVOA CALIBRATION

72	23.886	3565	3570	3578	rbV	163085	291942	3.68%	0.368%
----	--------	------	------	------	-----	--------	--------	-------	--------


Sum of corrected areas: 79251850

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002193.D
Acq On : 12 Mar 2020 20:26
Operator : CG/JU
Sample : L1786-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

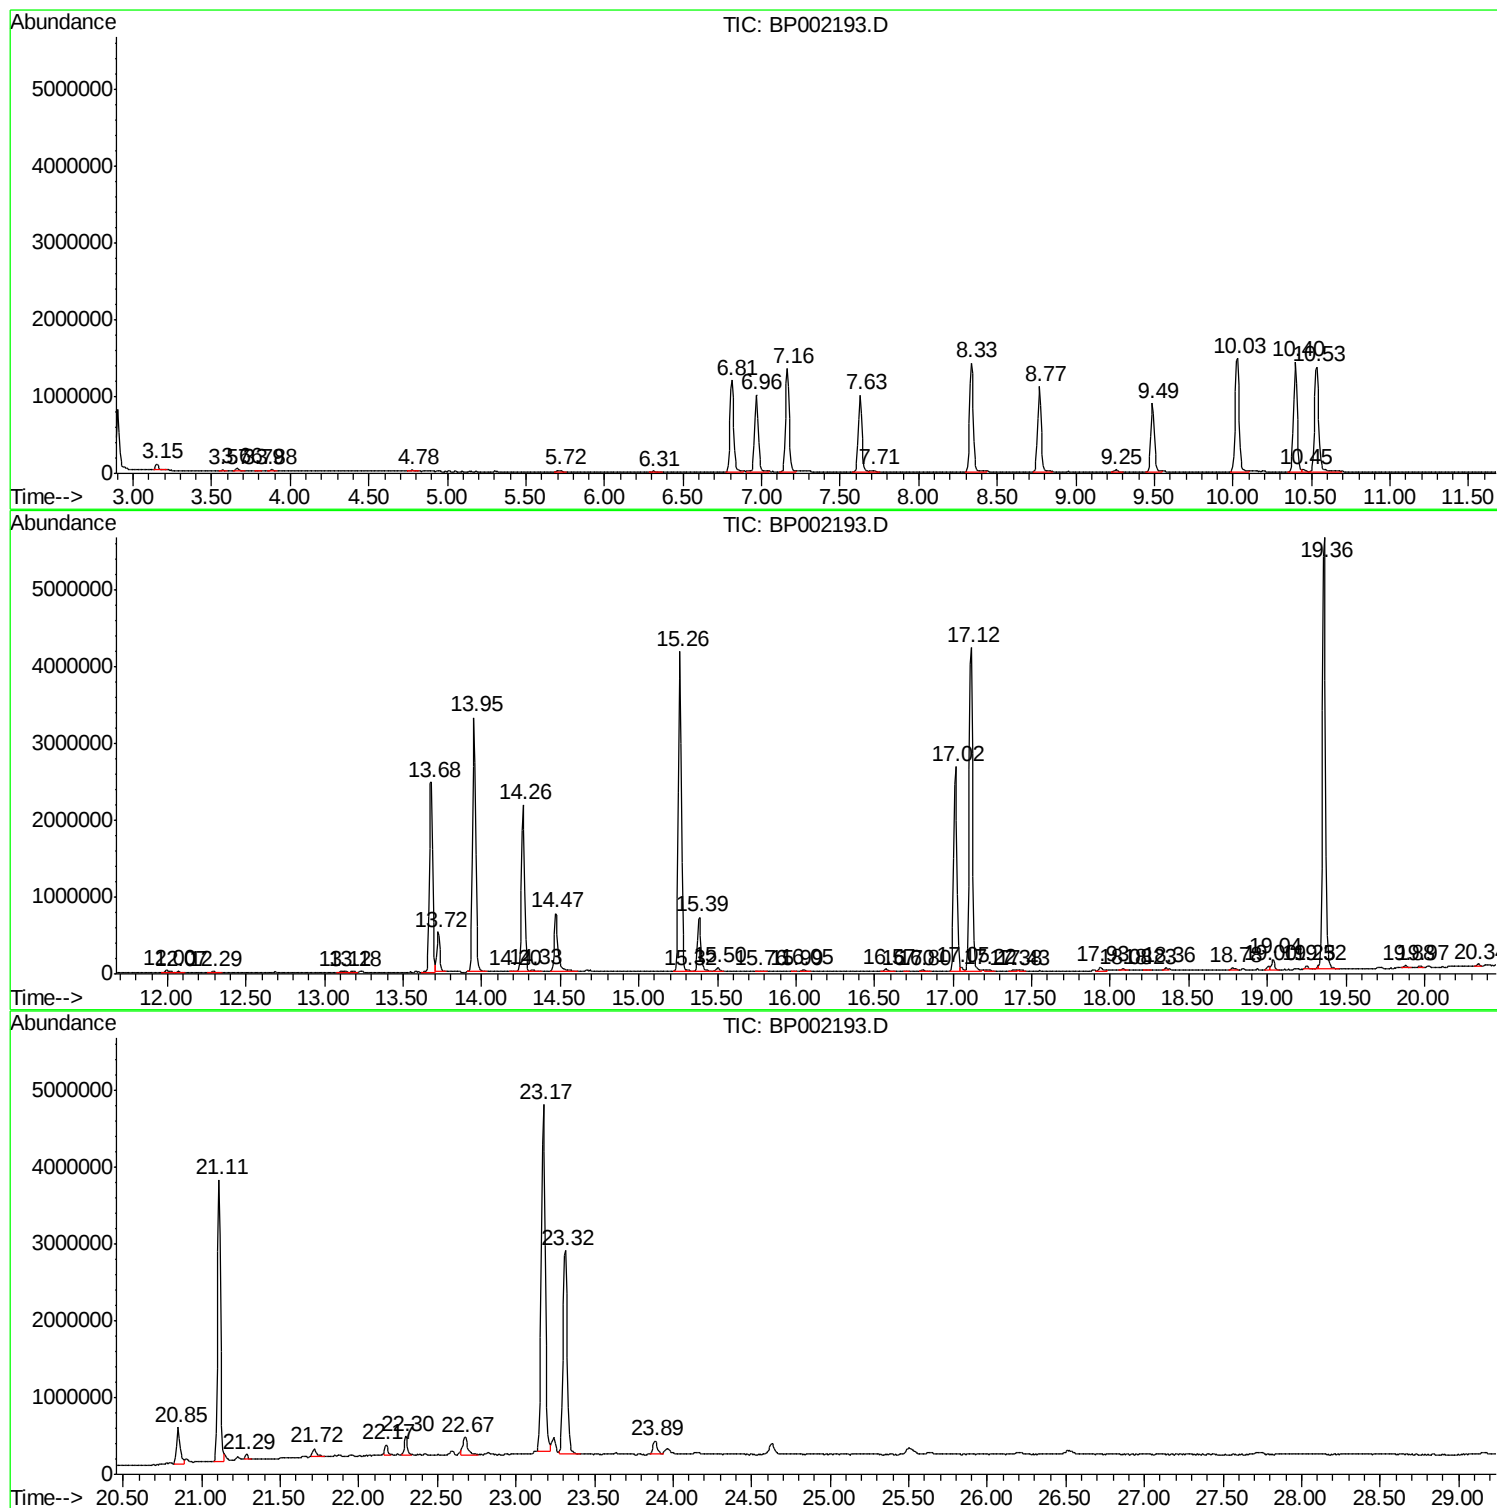

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
Data File : BP002193.D
Acq On : 12 Mar 2020 20:26
Operator : CG/JU
Sample : L1786-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB9










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentafluoropropionic acid, ... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.85	3.14 ng/ul	730051	Chrysene-d12	21.11

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
2		Behenic alcohol	326	C22H46O	000661-19-8	94
3		2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	94
4		1-Heneicosanol	312	C21H44O	015594-90-8	94
5		Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94

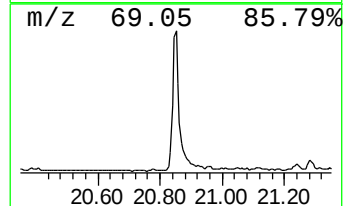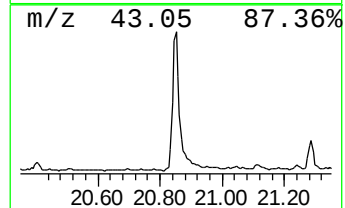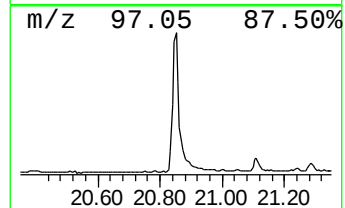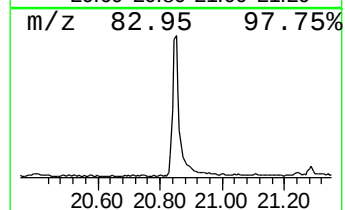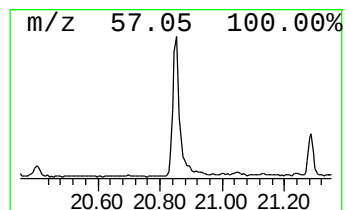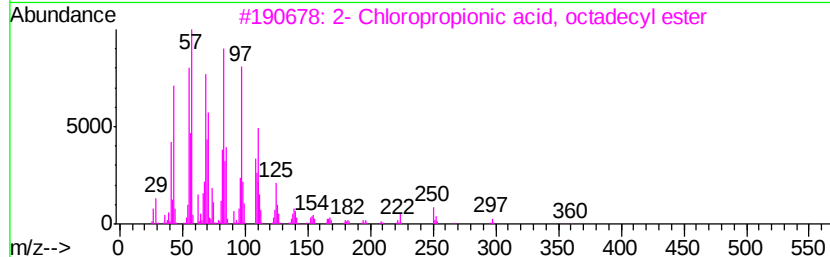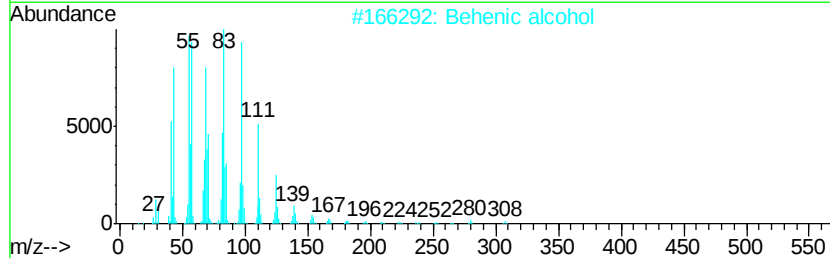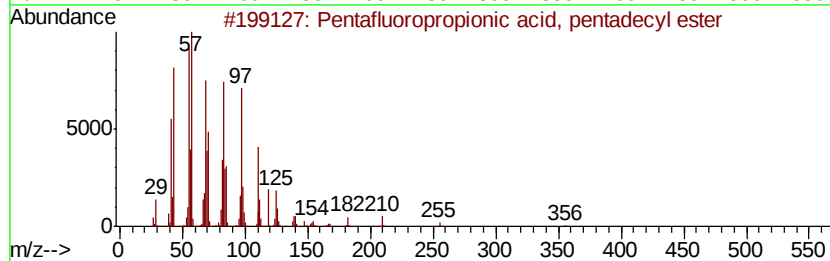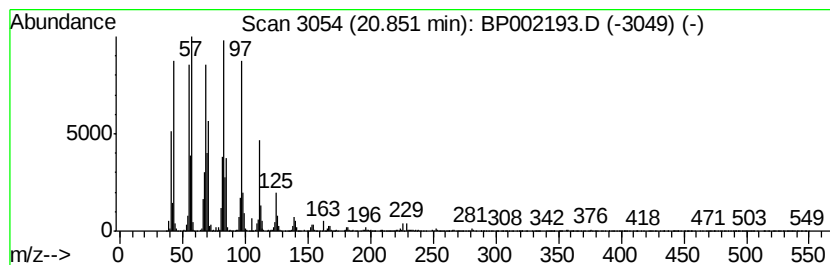

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002193.D
Acq On : 12 Mar 2020 20:26
Operator : CG/JU
Sample : L1786-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentafluoropropio...	20.85	3.1	ng/ul	730051	5	21.11	4644180	20.0