

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
 Data File : BP002196.D
 Acq On : 12 Mar 2020 22:08
 Operator : CG/JU
 Sample : L1899-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0EP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	41	44	48	rBV	56687	66646	0.75%	0.083%
2	3.875	164	168	174	rBV	24407	33807	0.38%	0.042%
3	4.099	201	206	211	rBV3	27122	41745	0.47%	0.052%
4	4.505	271	275	281	rBV2	14949	20781	0.24%	0.026%
5	6.811	661	667	680	rBV	194175	336691	3.81%	0.419%
6	6.963	687	693	708	rBV	694703	1117992	12.66%	1.391%
7	7.163	720	727	740	rBV	781328	1248591	14.14%	1.554%
8	7.628	798	806	816	rBV	1762883	2857099	32.35%	3.556%
9	7.705	816	819	828	rVB	12572	21686	0.25%	0.027%
10	8.334	920	926	946	rBV	553522	923110	10.45%	1.149%
11	8.769	992	1000	1016	rBV	806537	1316633	14.91%	1.638%
12	9.257	1076	1083	1089	rBV	55336	87921	1.00%	0.109%
13	9.487	1113	1122	1132	rBV	624194	1033969	11.71%	1.287%
14	10.028	1206	1214	1236	rBV	978678	1755393	19.88%	2.185%
15	10.399	1268	1277	1291	rBV	2500342	4127153	46.74%	5.136%
16	10.546	1294	1302	1311	rBV	38690	89693	1.02%	0.112%
17	11.746	1500	1506	1513	rBV2	16347	26621	0.30%	0.033%
18	11.998	1542	1549	1558	rBV	16664	33856	0.38%	0.042%
19	12.910	1697	1704	1710	rBV10	4114	10646	0.12%	0.013%
20	13.116	1735	1739	1743	rBV6	7233	9764	0.11%	0.012%
21	13.675	1827	1834	1839	rBV	2028268	2863810	32.43%	3.564%
22	13.722	1839	1842	1850	rVB	231673	325256	3.68%	0.405%
23	13.951	1873	1881	1895	rBV	2321835	3496539	39.59%	4.351%
24	14.198	1918	1923	1927	rBV5	8275	11653	0.13%	0.015%
25	14.263	1927	1934	1950	rVB	3860907	5528709	62.61%	6.880%
26	14.481	1964	1971	1987	rBV	90818	233719	2.65%	0.291%
27	15.263	2097	2104	2119	rBV	3347180	4758736	53.89%	5.922%
28	15.381	2119	2124	2136	rVV	730528	1094910	12.40%	1.363%
29	15.504	2140	2145	2152	rVB	37119	59016	0.67%	0.073%
30	15.869	2202	2207	2212	rVB7	7663	14905	0.17%	0.019%
31	16.045	2234	2237	2244	rVB2	14934	21938	0.25%	0.027%
32	16.334	2282	2286	2290	rBV7	6380	9916	0.11%	0.012%
33	16.528	2315	2319	2325	rVB3	20170	28507	0.32%	0.035%
34	16.698	2344	2348	2354	rVB6	7358	11904	0.13%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP031220\
 Data File : BP002196.D
 Acq On : 12 Mar 2020 22:08
 Operator : CG/JU
 Sample : L1899-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0EP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Title : SVOA CALIBRATION

35	16.804	2361	2366	2373	rVB	23193	40380	0.46%	0.050%
36	17.016	2395	2402	2412	rBV	4484362	6409382	72.58%	7.976%
37	17.116	2412	2419	2430	rVV	4004216	5924302	67.09%	7.373%
38	17.275	2442	2446	2456	rVB6	25594	38262	0.43%	0.048%
39	17.422	2464	2471	2482	rVB3	54441	84502	0.96%	0.105%
40	17.933	2554	2558	2563	rBV3	29479	42970	0.49%	0.053%
41	18.357	2626	2630	2634	rBV2	30514	36506	0.41%	0.045%
42	18.580	2665	2668	2671	rBV3	11760	14718	0.17%	0.018%
43	18.622	2671	2675	2680	rVB3	29188	34563	0.39%	0.043%
44	19.004	2736	2740	2747	rBV2	47601	68079	0.77%	0.085%
45	19.251	2778	2782	2788	rVB	43144	58928	0.67%	0.073%
46	19.363	2795	2801	2815	rVB	5334209	7215034	81.70%	8.979%
47	19.922	2893	2896	2900	rBV	38984	39900	0.45%	0.050%
48	20.857	3050	3055	3059	rBV	297677	376505	4.26%	0.469%
49	21.110	3093	3098	3106	rBV	6207717	7575514	85.78%	9.427%
50	21.227	3115	3118	3123	rVB	37970	48670	0.55%	0.061%
51	21.716	3197	3201	3204	rBV	135774	171772	1.95%	0.214%
52	22.174	3275	3279	3284	rVB	115669	147304	1.67%	0.183%
53	22.298	3296	3300	3306	rVB	435039	550500	6.23%	0.685%
54	22.674	3360	3364	3370	rBV	173065	226341	2.56%	0.282%
55	23.174	3441	3449	3456	rBV	4678430	8244120	93.36%	10.259%
56	23.239	3457	3460	3465	rVV	189702	300505	3.40%	0.374%
57	23.316	3465	3473	3491	rVB	4703670	8830843	100.00%	10.990%
58	23.886	3565	3570	3575	rBV2	147944	257791	2.92%	0.321%


Sum of corrected areas: 80356706

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002196.D
Acq On : 12 Mar 2020 22:08
Operator : CG/JU
Sample : L1899-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EP7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

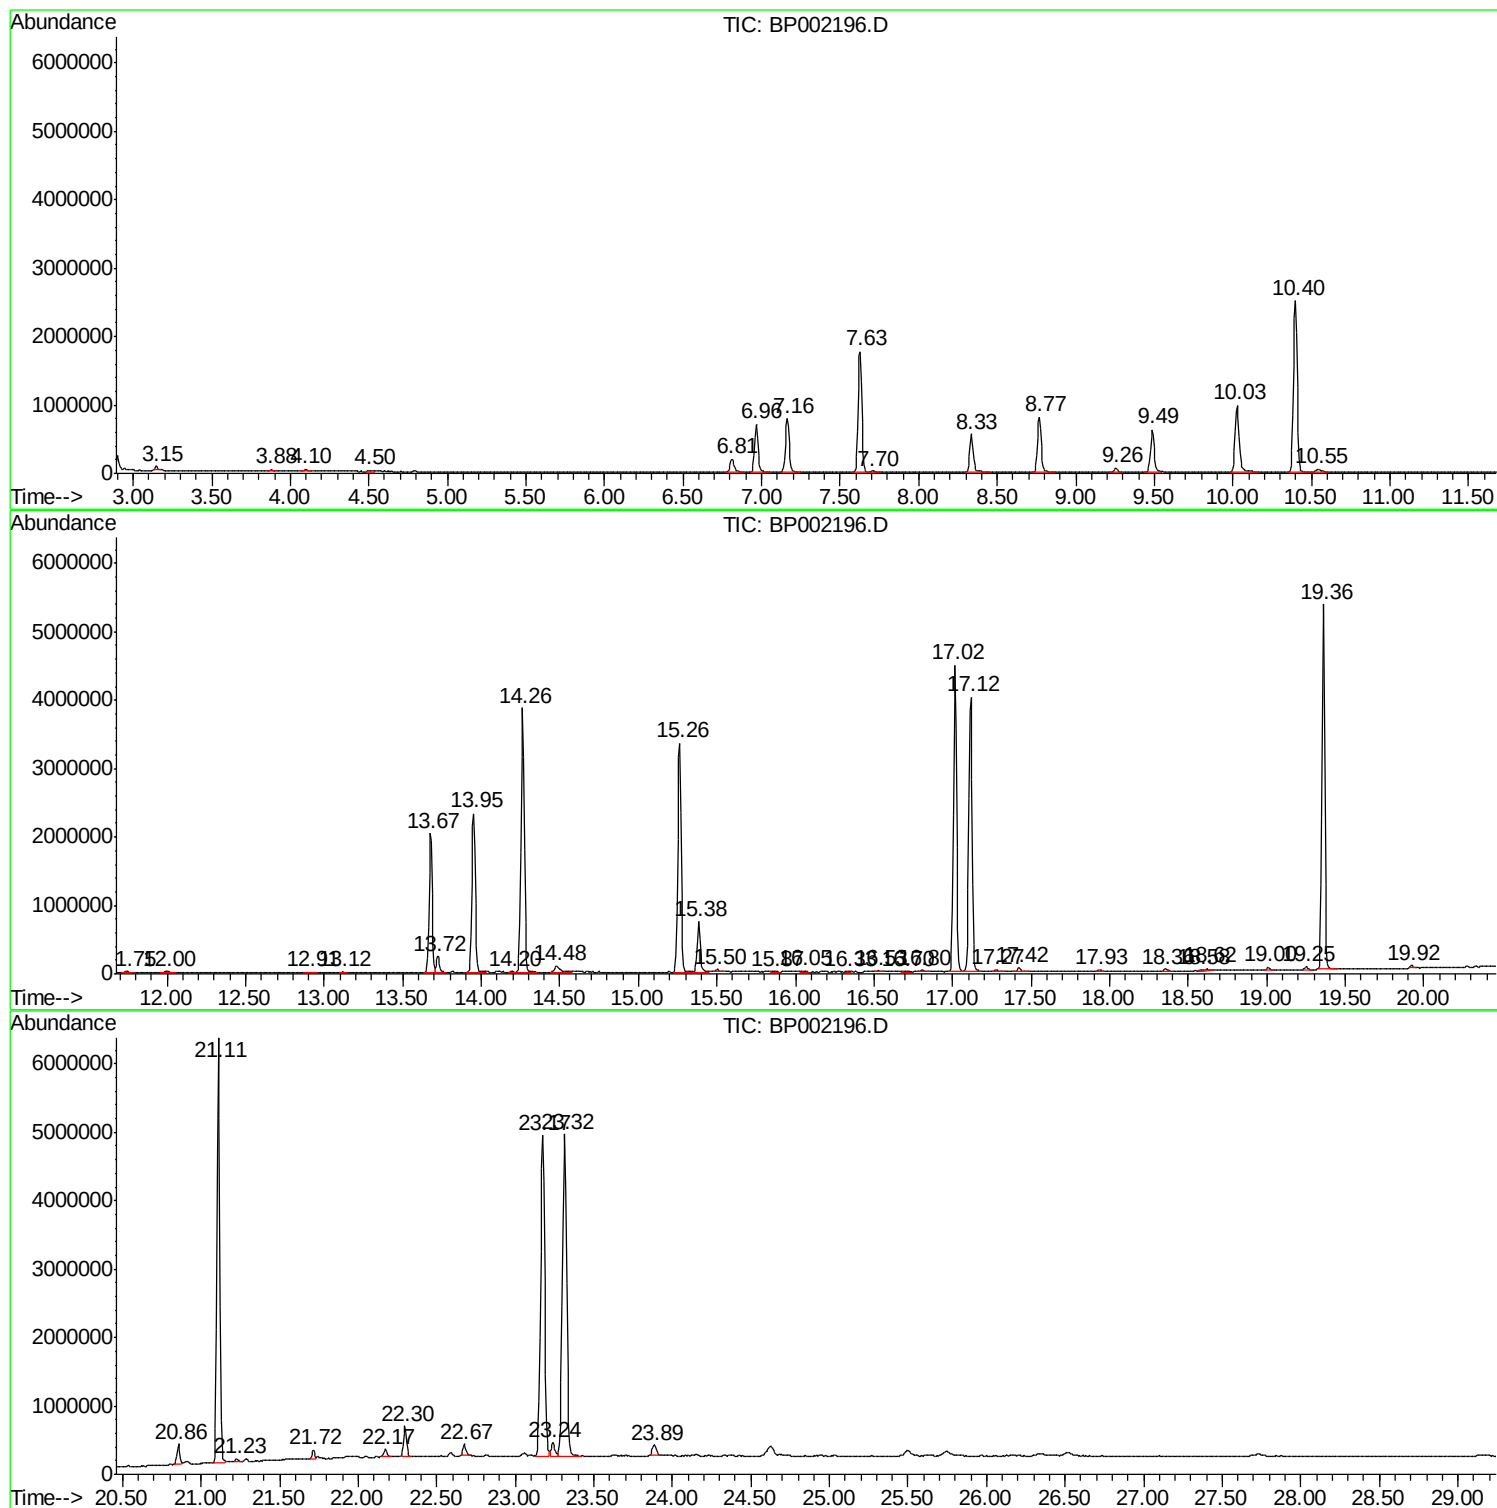

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002196.D
Acq On : 12 Mar 2020 22:08
Operator : CG/JU
Sample : L1899-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EP7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031220\
Data File : BP002196.D
Acq On : 12 Mar 2020 22:08
Operator : CG/JU
Sample : L1899-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0EP7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc