
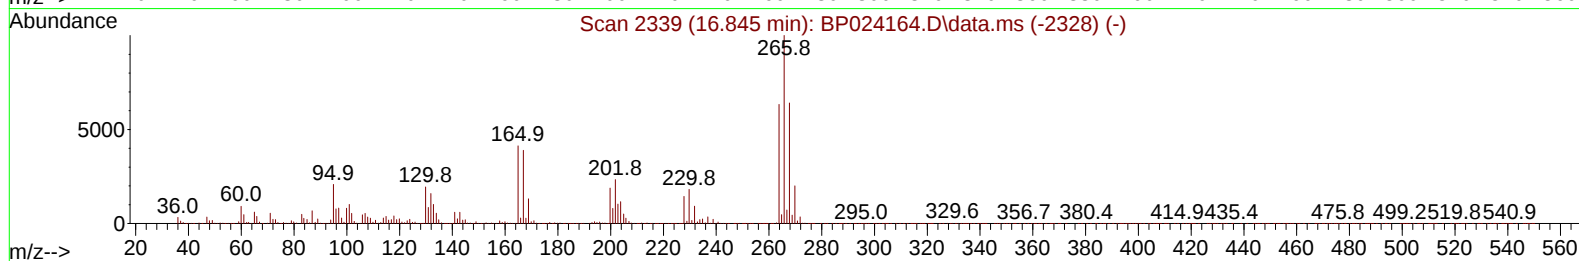
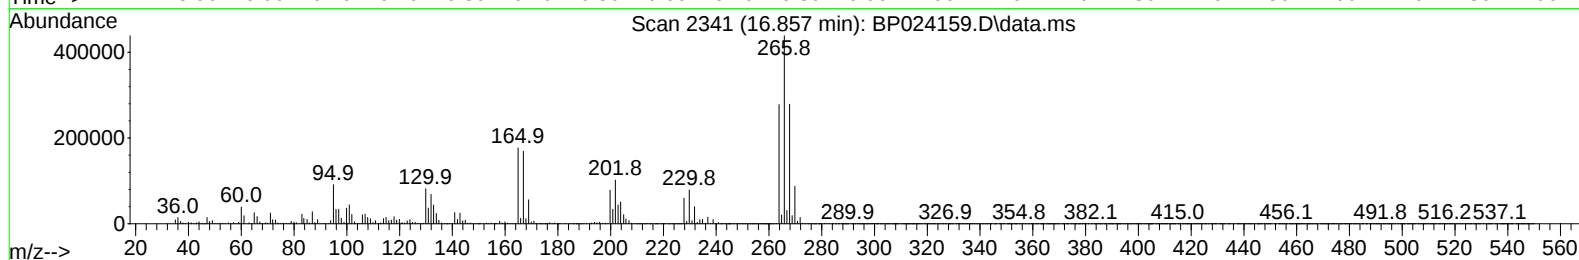


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024159.D
Acq On : 12 Mar 2025 15:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 05:56:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

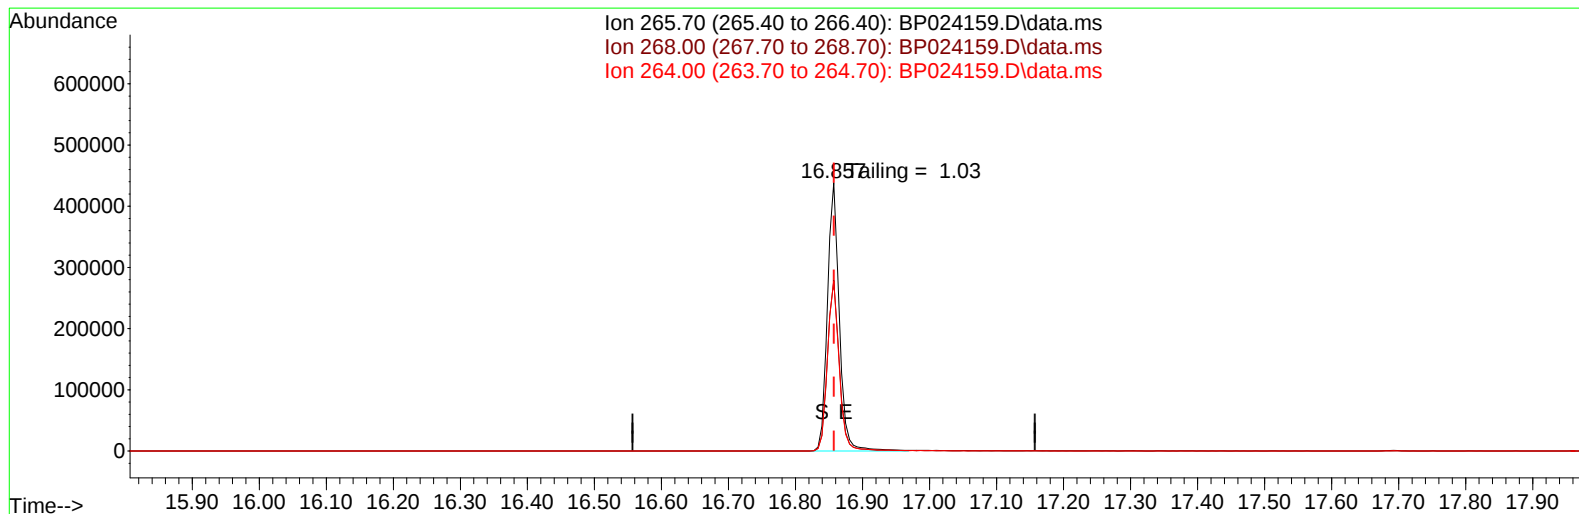

TIC: BP024159.D\data.ms

(70) Pentachlorophenol (C)




16.857min (0.000) 4607317.61 ng

response 542052

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.56
264.00	63.30	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024159.D
Acq On : 12 Mar 2025 15:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 05:56:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

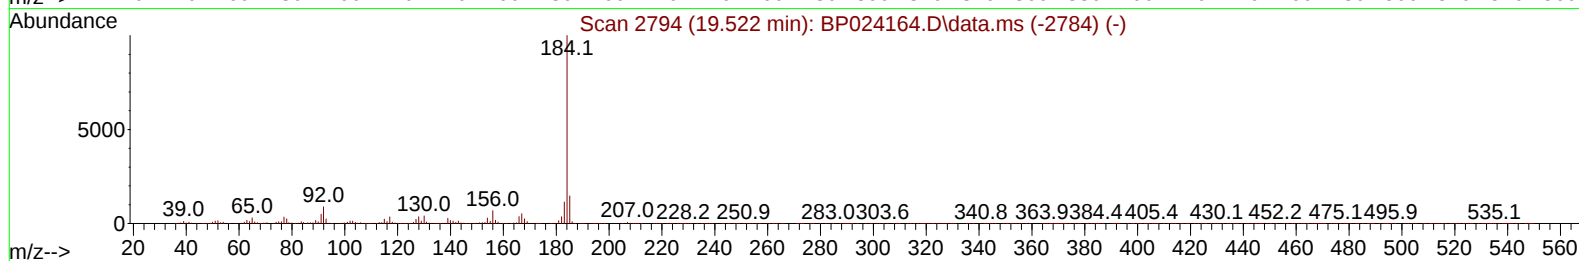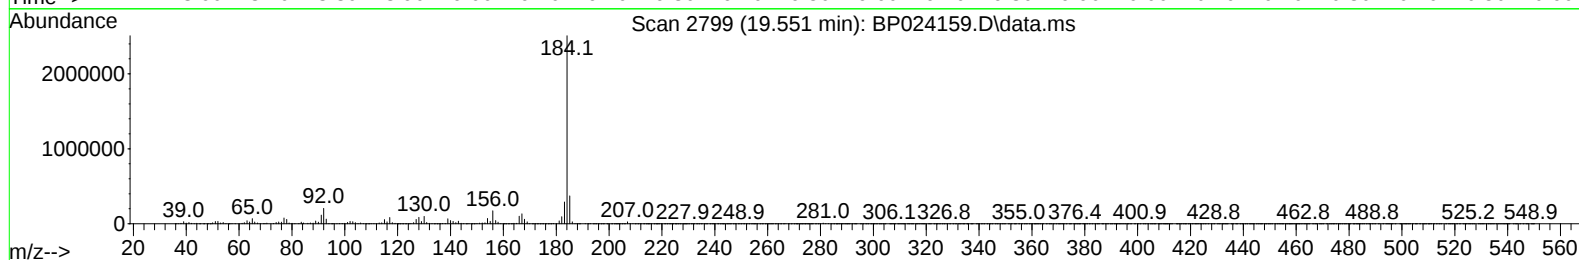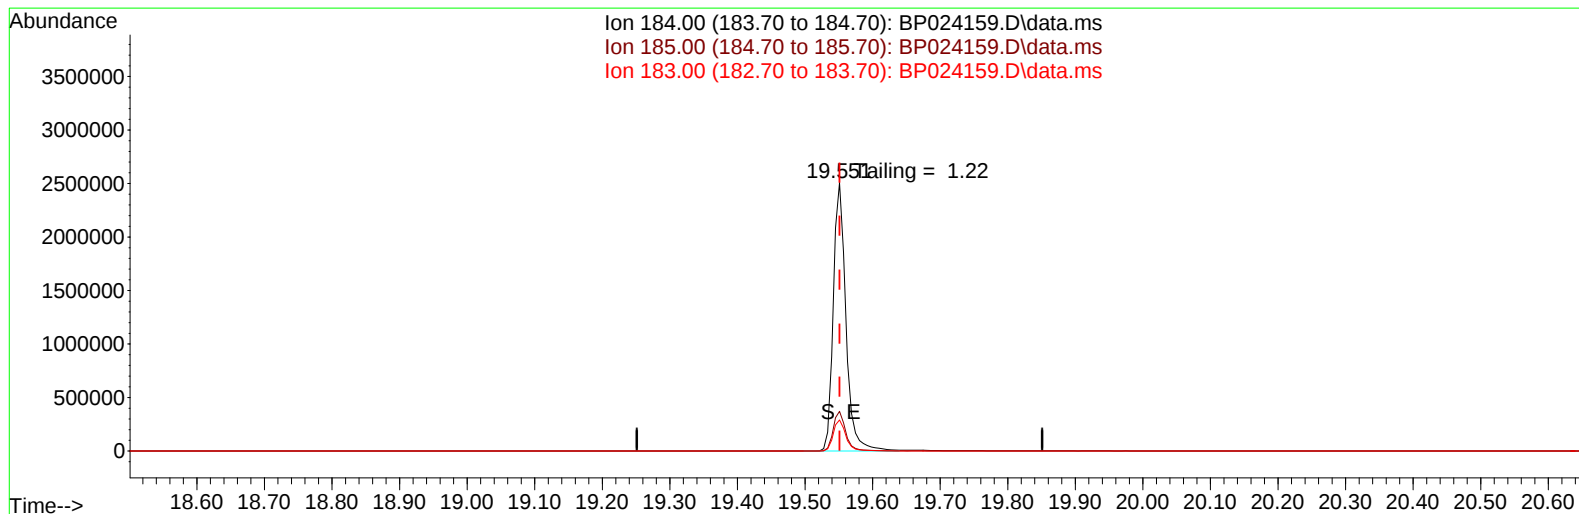

TIC: BP024159.D\data.ms

(77) Benzidine**19.551min (0.000) 3117449.49 ng****response 3272103**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.81
183.00	11.40	11.59
0.00	0.00	0.00