

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024169.D
Acq On : 12 Mar 2025 22:24
Operator : RC/JU
Sample : PB167078BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167078BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	384	390	405	rBV	6177172	8876877	42.05%	9.978%
2	6.952	649	657	676	rBV	5923830	9045559	42.85%	10.167%
3	7.769	787	796	806	rBV	1183572	1838992	8.71%	2.067%
4	8.922	984	992	1009	rBV	3444145	5629012	26.67%	6.327%
5	10.552	1261	1269	1285	rBV	1524708	2568048	12.17%	2.887%
6	13.016	1680	1688	1700	rBV	9777687	13674177	64.78%	15.370%
7	14.404	1917	1924	1939	rBV	2370203	3388468	16.05%	3.809%
8	15.916	2172	2181	2209	rBV	6630167	10106992	47.88%	11.361%
9	17.204	2393	2400	2412	rBV2	2715358	3939537	18.66%	4.428%
10	19.928	2857	2863	2876	rBV	15558754	21109034	100.00%	23.727%
11	21.657	3151	3157	3168	rBV2	2747083	4320627	20.47%	4.857%
12	25.069	3729	3737	3752	rVB	1662243	4468383	21.17%	5.023%




Sum of corrected areas: 88965706

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024169.D
Acq On : 12 Mar 2025 22:24
Operator : RC/JU
Sample : PB167078BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167078BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

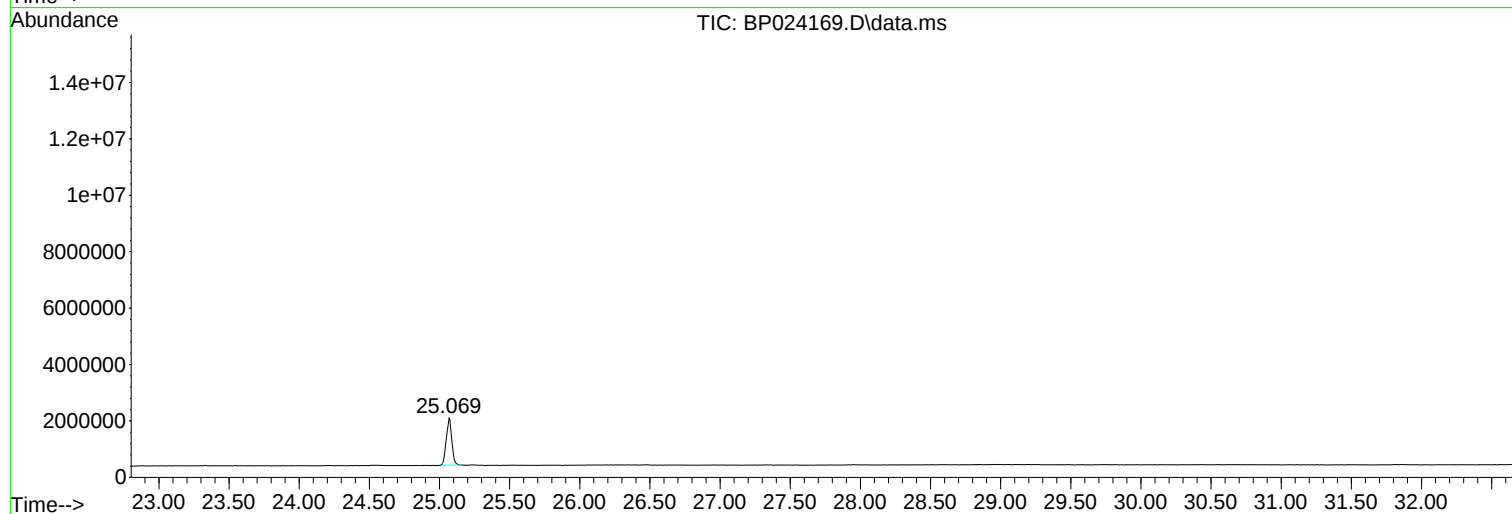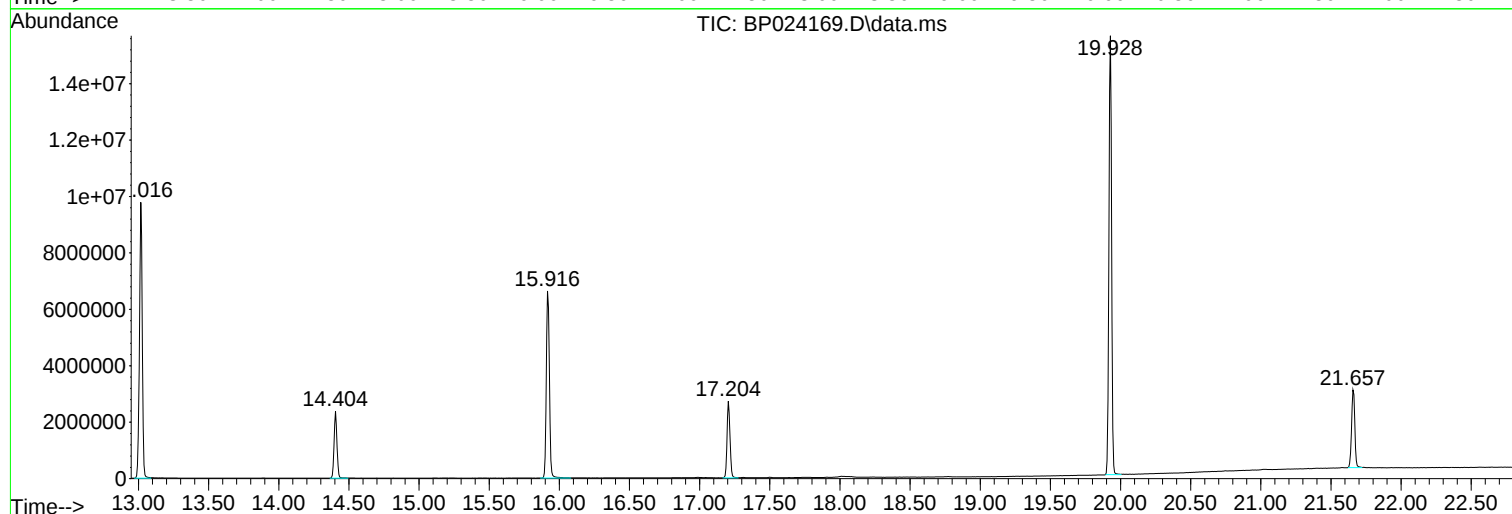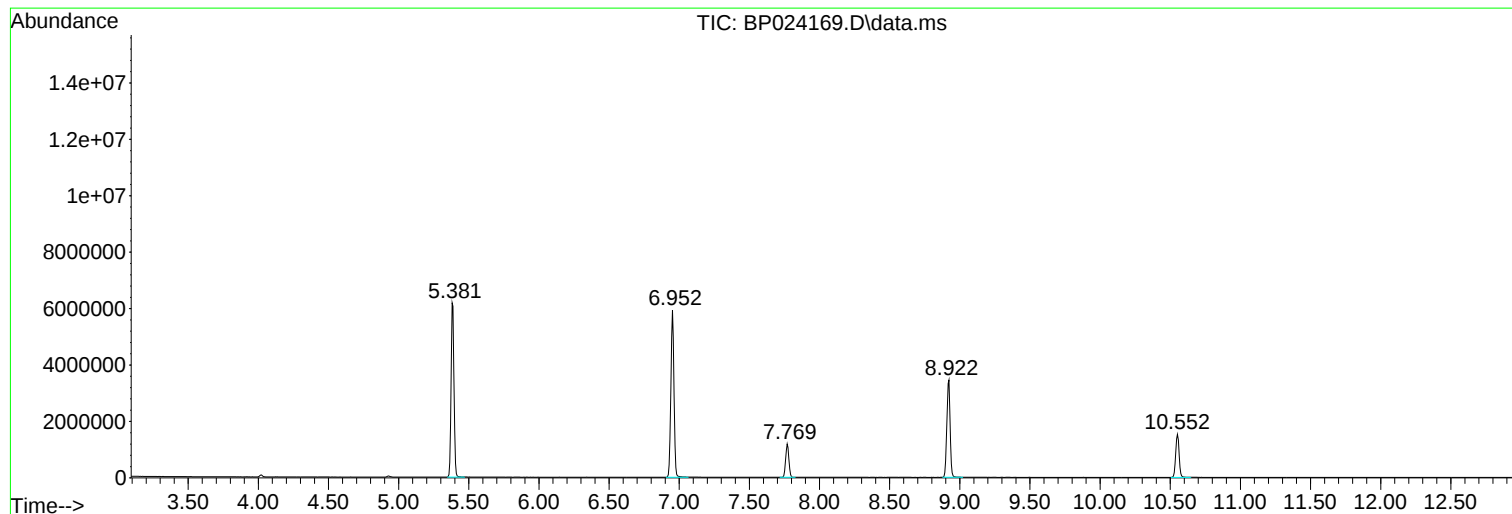

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024169.D
Acq On : 12 Mar 2025 22:24
Operator : RC/JU
Sample : PB167078BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167078BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024169.D
Acq On : 12 Mar 2025 22:24
Operator : RC/JU
Sample : PB167078BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167078BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------