
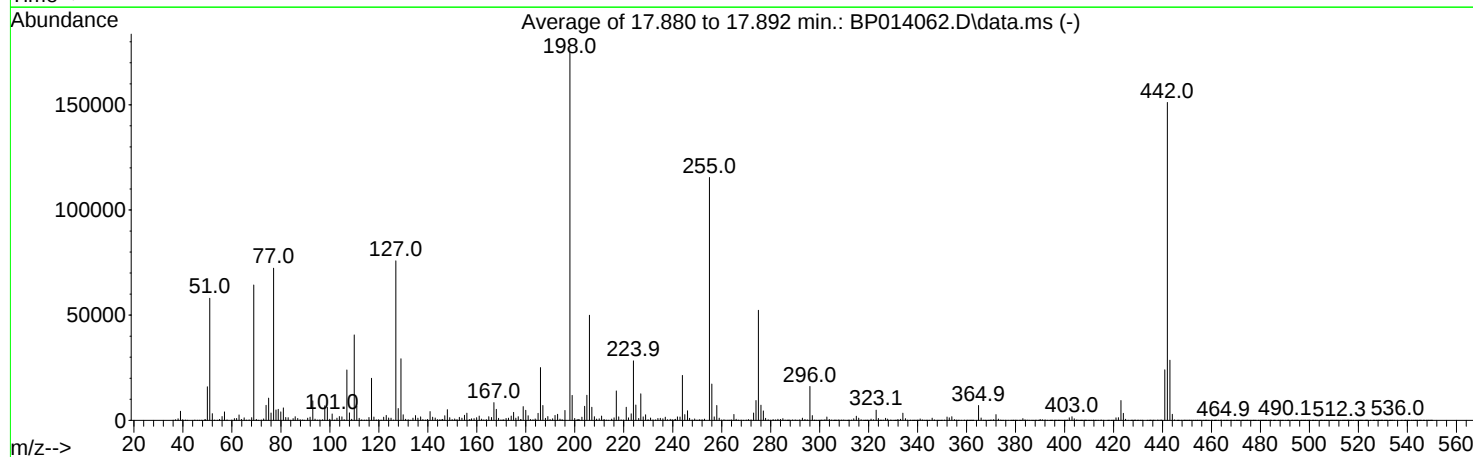


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031323\
 Data File : BP014062.D
 Acq On : 13 Mar 2023 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 14 04:15:47 2023

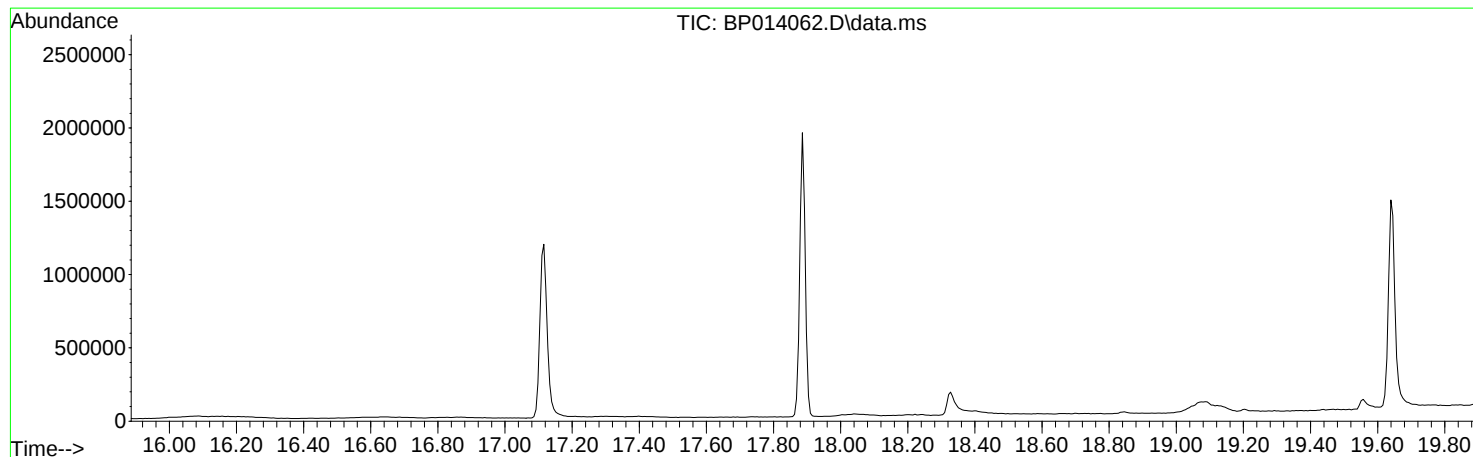




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	58015	PASS
68	69	0.00	2	2.0	1263	PASS
69	198	0.00	100	36.8	64357	PASS
70	69	0.00	2	0.6	416	PASS
127	198	10	80	43.4	75838	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	174921	PASS
199	198	5	9	6.8	11837	PASS
275	198	10	60	29.9	52325	PASS
365	198	1	100	4.0	7017	PASS
441	198	0.01	100	13.7	24039	PASS
442	442	100	100	100.0	151154	PASS
443	442	15	24	18.9	28590	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031323\
Data File : BP014062.D
Acq On : 13 Mar 2023 09:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 14 06:27:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 04:15:47 2023
Response via : Initial Calibration

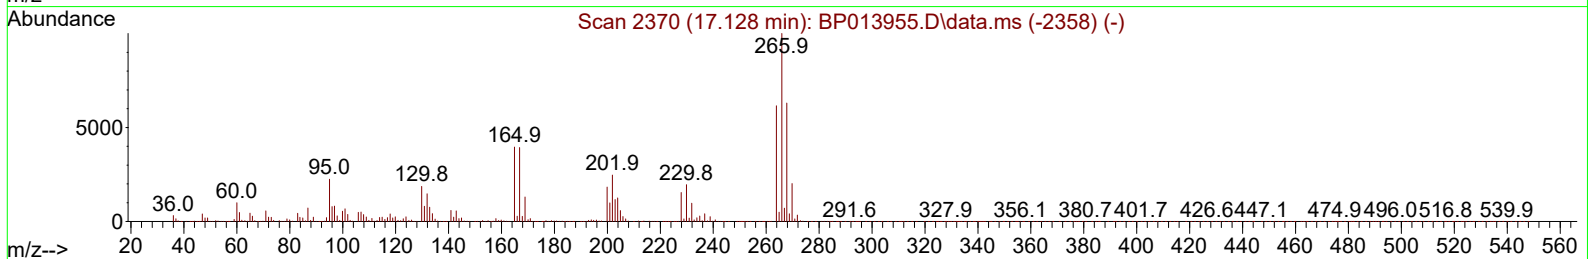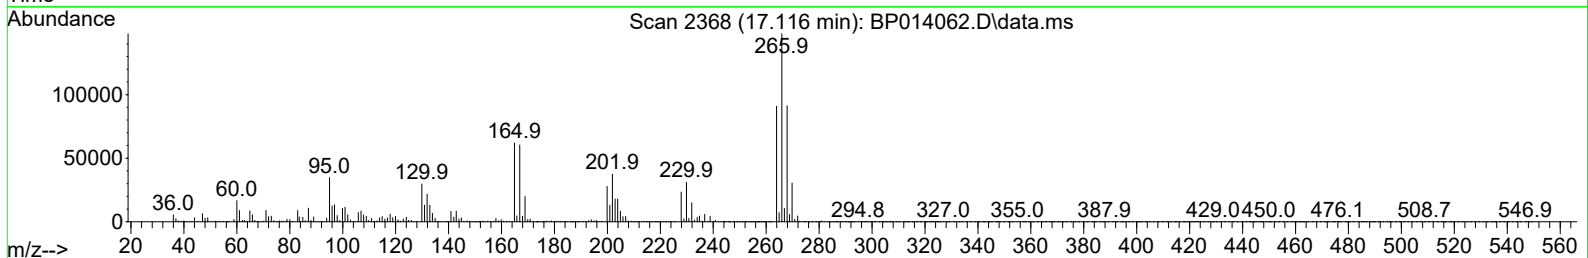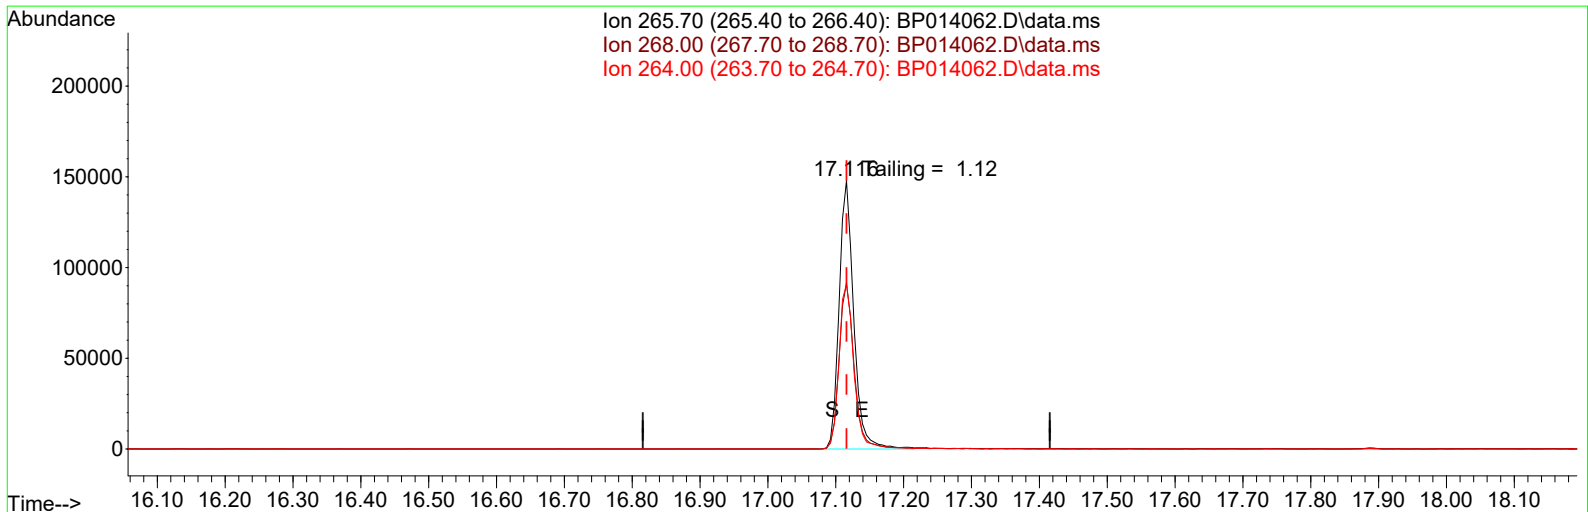

TIC: BP014062.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.000) 897726.13 ng




response 220311

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.69
264.00	61.50	61.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031323\
Data File : BP014062.D
Acq On : 13 Mar 2023 09:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 14 06:27:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 04:15:47 2023
Response via : Initial Calibration

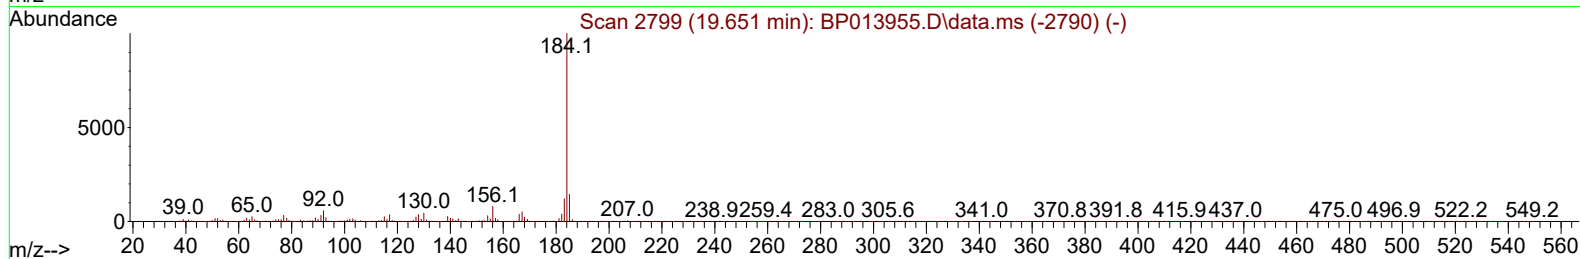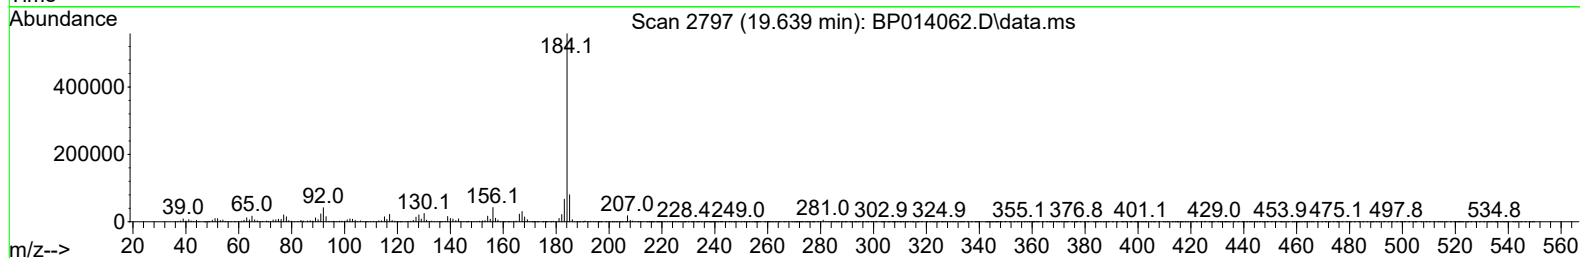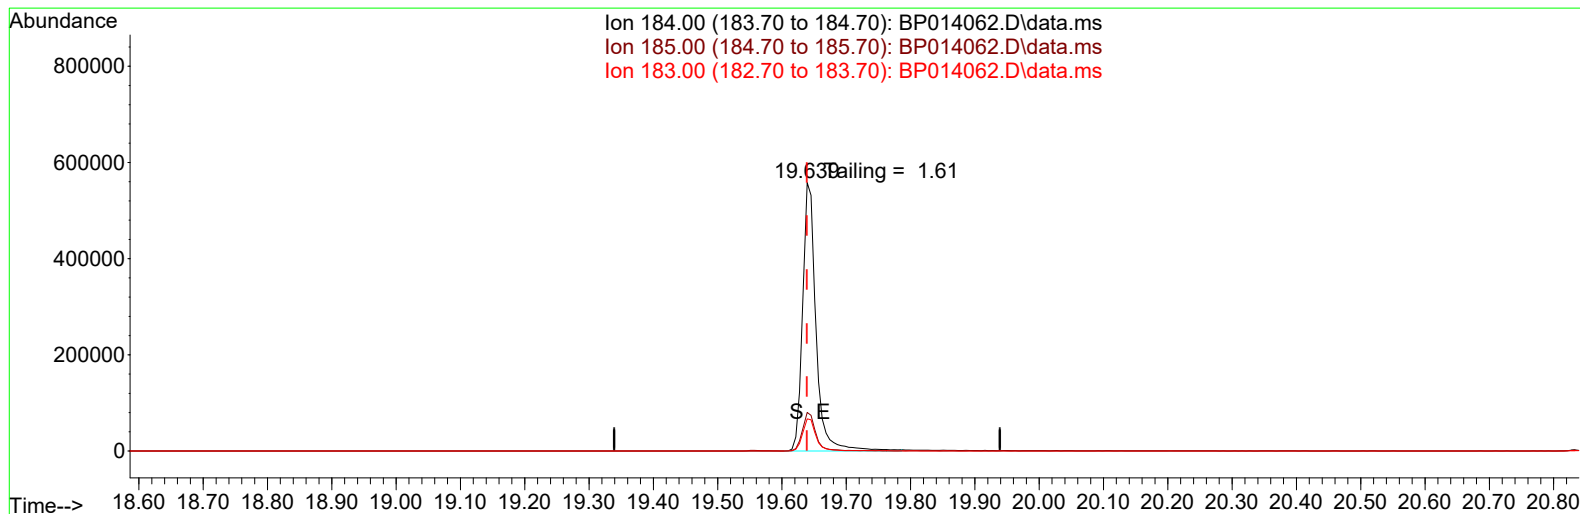

TIC: BP014062.D\data.ms

(77) Benzidine

19.639min (-0.000) -20.00 ng

response 814332

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.38
183.00	12.10	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2023	BNA_P	<u>BP014062.D</u>
Compound Name	Response	Retention Time
DDT	510961	20.833
DDD	6399	20.457
DDE	271	19.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6670	517631	1.29

Instrument :
BNA_P
ClientSampleId :
DFTPP