
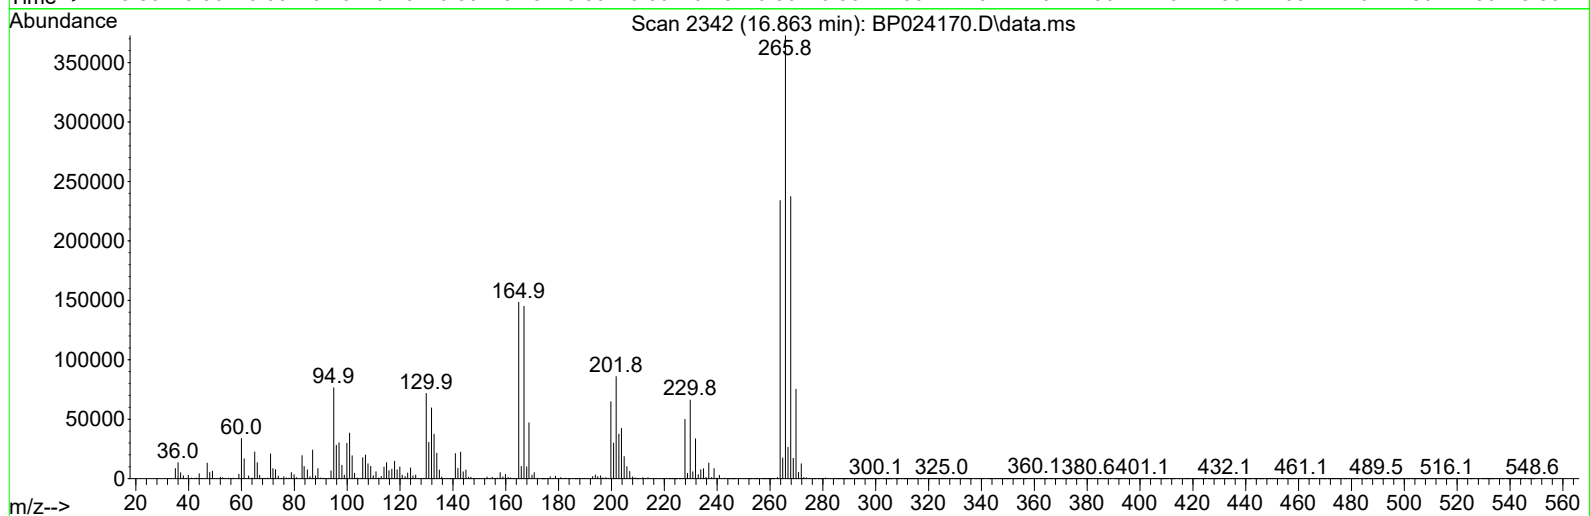


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031325\
Data File : BP024170.D
Acq On : 13 Mar 2025 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 11:49:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

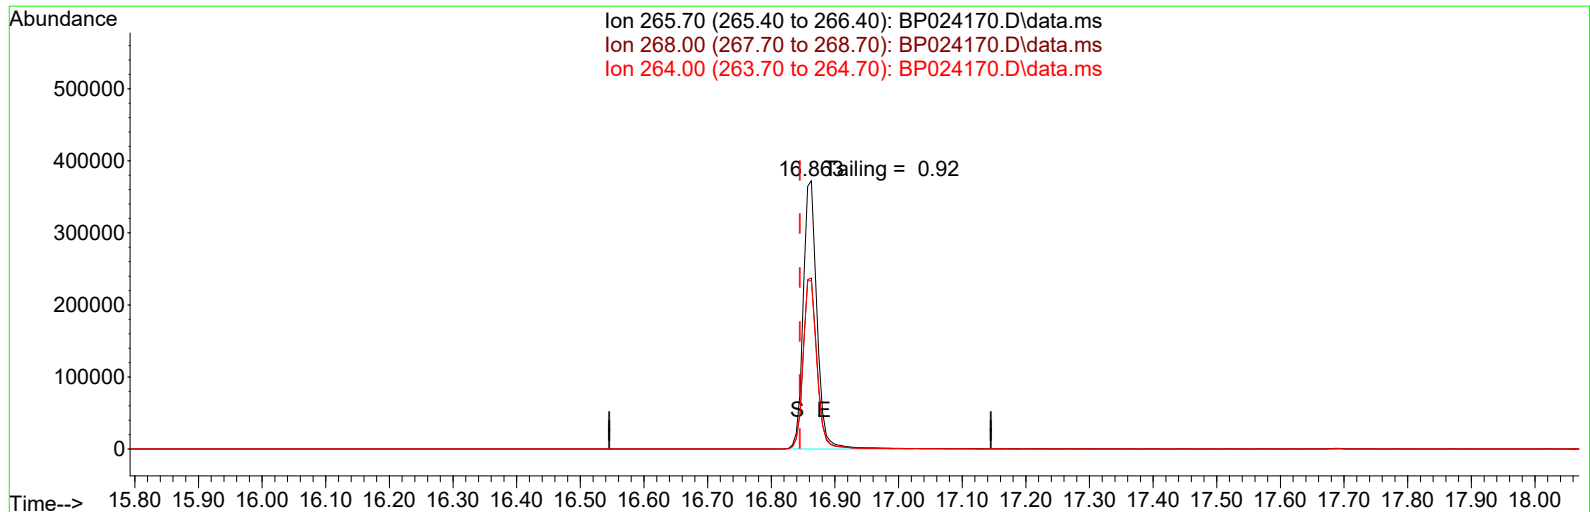



TIC: BP024170.D\data.ms

(70) Pentachlorophenol (C)**16.863min (+ 0.018) 604215.30 ng****response 563611**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.70
264.00	63.30	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031325\
Data File : BP024170.D
Acq On : 13 Mar 2025 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 11:49:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

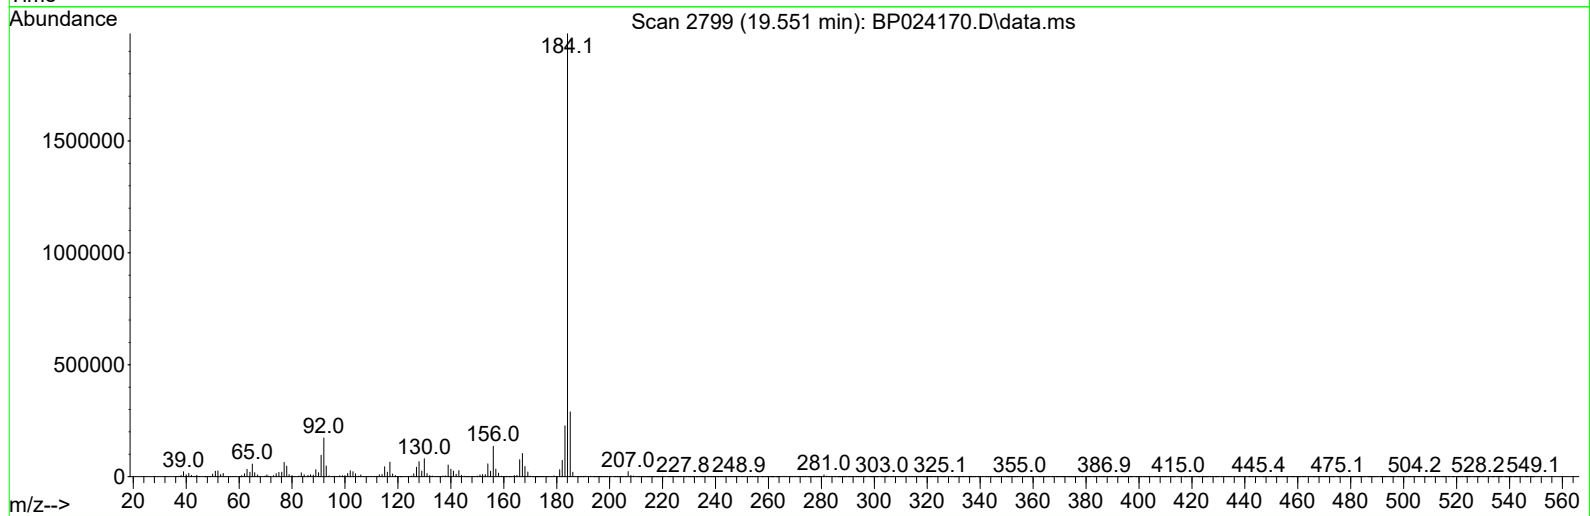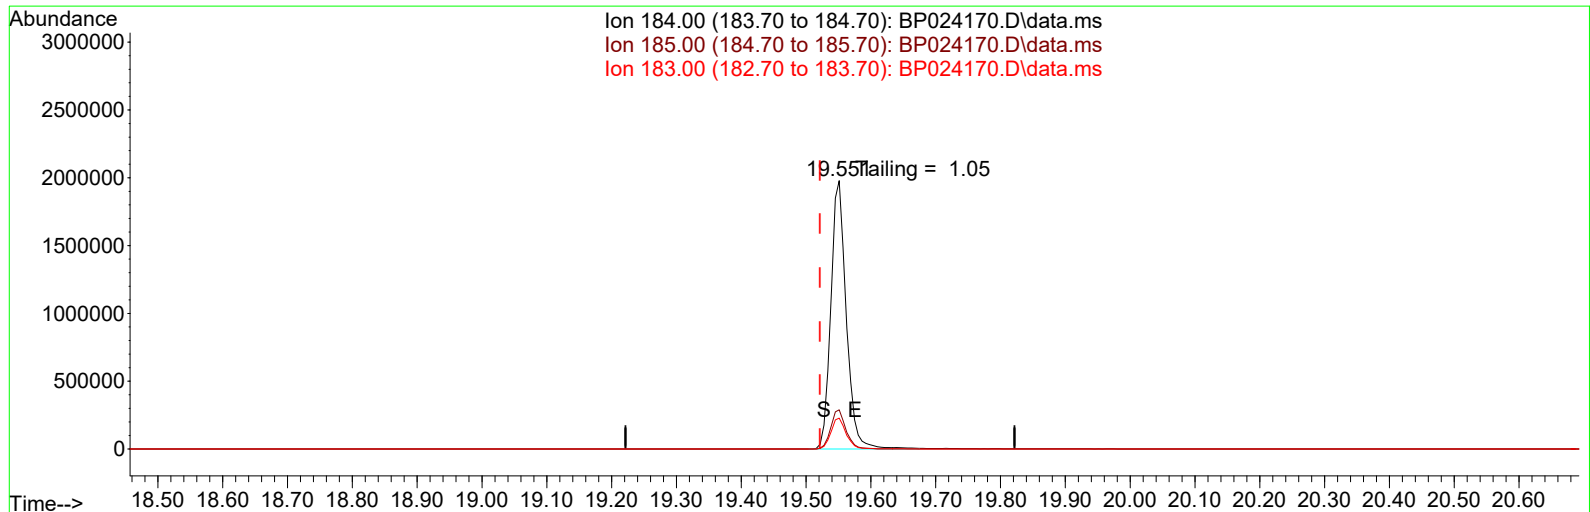

TIC: BP024170.D\data.ms

(77) Benzidine**19.551min (+ 0.029) 3326037.58 ng****response 3272849**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.62
183.00	11.40	11.51
0.00	0.00	0.00