
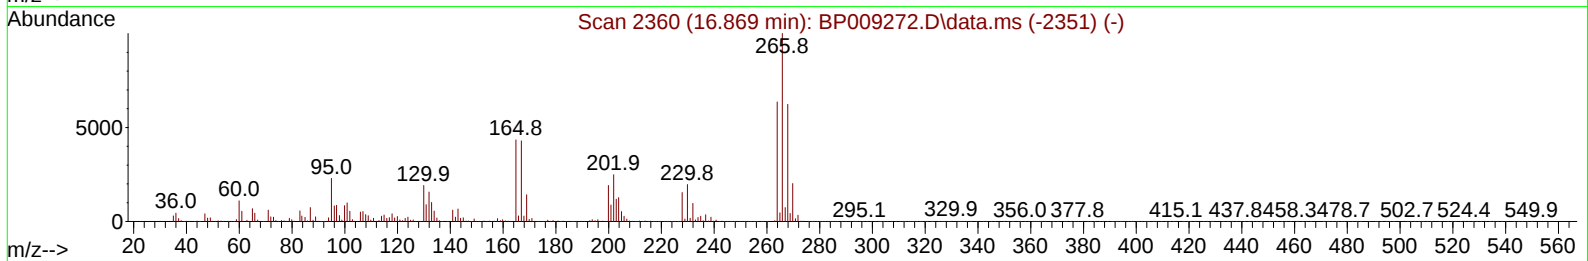
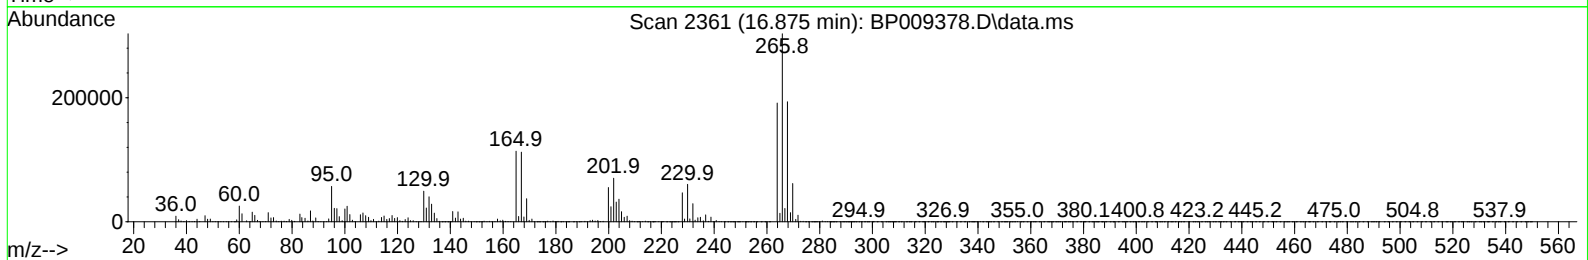


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP031422\  
 Data File : BP009378.D  
 Acq On : 14 Mar 2022 11:22  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 02:30:28 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP030522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Mar 05 01:55:59 2022  
 Response via : Initial Calibration

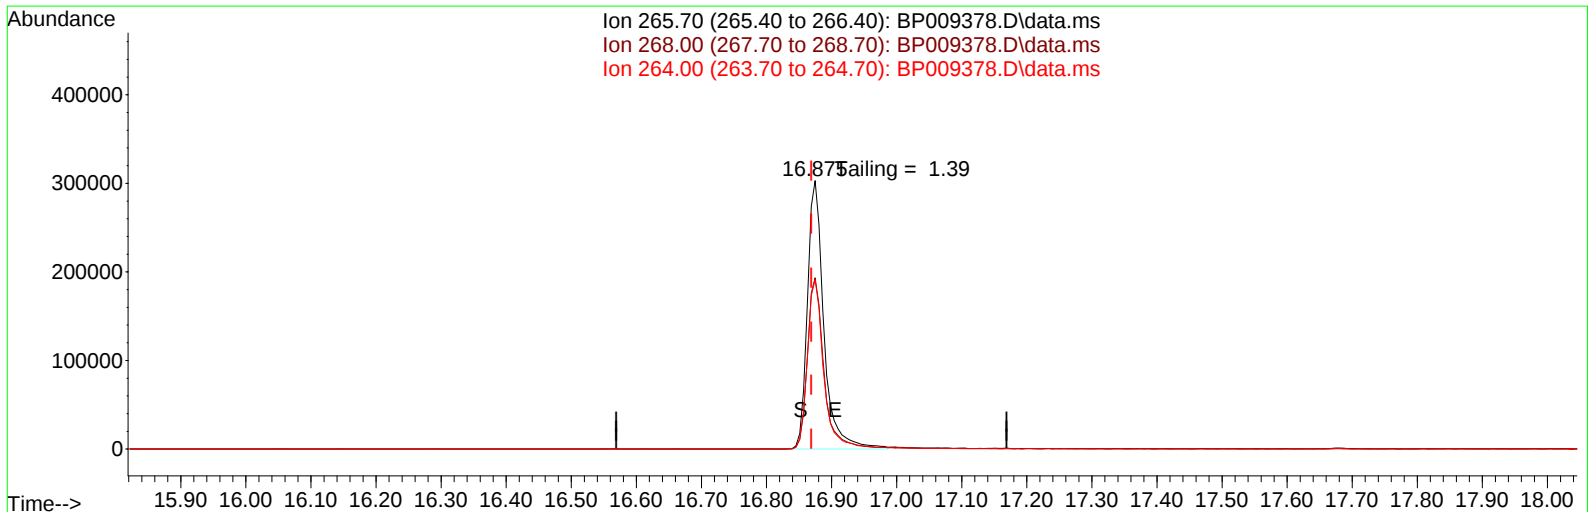

TIC: BP009378.D\data.ms

**(70) Pentachlorophenol (C)**




**16.875min (+ 0.006) 245789.04 ng**

**response 539146**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.30  | 63.81  |
| 264.00 | 63.60  | 63.15  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP031422\  
Data File : BP009378.D  
Acq On : 14 Mar 2022 11:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 02:30:28 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP030522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Mar 05 01:55:59 2022  
Response via : Initial Calibration

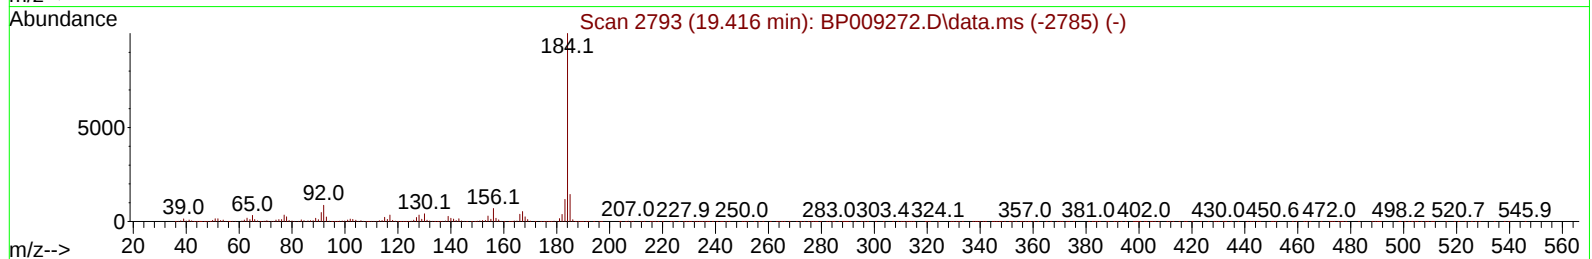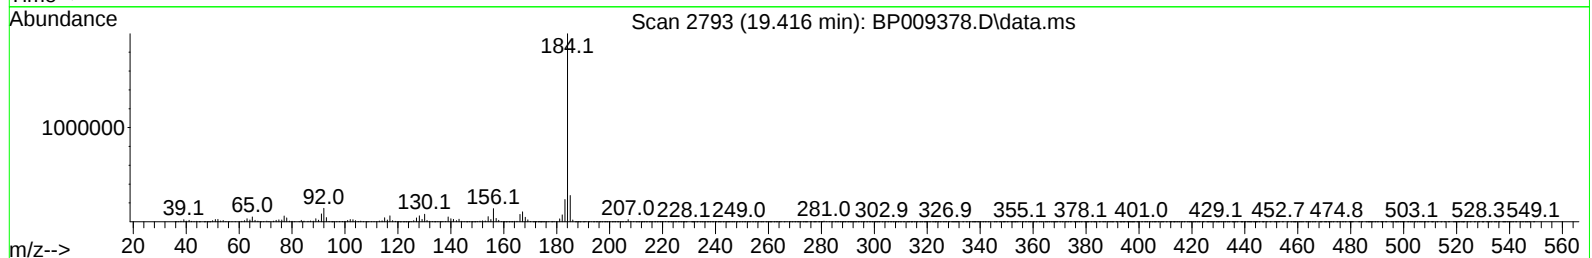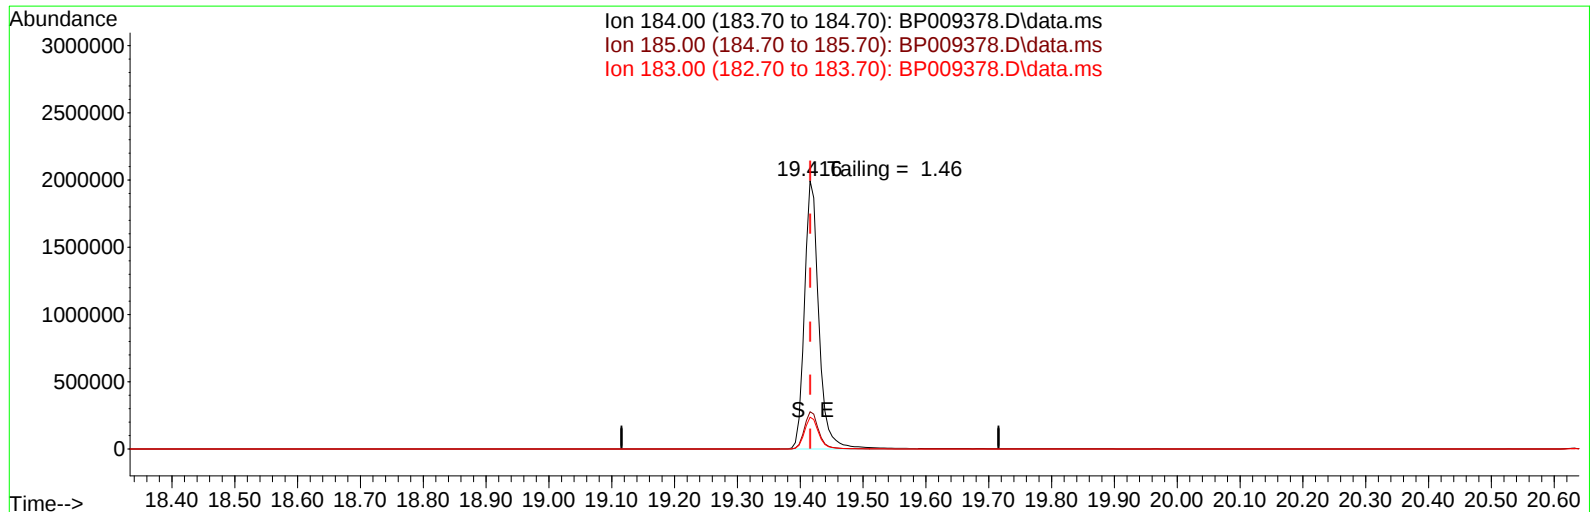

TIC: BP009378.D\data.ms

**(77) Benzidine****19.416min (-0.000) 63032.71 ng****response 3183525**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 13.92  |
| 183.00 | 11.70  | 11.87  |
| 0.00   | 0.00   | 0.00   |