

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
 Data File : BP009387.D
 Acq On : 14 Mar 2022 18:00
 Operator : CG/JU
 Sample : N1908-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WC-8-9-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	20	rVB4	642438	1237808	1.10%	0.120%
2	3.146	20	27	29	rBV3	998459	1882027	1.68%	0.182%
3	3.576	88	100	112	rBV3	8504849	30241078	26.93%	2.928%
4	3.723	117	125	135	rBV	6705313	16151533	14.38%	1.564%
5	3.811	135	140	150	rVB	5178947	11695635	10.41%	1.132%
6	3.923	150	159	172	rBV5	4211147	16948767	15.09%	1.641%
7	4.034	172	178	180	rBV	4992174	8969150	7.99%	0.868%
8	4.152	191	198	204	rBV3	1979267	4971569	4.43%	0.481%
9	4.228	204	211	214	rBV2	16466467	36846021	32.81%	3.567%
10	4.364	224	234	247	rVB3	12738926	40522052	36.08%	3.923%
11	4.511	247	259	267	rBV2	14548588	47677376	42.45%	4.616%
12	4.593	267	273	285	rBV4	7263626	22228058	19.79%	2.152%
13	4.693	285	290	301	rVB3	5609839	16245621	14.46%	1.573%
14	4.799	301	308	319	rBV	16794494	53887688	47.98%	5.217%
15	4.899	319	325	330	rBV	8568494	23191807	20.65%	2.245%
16	4.999	338	342	346	rBV	6055520	9675533	8.61%	0.937%
17	5.064	346	353	366	rVB	24667405	80327839	71.52%	7.776%
18	5.170	368	371	374	rBV	3508428	4991567	4.44%	0.483%
19	5.217	375	379	385	rBV	6143070	12191269	10.85%	1.180%
20	5.293	388	392	404	rVB	18997552	49364894	43.95%	4.779%
21	5.428	406	415	428	rVB5	9088093	34959573	31.13%	3.384%
22	5.546	428	435	445	rBV4	8636873	24746861	22.03%	2.396%
23	5.652	446	453	460	rBV3	9835365	26892098	23.94%	2.603%
24	5.734	460	467	474	rBV2	14358280	50097729	44.61%	4.850%
25	5.811	475	480	486	rBV2	10922259	24296142	21.63%	2.352%
26	5.946	498	503	514	rVB2	10823370	28038261	24.96%	2.714%
27	6.134	525	535	546	rBV5	23599157	98402308	87.61%	9.526%
28	6.352	564	572	579	rBV3	21774925	71995317	64.10%	6.970%
29	6.758	635	641	647	rVB4	8666073	21651460	19.28%	2.096%
30	6.828	648	653	669	rVB2	14724830	50339892	44.82%	4.873%
31	7.005	670	683	698	rBV5	24651404	112312592	100.00%	10.873%




Sum of corrected areas: 1032979525

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009387.D
Acq On : 14 Mar 2022 18:00
Operator : CG/JU
Sample : N1908-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WC-8-9-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

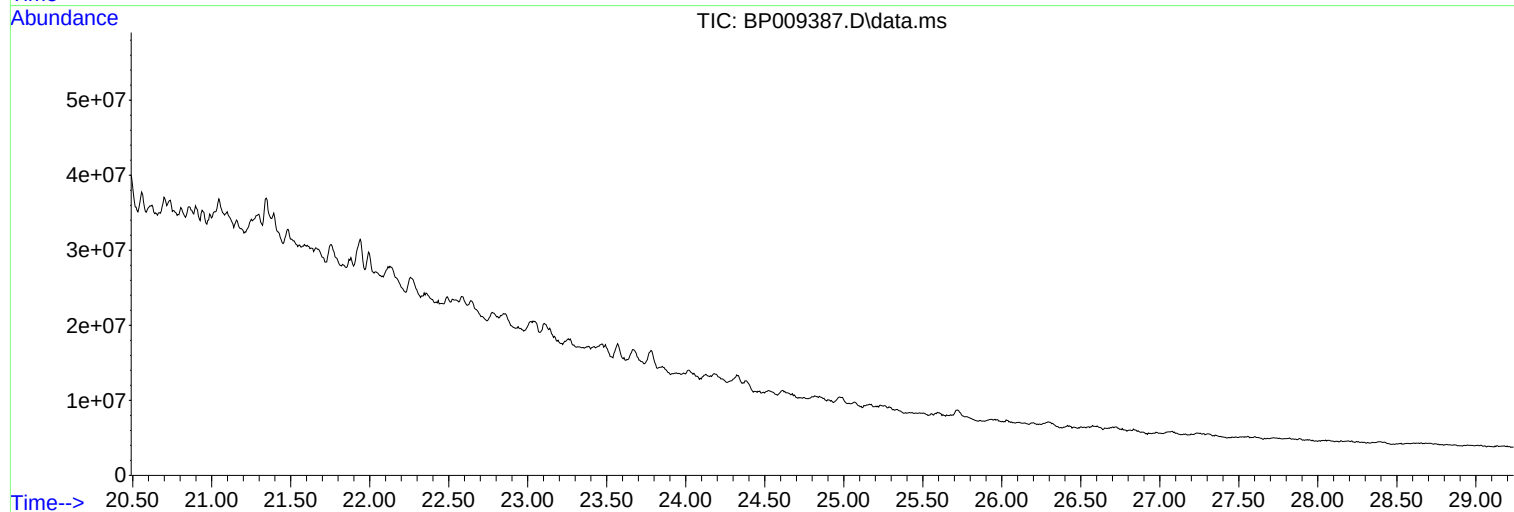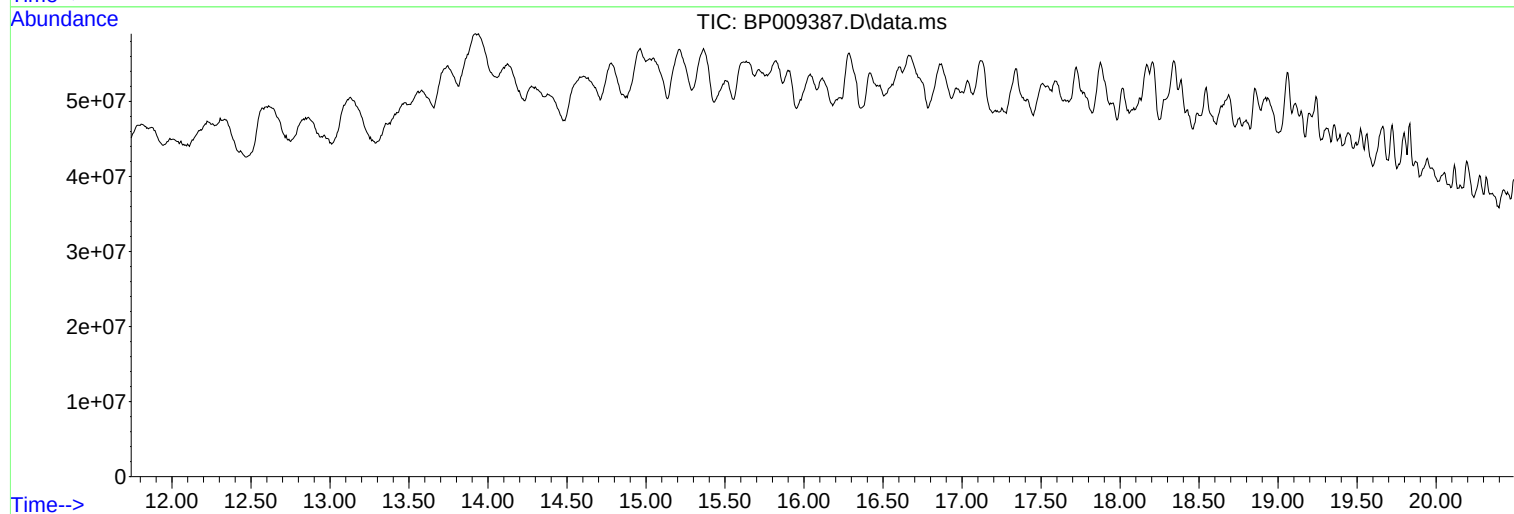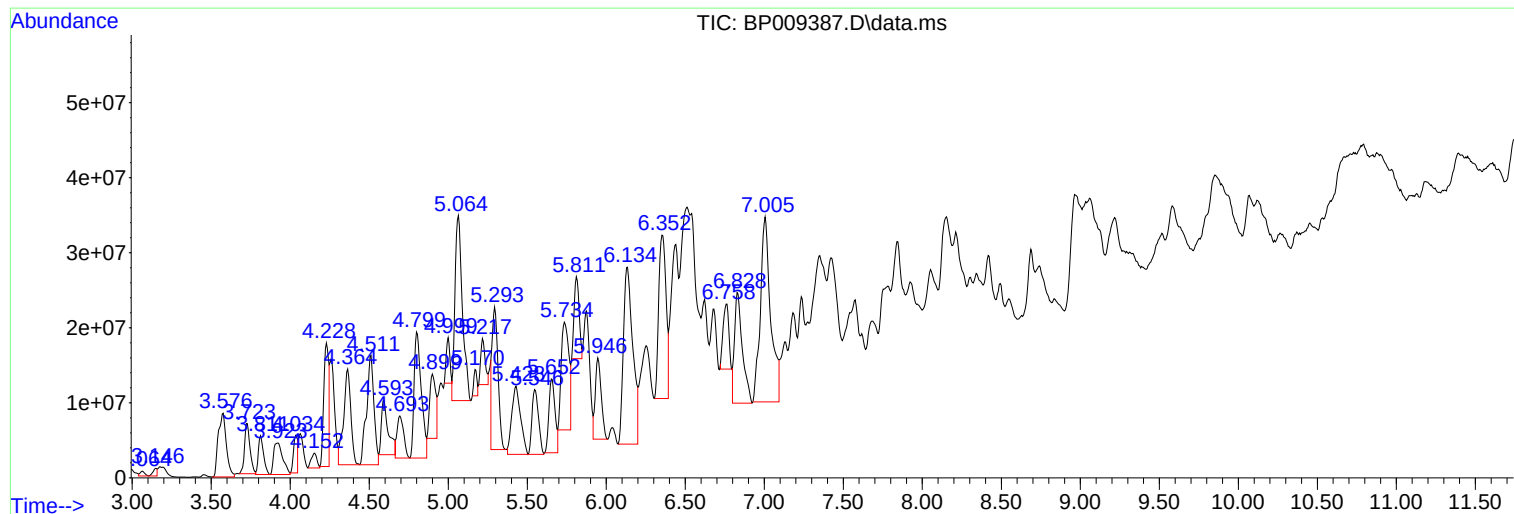

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009387.D
Acq On : 14 Mar 2022 18:00
Operator : CG/JU
Sample : N1908-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WC-8-9-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009387.D
Acq On : 14 Mar 2022 18:00
Operator : CG/JU
Sample : N1908-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WC-8-9-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------