

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
 Data File : BP009391.D
 Acq On : 14 Mar 2022 20:14
 Operator : CG/JU
 Sample : N1888-03 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 2

Instrument :
 BNA_P
 ClientSampleId :
 SS-3(PILE-3)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	9	12	22	rVB	103409	184624	3.14%	0.469%
2	5.422	407	414	427	rBV	931418	1593274	27.12%	4.049%
3	7.011	676	684	697	rBV	896916	1670708	28.44%	4.246%
4	7.816	813	821	835	rBV	1578798	2711702	46.16%	6.891%
5	8.969	1005	1017	1030	rBV	601878	1092721	18.60%	2.777%
6	10.410	1253	1262	1271	rBV4	23114	68029	1.16%	0.173%
7	10.610	1287	1296	1310	rBV	2072846	3822156	65.07%	9.713%
8	13.075	1708	1715	1728	rBV	1689740	2693004	45.84%	6.844%
9	14.334	1921	1929	1932	rBV4	23447	66987	1.14%	0.170%
10	14.457	1943	1950	1964	rBV	3225796	5134319	87.40%	13.048%
11	15.951	2198	2204	2214	rBV	1275424	2008445	34.19%	5.104%
12	17.216	2413	2419	2425	rBV	3854641	5874287	100.00%	14.929%
13	19.792	2852	2857	2861	rBV	2393597	3119969	53.11%	7.929%
14	21.327	3114	3118	3124	rVB	3356099	4714166	80.25%	11.980%
15	23.739	3523	3528	3541	rVB	2202010	4594529	78.21%	11.676%




Sum of corrected areas: 39348920

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009391.D
Acq On : 14 Mar 2022 20:14
Operator : CG/JU
Sample : N1888-03 5X
Misc :
ALS Vial : 14 Sample Multiplier: 2

Instrument :
BNA_P
ClientSampleId :
SS-3(PILE-3)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

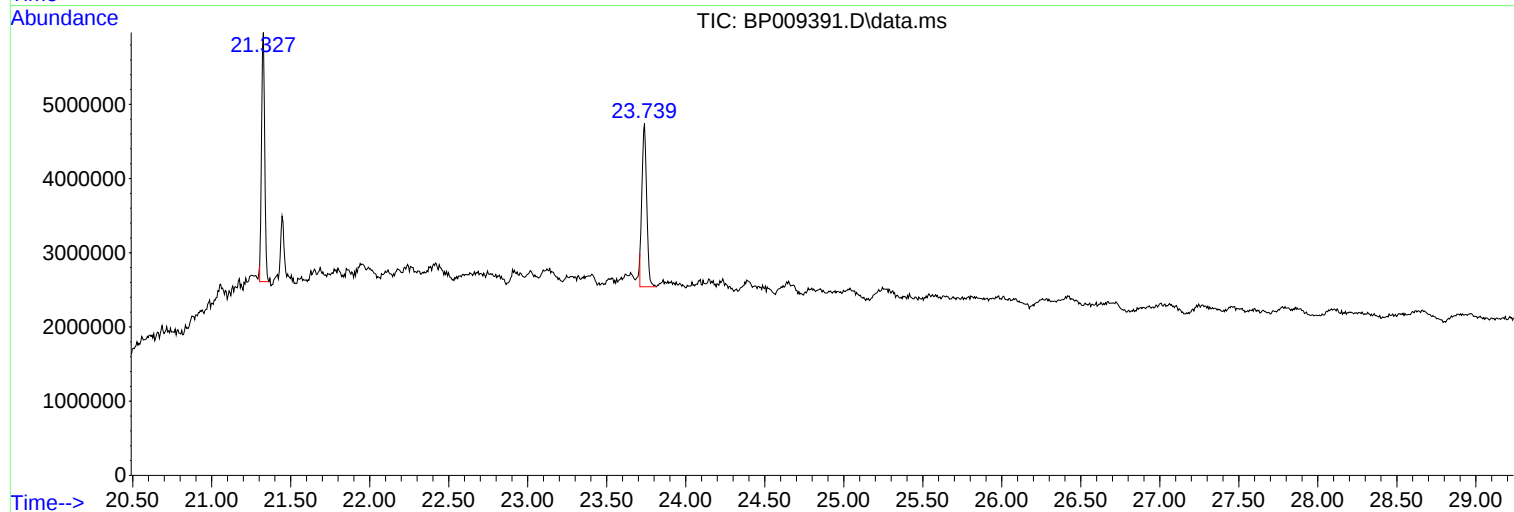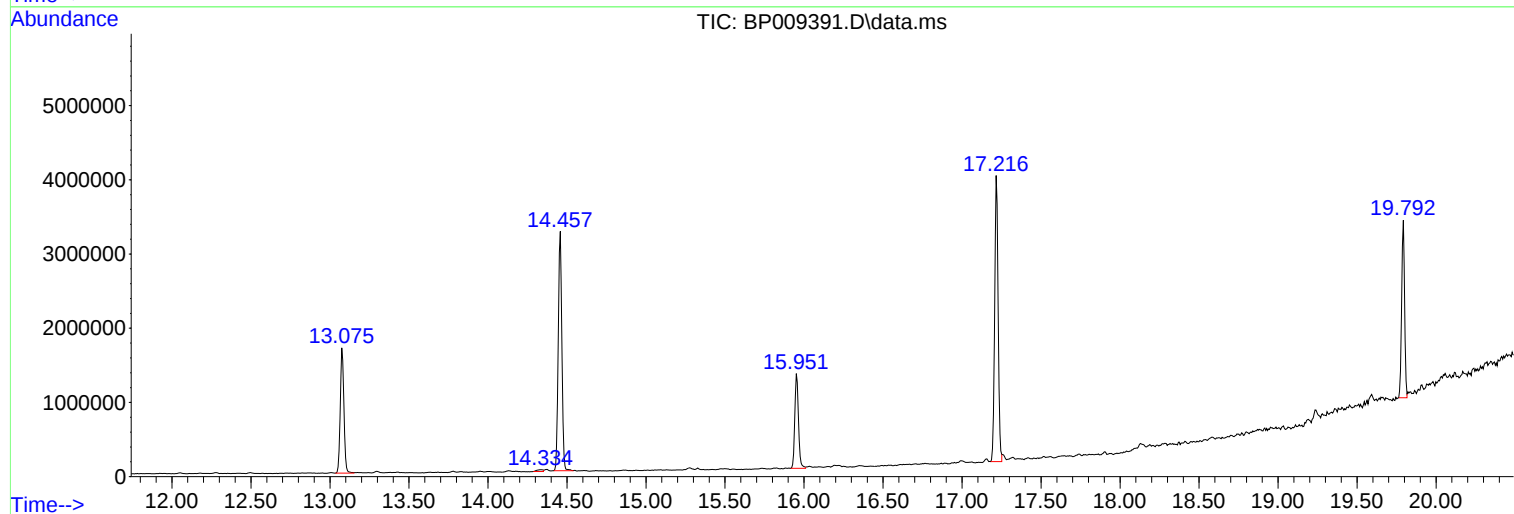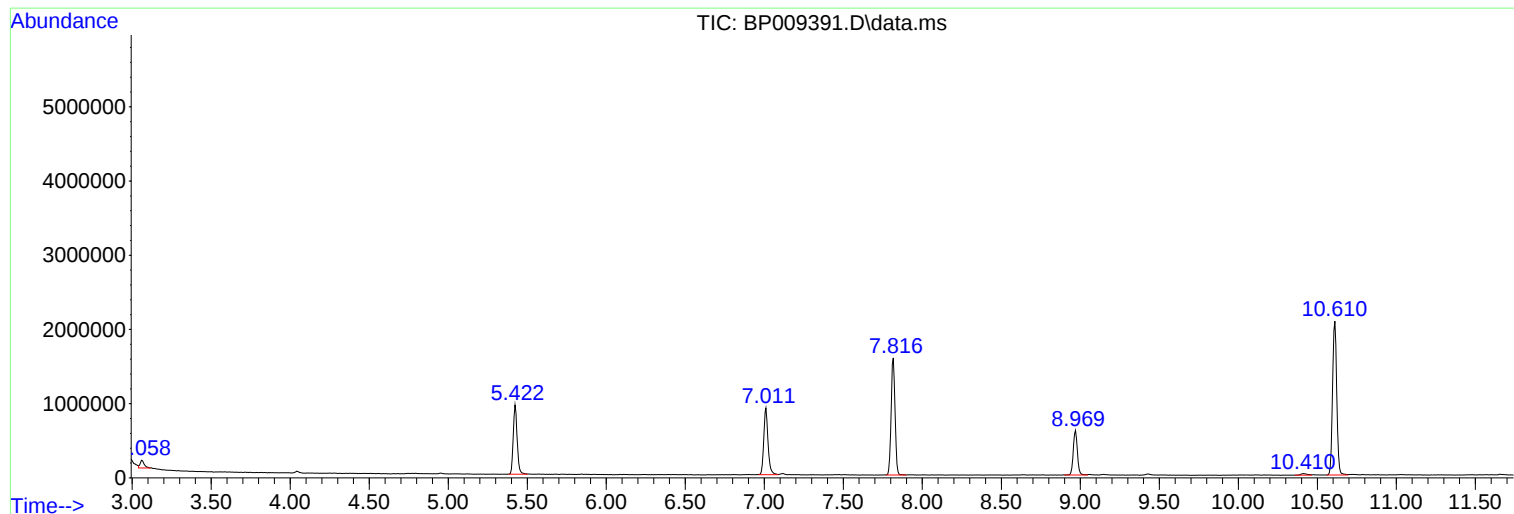

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009391.D
Acq On : 14 Mar 2022 20:14
Operator : CG/JU
Sample : N1888-03 5X
Misc :
ALS Vial : 14 Sample Multiplier: 2

Instrument :
BNA_P
ClientSampleId :
SS-3(PILE-3)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009391.D
Acq On : 14 Mar 2022 20:14
Operator : CG/JU
Sample : N1888-03 5X
Misc :
ALS Vial : 14 Sample Multiplier: 2

Instrument :
BNA_P
ClientSampleId :
SS-3(PILE-3)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------