

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
 Data File : BP009393.D
 Acq On : 14 Mar 2022 21:21
 Operator : CG/JU
 Sample : N1888-01 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SS-1(PILE-1)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	9	12	21	rVB	81178	140697	2.42%	0.337%
2	5.422	407	414	431	rBV	760137	1344717	23.12%	3.217%
3	7.010	676	684	698	rBV	750186	1418517	24.39%	3.394%
4	7.816	813	821	829	rBV	1397027	2412982	41.48%	5.773%
5	8.969	1007	1017	1027	rBV	498810	938386	16.13%	2.245%
6	10.610	1288	1296	1310	rBV	1864167	3458950	59.46%	8.276%
7	13.075	1708	1715	1725	rBV	1521213	2465899	42.39%	5.900%
8	13.787	1830	1836	1841	rBV3	131624	209749	3.61%	0.502%
9	14.175	1898	1902	1908	rVB2	39414	63715	1.10%	0.152%
10	14.457	1941	1950	1957	rBV	3125009	4864584	83.62%	11.638%
11	15.951	2198	2204	2214	rBV	1229641	2000515	34.39%	4.786%
12	17.216	2413	2419	2425	rBV	3666322	5817170	100.00%	13.918%
13	18.128	2570	2574	2580	rBV3	194902	324646	5.58%	0.777%
14	19.239	2759	2763	2766	rBV	310390	438714	7.54%	1.050%
15	19.586	2820	2822	2827	rVB	211777	233856	4.02%	0.559%
16	19.792	2852	2857	2862	rBV	2860198	3640133	62.58%	8.709%
17	21.327	3113	3118	3123	rBV	3947719	5484342	94.28%	13.121%
18	21.445	3135	3138	3149	rVB	925958	1522809	26.18%	3.643%
19	23.739	3523	3528	3538	rVB2	2411354	5017062	86.25%	12.003%




Sum of corrected areas: 41797443

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009393.D
Acq On : 14 Mar 2022 21:21
Operator : CG/JU
Sample : N1888-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SS-1(PILE-1)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

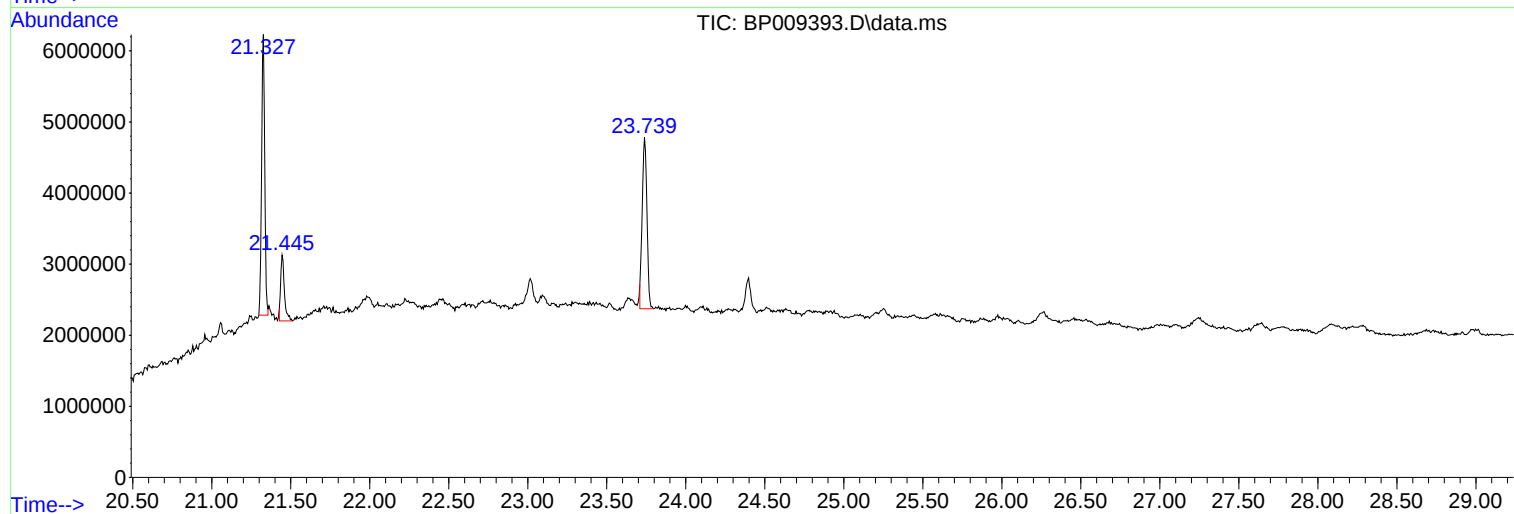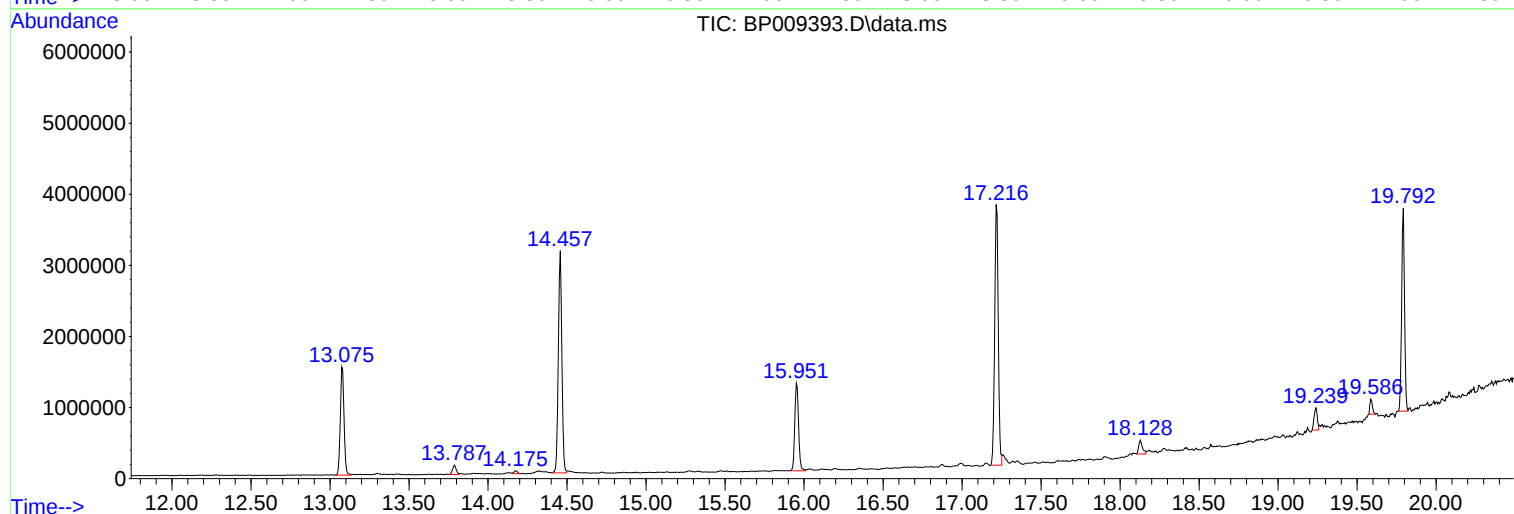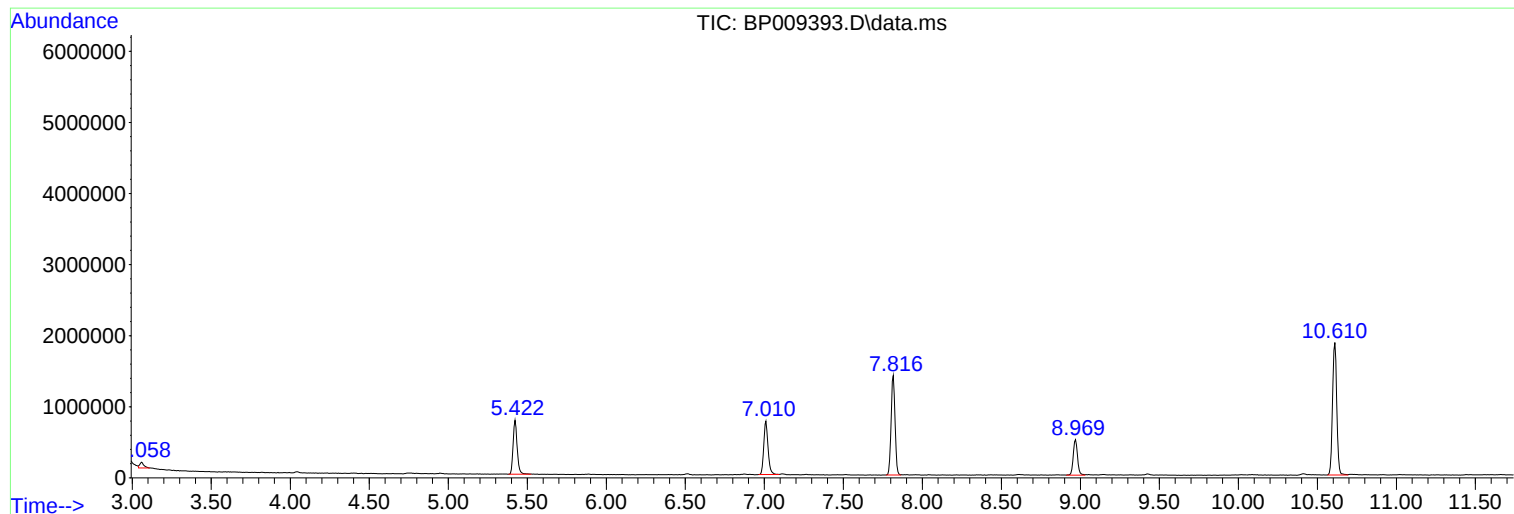

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009393.D
Acq On : 14 Mar 2022 21:21
Operator : CG/JU
Sample : N1888-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SS-1(PILE-1)










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.445	5.55 ng	1522810	Chrysene-d12	21.327

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	94
2			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	59
3			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	38
4			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	38
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	36

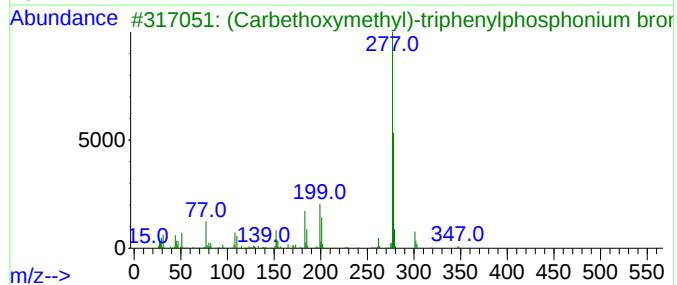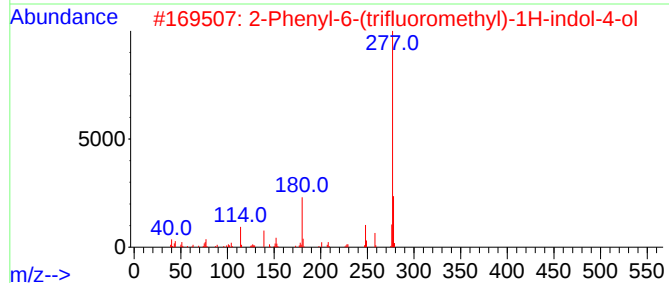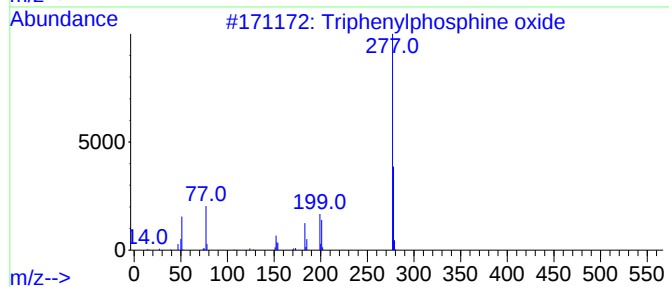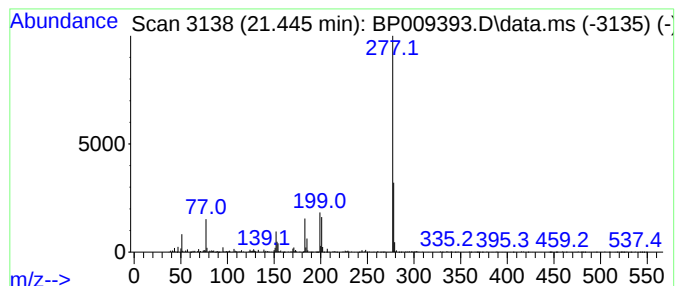

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009393.D
Acq On : 14 Mar 2022 21:21
Operator : CG/JU
Sample : N1888-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SS-1(PILE-1)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.445	5.5	ng	1522810	5	21.327	5484340	20.0