
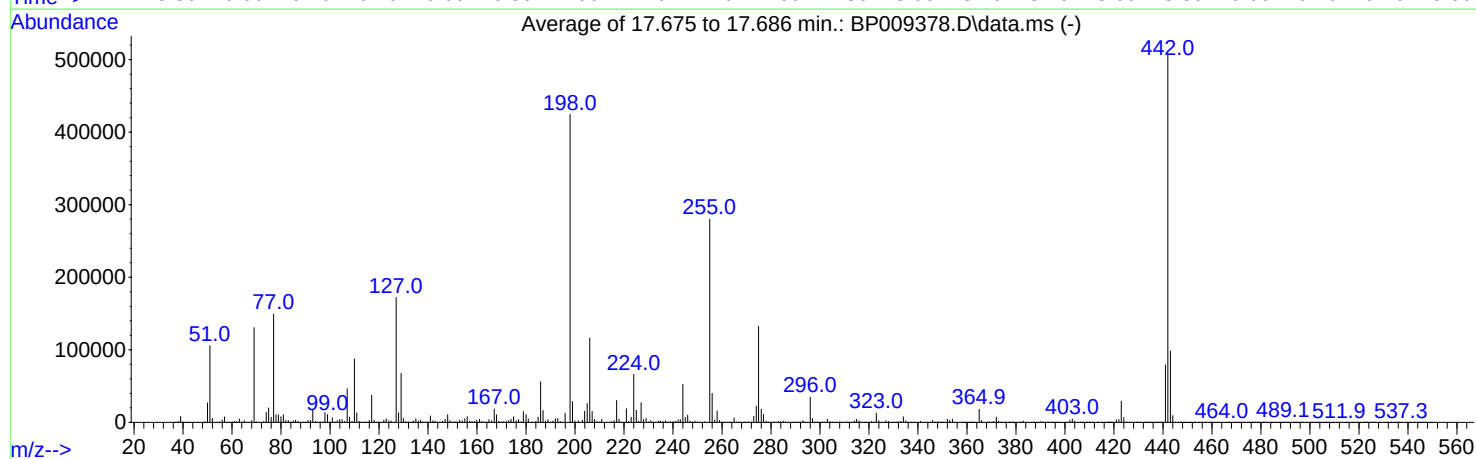


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
 Data File : BP009378.D
 Acq On : 14 Mar 2022 11:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

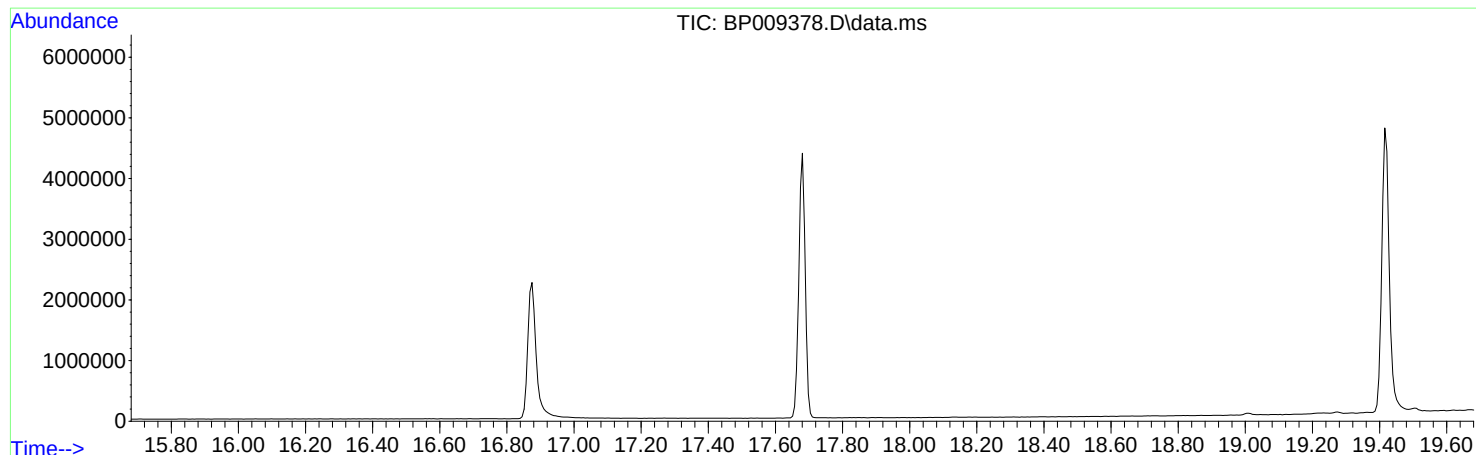




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	105743	PASS
68	69	0.00	2	1.8	2345	PASS
69	198	0.00	100	30.7	130476	PASS
70	69	0.00	2	0.6	792	PASS
127	198	10	80	40.5	171984	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	424325	PASS
199	198	5	9	6.8	28691	PASS
275	198	10	60	31.2	132329	PASS
365	198	1	100	4.3	18170	PASS
441	198	0.01	100	18.7	79251	PASS
442	442	100	100	100.0	507045	PASS
443	442	15	24	19.4	98369	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009378.D
Acq On : 14 Mar 2022 11:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 15 02:30:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

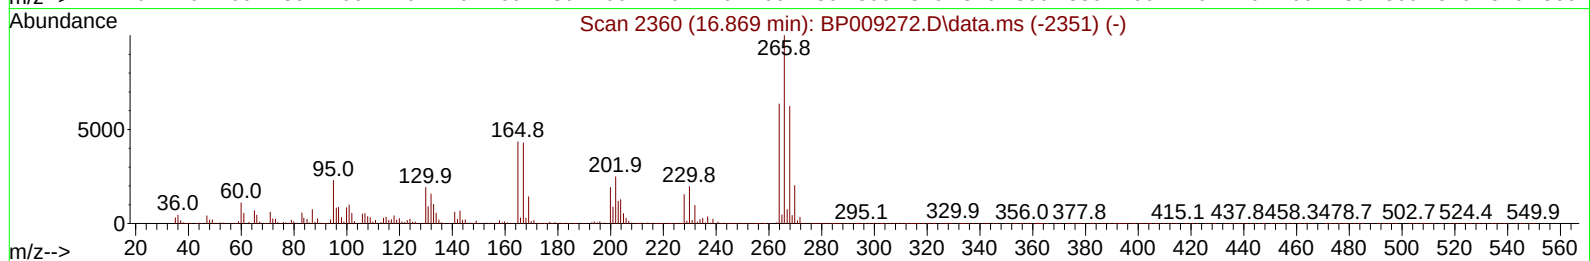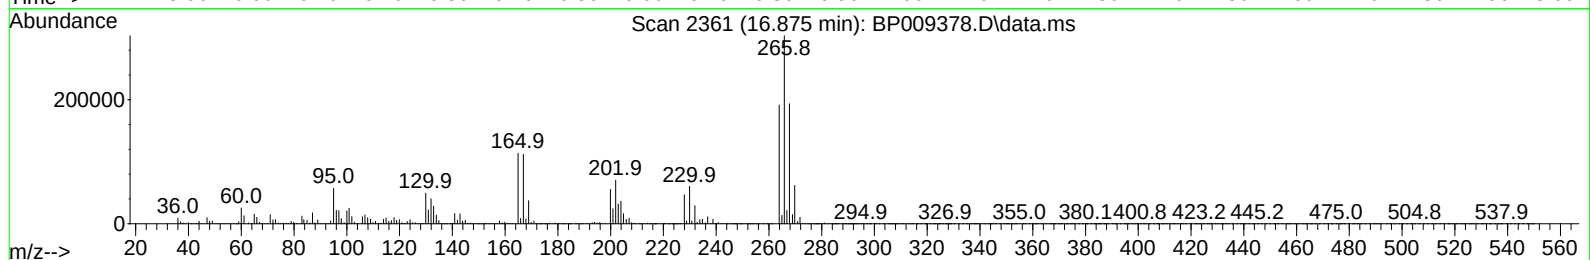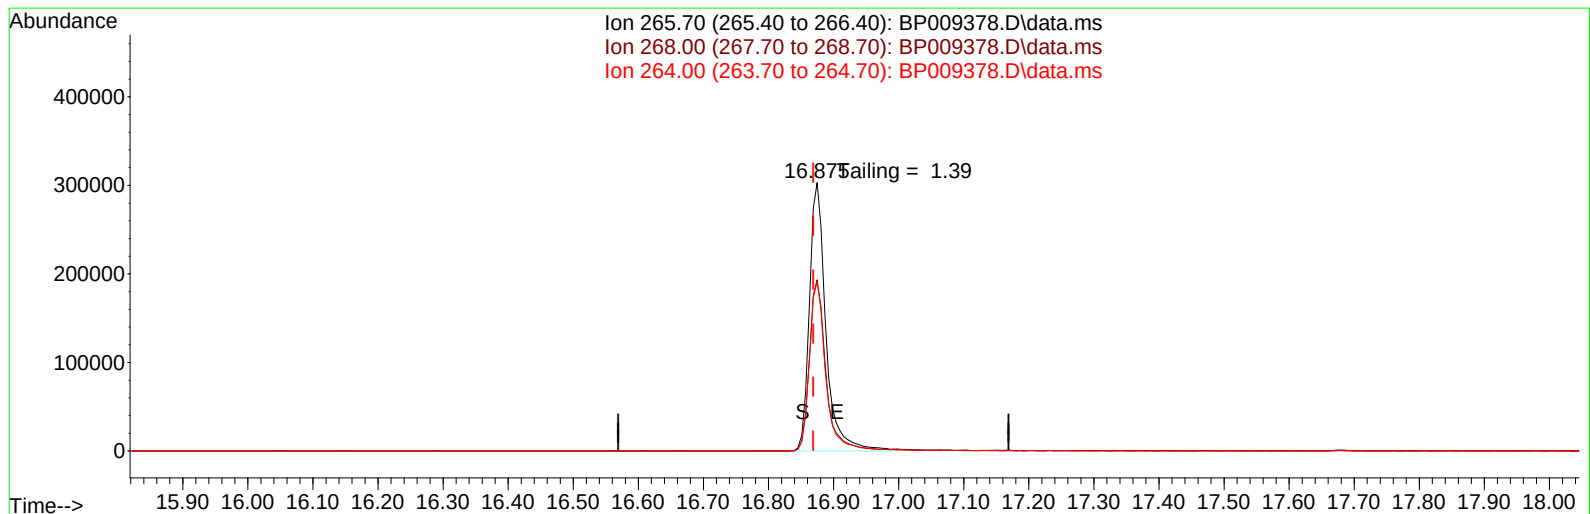

TIC: BP009378.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.006) 245789.04 ng




response 539146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.81
264.00	63.60	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031422\
Data File : BP009378.D
Acq On : 14 Mar 2022 11:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 15 02:30:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

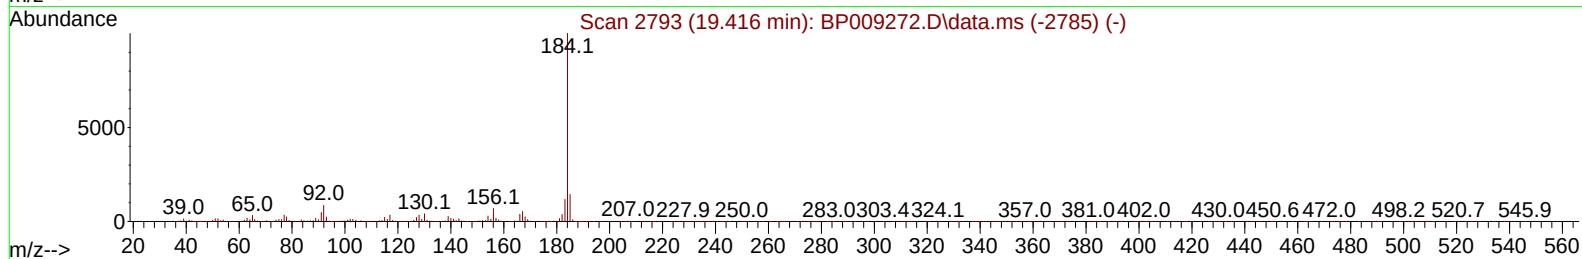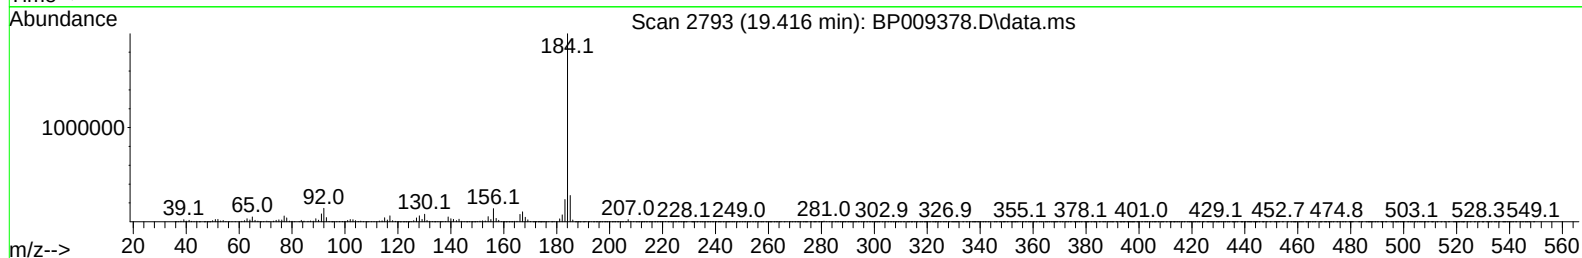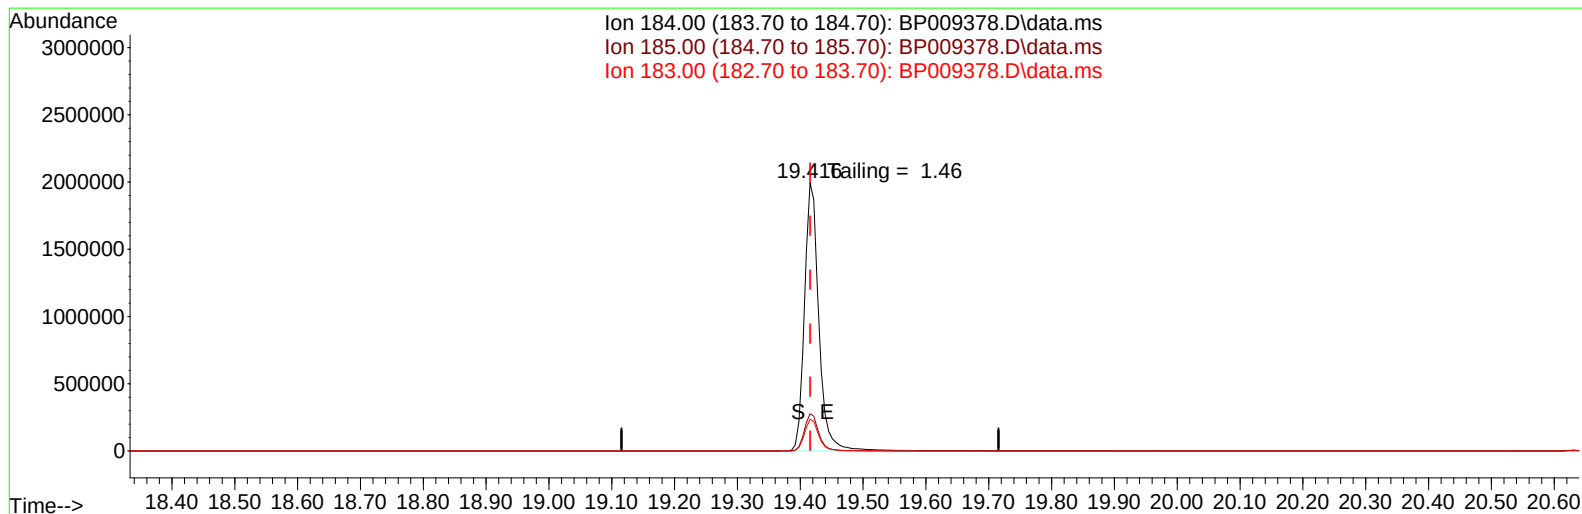

TIC: BP009378.D\data.ms

(77) Benzidine

19.416min (-0.000) 63032.71 ng

response 3183525

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.92
183.00	11.70	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2022	BNA_P	<u>BP009378.D</u>
Compound Name	Response	Retention Time
DDT	1646176	20.633
DDD	42499	20.198
DDE	3141	19.698
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45640	1691816	2.70

Instrument :
BNA_P
ClientSampleId :
DFTPP