
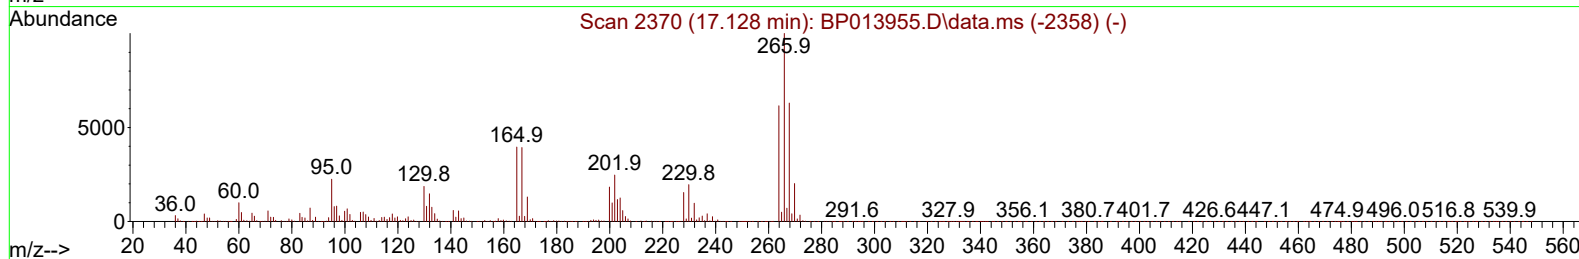
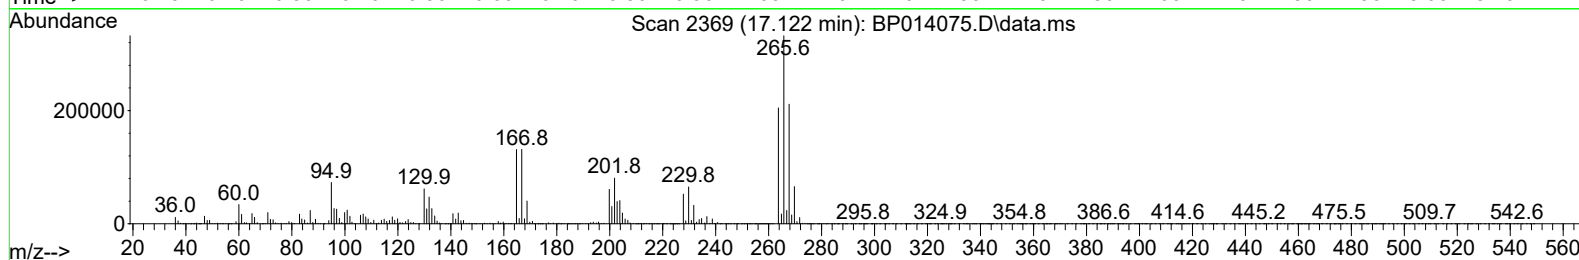


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014075.D
Acq On : 14 Mar 2023 09:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:42:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 04:15:47 2023
Response via : Initial Calibration

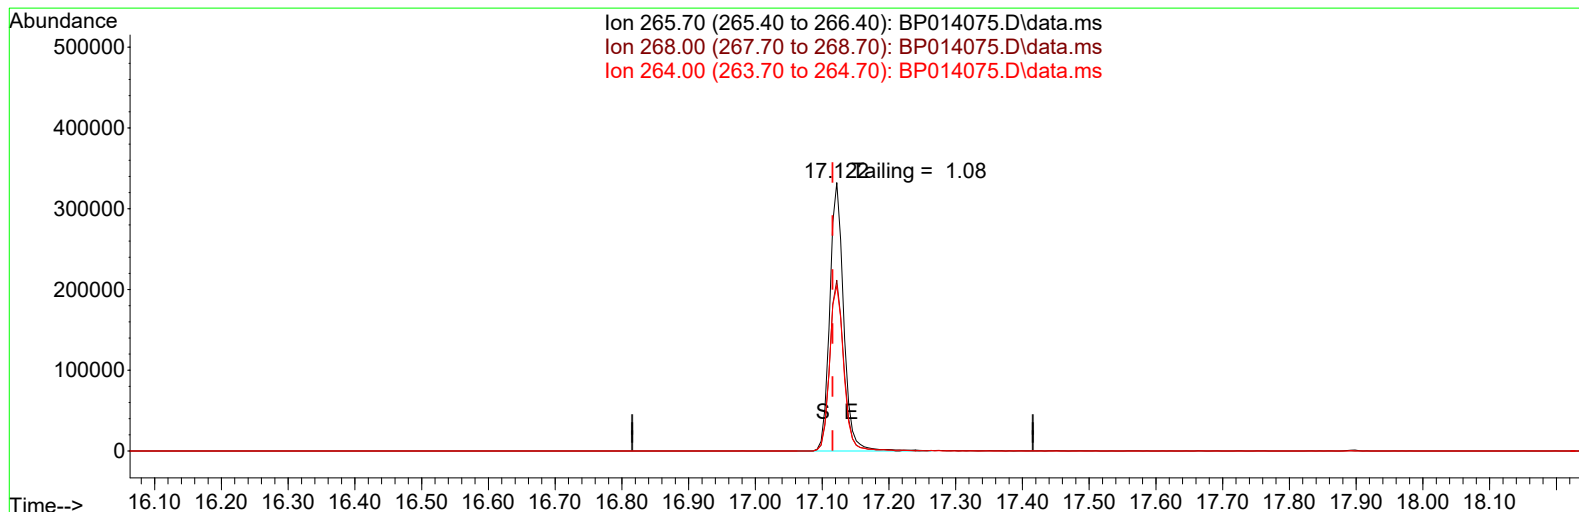

TIC: BP014075.D\data.ms

(70) Pentachlorophenol (C)




17.122min (+ 0.006) 177815.86 ng

response 481834

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	68.25
264.00	61.50	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
 Data File : BP014075.D
 Acq On : 14 Mar 2023 09:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:42:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 04:15:47 2023
 Response via : Initial Calibration

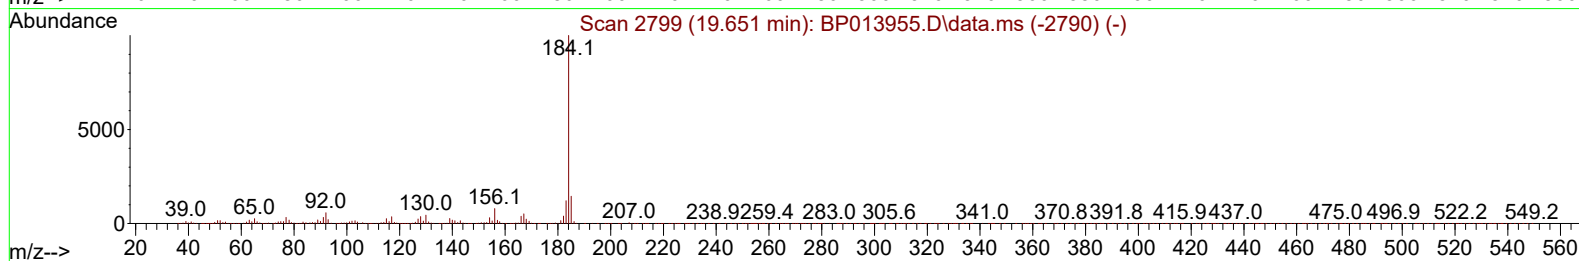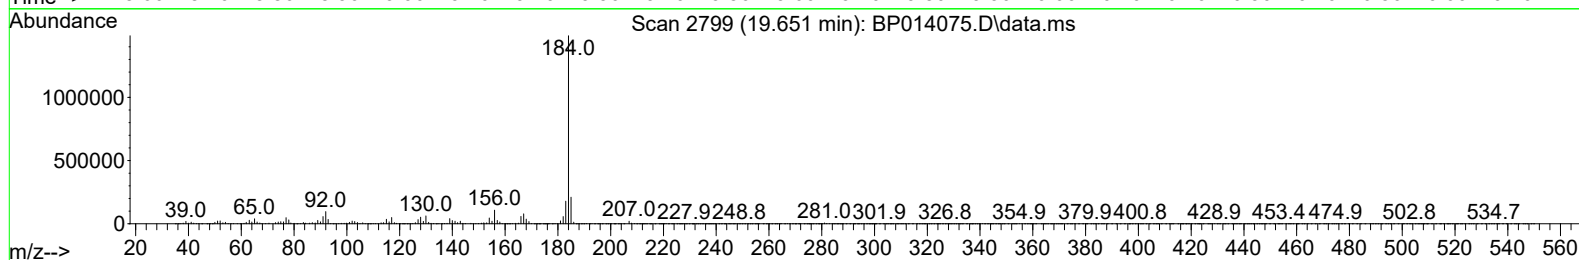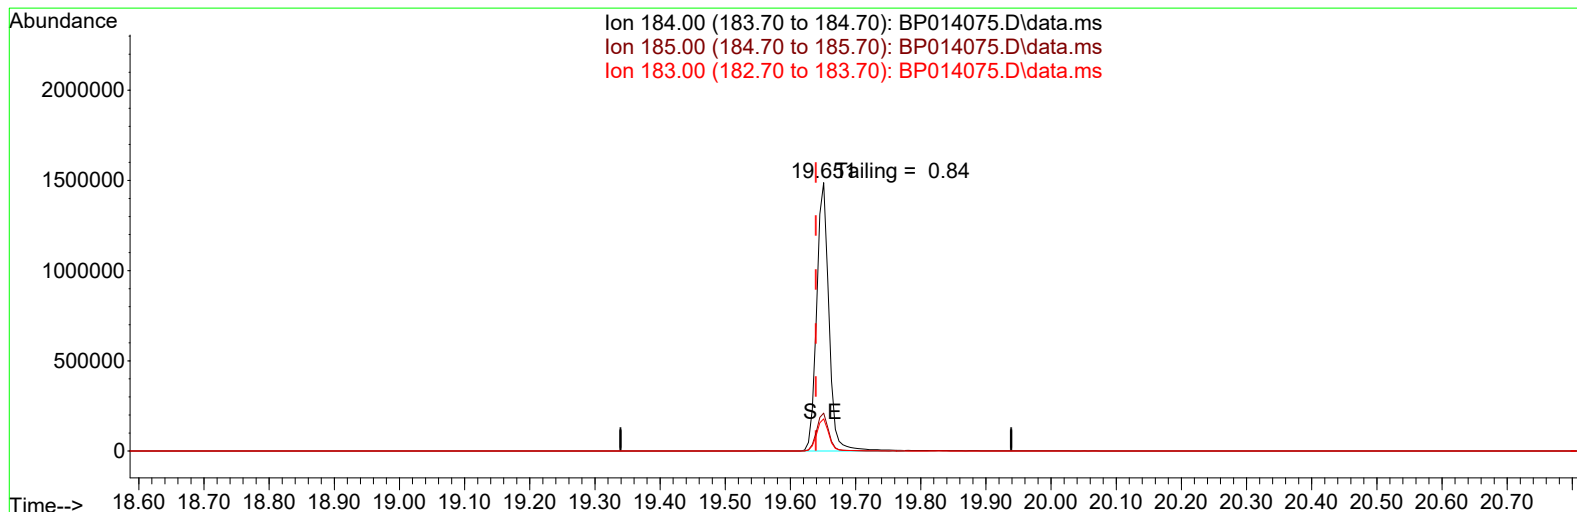

TIC: BP014075.D\data.ms

(77) Benzidine**19.651min (+ 0.012) -20.00 ng****response 1952243**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.13
183.00	12.10	11.99
0.00	0.00	0.00