

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
 Data File : BP014093.D
 Acq On : 14 Mar 2023 21:09
 Operator : CG/JU
 Sample : 01905-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MAPLE-2

Quant Time: Mar 15 04:36:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 04:15:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.069	152	108931	20.000	ng	0.00
21) Naphthalene-d8	10.886	136	396656	20.000	ng	#-0.01
39) Acenaphthene-d10	14.704	164	237156	20.000	ng	-0.01
64) Phenanthrene-d10	17.463	188	508273	20.000	ng	0.00
76) Chrysene-d12	21.539	240	488768	20.000	ng	0.00
86) Perylene-d12	24.074	264	512559	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.610	112	952483	141.804	ng	0.00
7) Phenol-d6	7.222	99	1114300	126.355	ng	0.00
23) Nitrobenzene-d5	9.239	82	869102	100.144	ng	-0.01
42) 2,4,6-Tribromophenol	16.198	330	533202	138.669	ng	0.00
45) 2-Fluorobiphenyl	13.327	172	1808644	98.806	ng	-0.01
79) Terphenyl-d14	19.998	244	2971827	100.260	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014093.D
Acq On : 14 Mar 2023 21:09
Operator : CG/JU
Sample : 01905-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MAPLE-2

Quant Time: Mar 15 04:36:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 04:15:47 2023
Response via : Initial Calibration




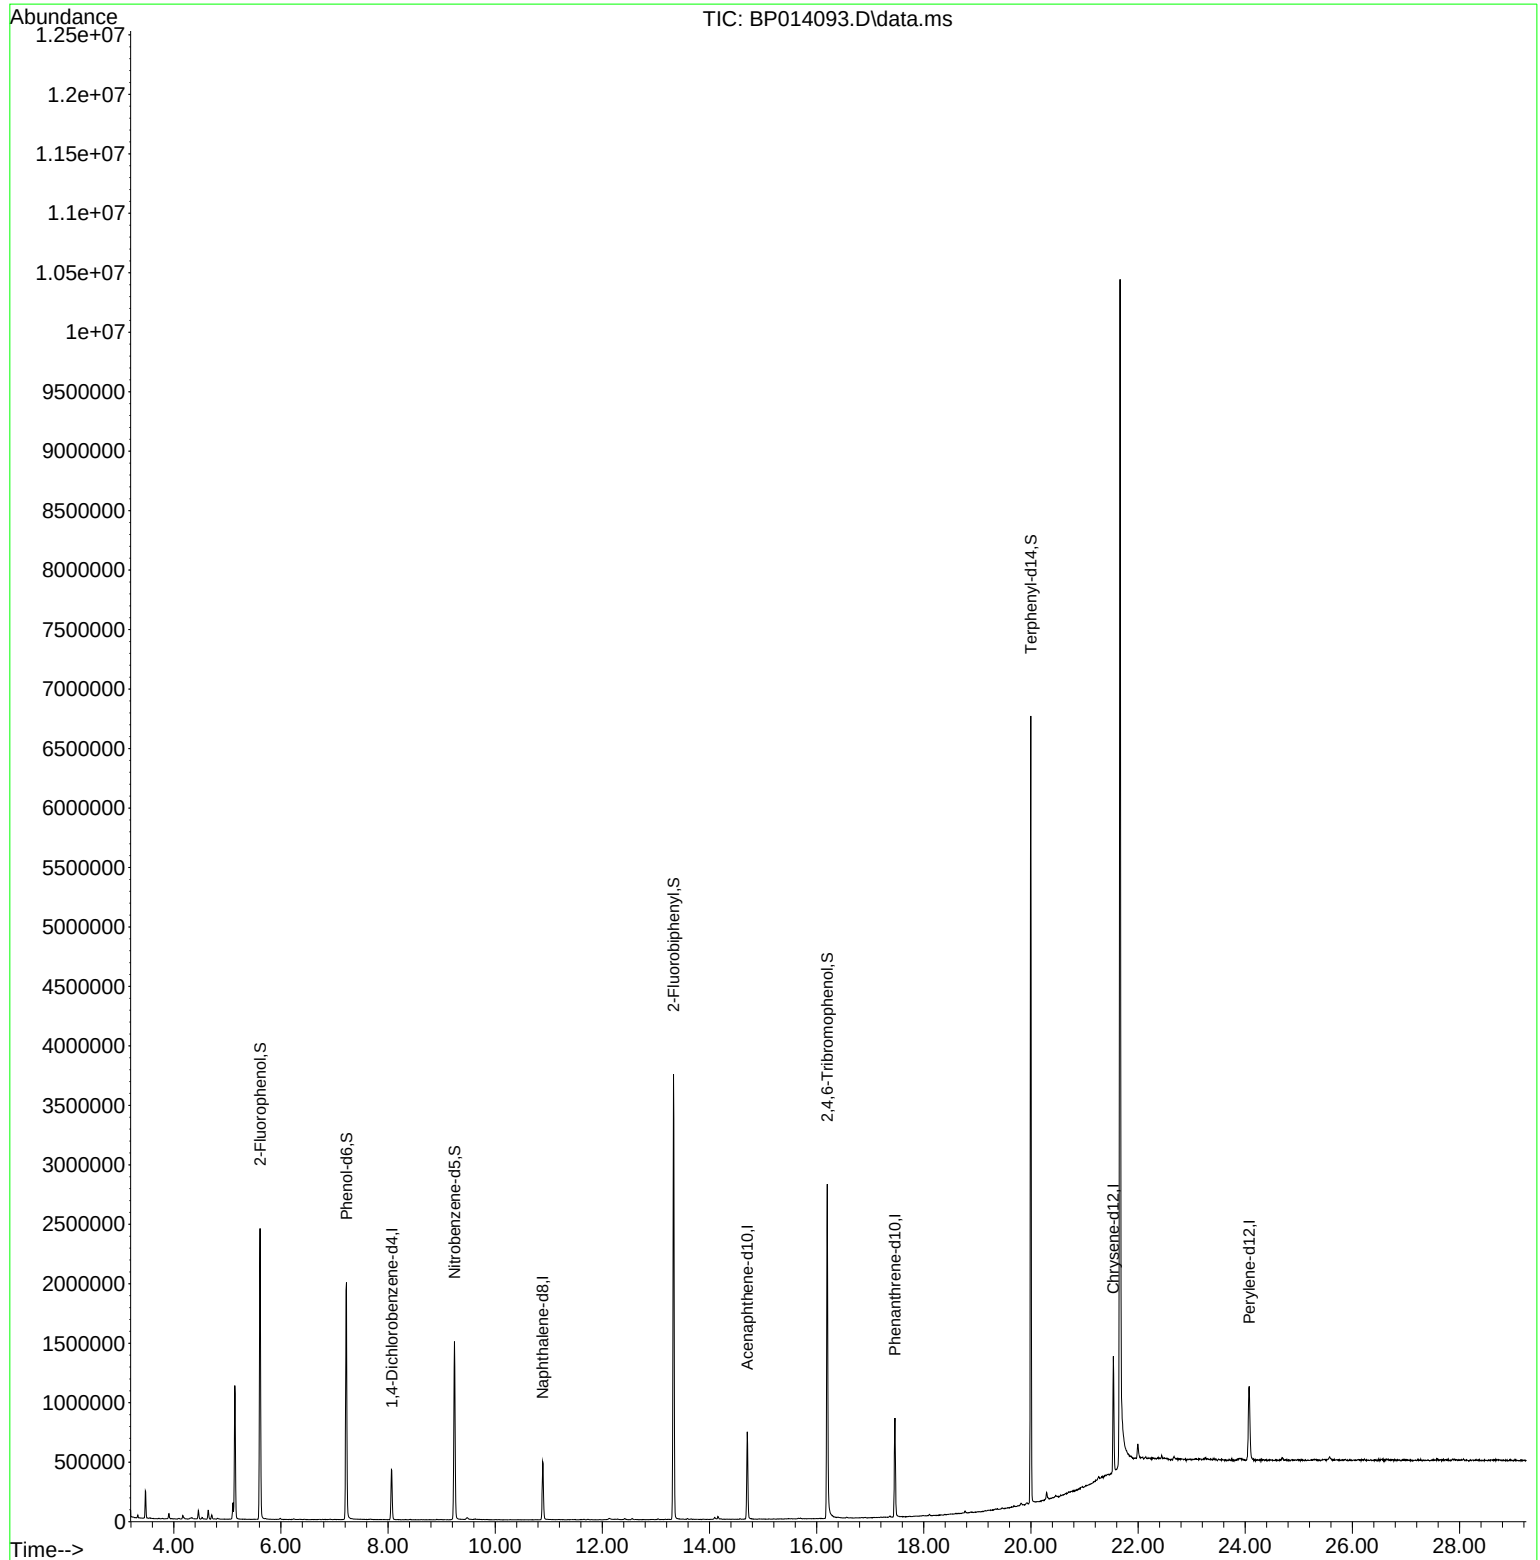


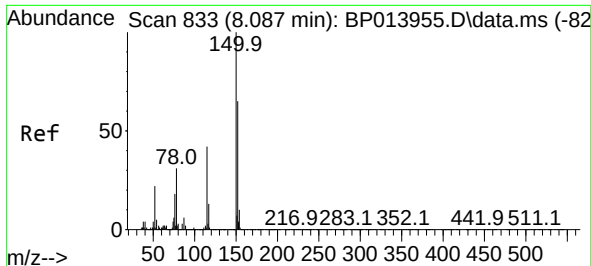

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.069 min Scan# 81
 Delta R.T. -0.006 min
 Lab File: BP014093.D
 Acq: 14 Mar 2023 21:09




Instrument :
 BNA_P
 ClientSampleId :
 MAPLE-2


Tgt Ion:152 Resp: 108931
 Ion Ratio Lower Upper
 152 100
 150 155.6 122.3 183.5
 115 64.3 51.6 77.4

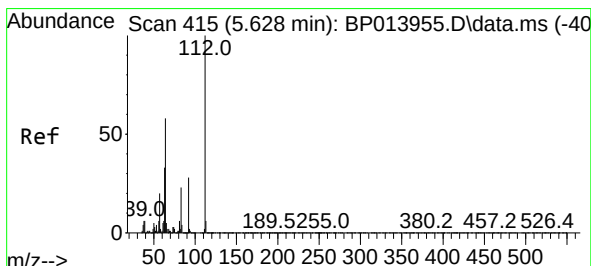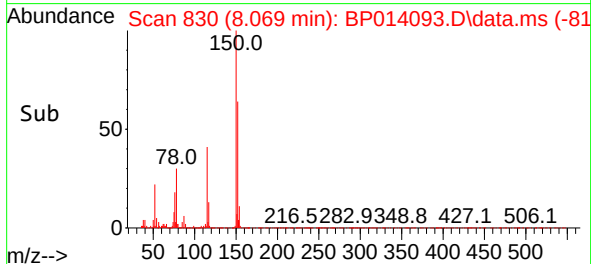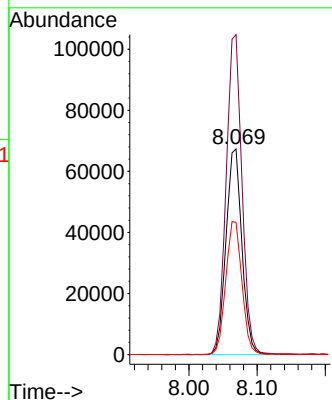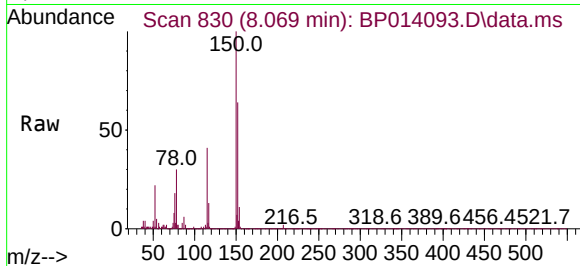

#5
 2-Fluorophenol
 Concen: 141.804 ng
 RT: 5.610 min Scan# 412
 Delta R.T. -0.006 min
 Lab File: BP014093.D
 Acq: 14 Mar 2023 21:09

Tgt Ion:112 Resp: 952483
 Ion Ratio Lower Upper
 112 100
 64 62.8 46.7 70.1
 63 32.8 26.6 40.0


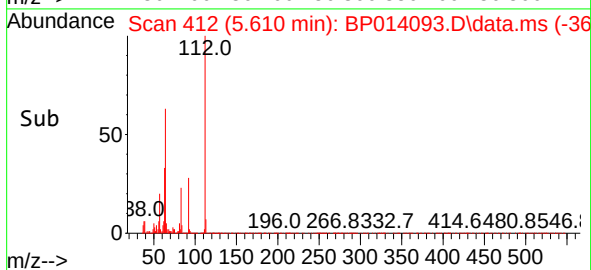
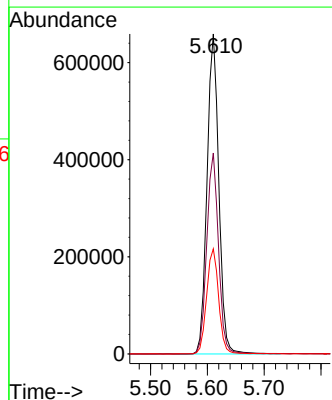
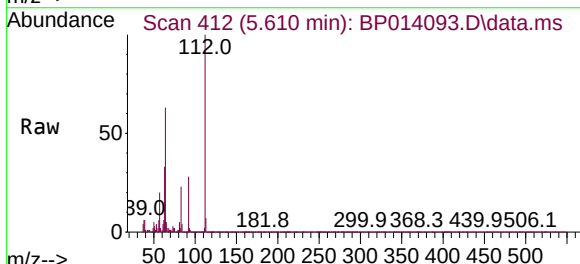


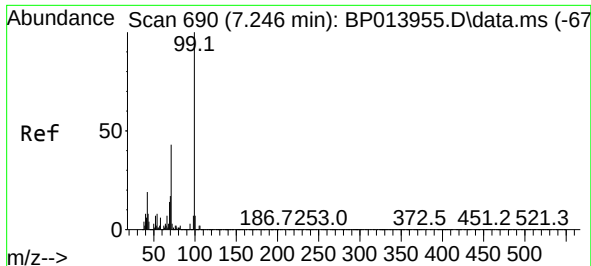

#7
Phenol-d6
Concen: 126.355 ng
RT: 7.222 min Scan# 68
Delta R.T. -0.006 min
Lab File: BP014093.D
Acq: 14 Mar 2023 21:09




Instrument :
BNA_P
ClientSampleId :
MAPLE-2


Tgt Ion: 99 Resp: 1114300
Ion Ratio Lower Upper
99 100
42 18.7 15.0 22.6
71 40.6 34.3 51.5

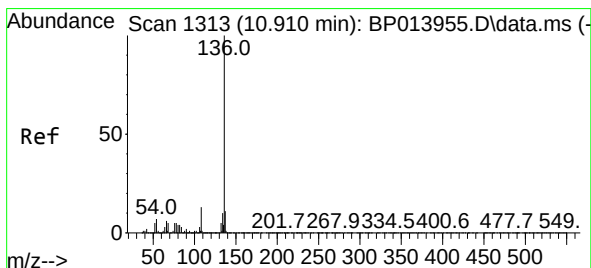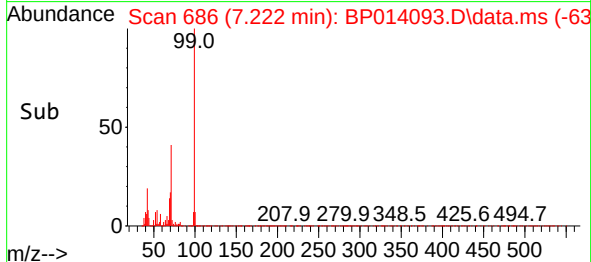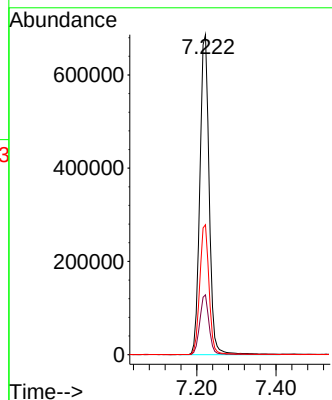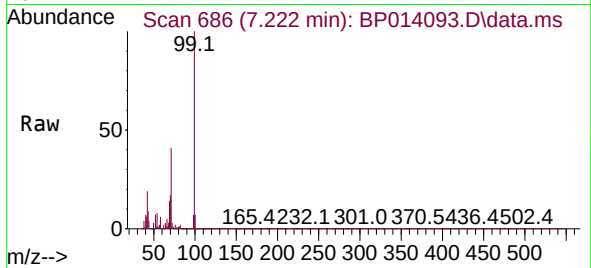

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.886 min Scan# 1309
Delta R.T. -0.012 min
Lab File: BP014093.D
Acq: 14 Mar 2023 21:09

Tgt Ion: 136 Resp: 396656
Ion Ratio Lower Upper
136 100
137 10.6 8.7 13.1
54 8.7 5.8 8.8
68 6.3 4.0 6.0#


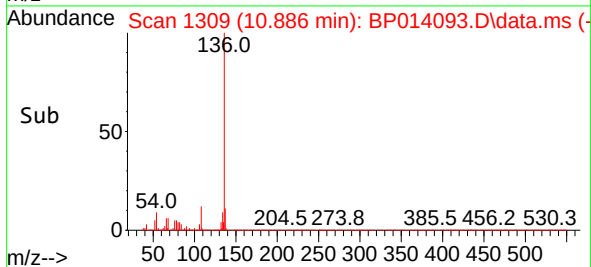
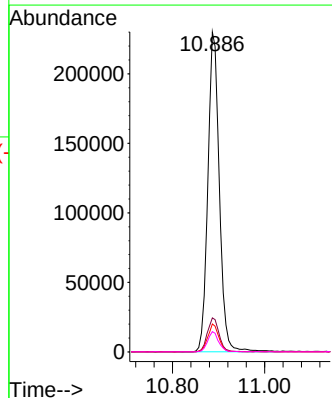
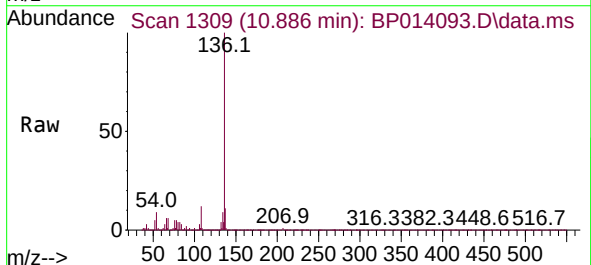


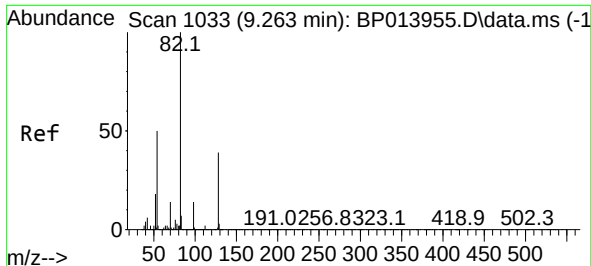

#23
Nitrobenzene-d5
Concen: 100.144 ng
RT: 9.239 min Scan# 1029
Delta R.T. -0.012 min
Lab File: BP014093.D
Acq: 14 Mar 2023 21:09




Instrument :
BNA_P
ClientSampleId :
MAPLE-2


Tgt Ion: 82 Resp: 869102
Ion Ratio Lower Upper
82 100
128 38.3 31.1 46.7
54 49.6 40.0 60.0

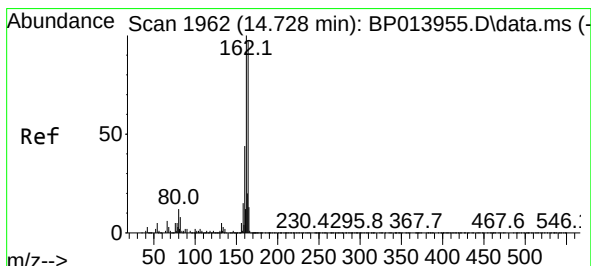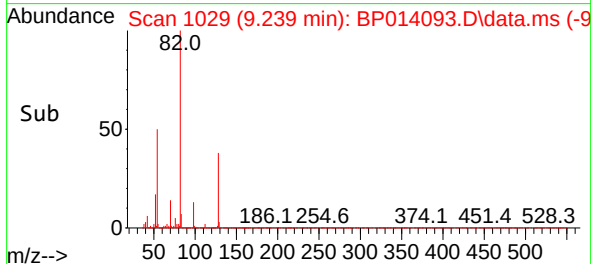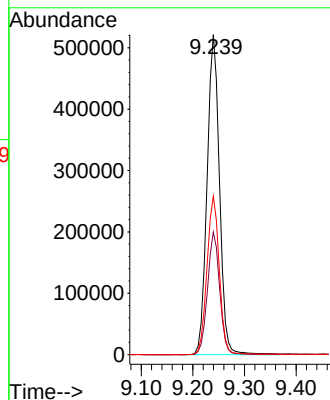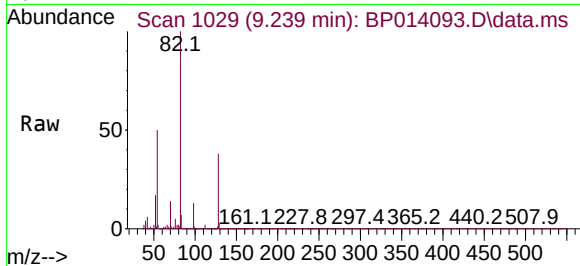

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.704 min Scan# 1958
Delta R.T. -0.012 min
Lab File: BP014093.D
Acq: 14 Mar 2023 21:09

Tgt Ion: 164 Resp: 237156
Ion Ratio Lower Upper
164 100
162 103.8 82.1 123.1
160 46.9 36.2 54.2


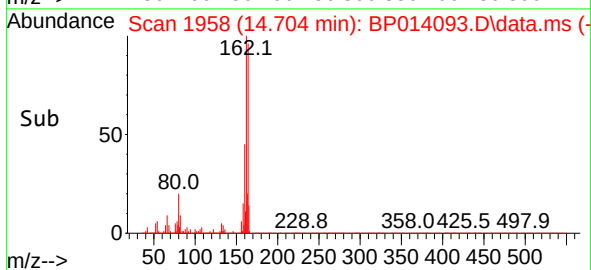
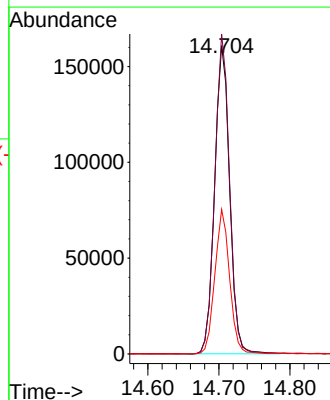
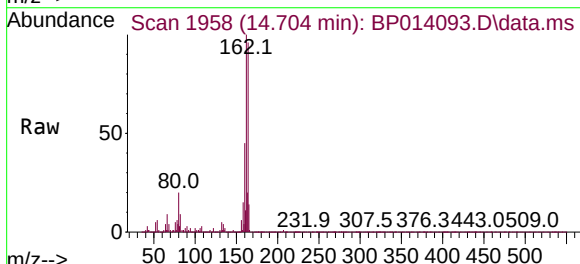


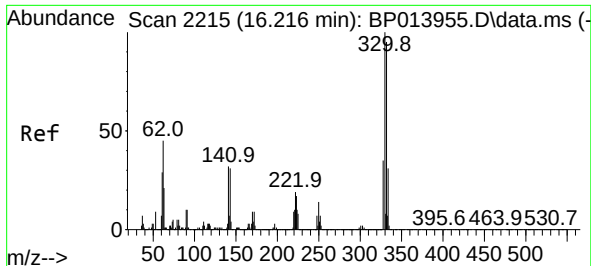

#42
2,4,6-Tribromophenol
Concen: 138.669 ng
RT: 16.198 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP014093.D
Acq: 14 Mar 2023 21:09




Instrument :
BNA_P
ClientSampleId :
MAPLE-2


Tgt Ion:330 Resp: 533202
Ion Ratio Lower Upper
330 100
332 97.1 77.1 115.7
141 33.2 25.6 38.4

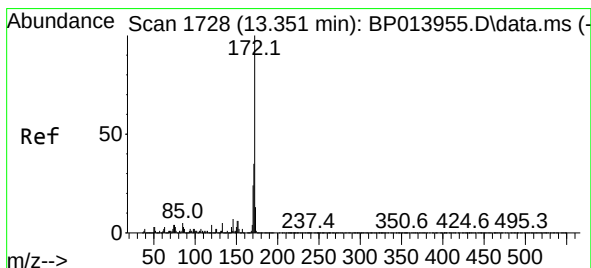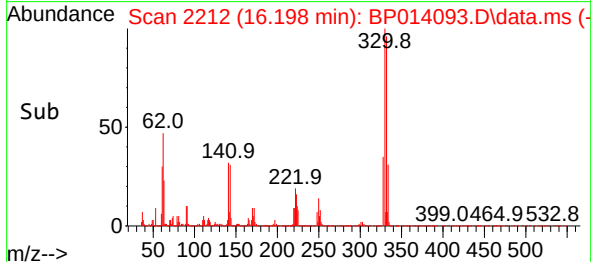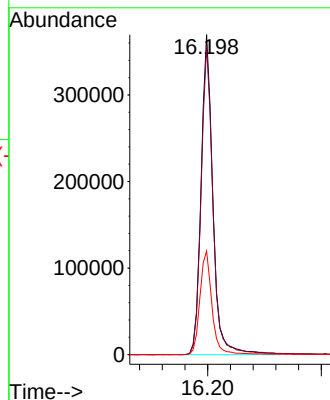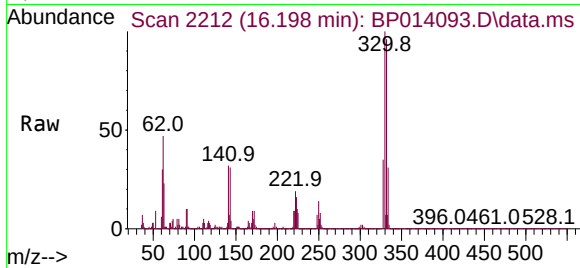

#45
2-Fluorobiphenyl
Concen: 98.806 ng
RT: 13.327 min Scan# 1724
Delta R.T. -0.012 min
Lab File: BP014093.D
Acq: 14 Mar 2023 21:09

Tgt Ion:172 Resp: 1808644
Ion Ratio Lower Upper
172 100
171 35.2 28.3 42.5
170 23.2 19.0 28.4

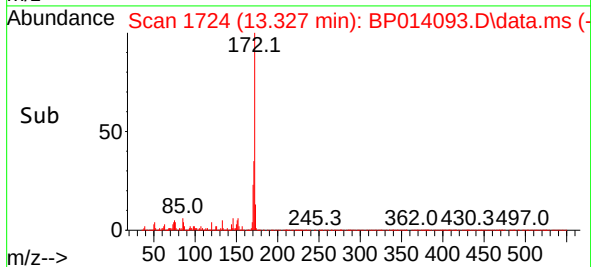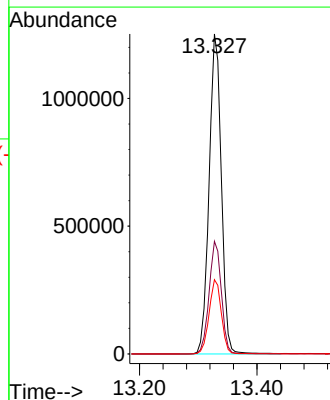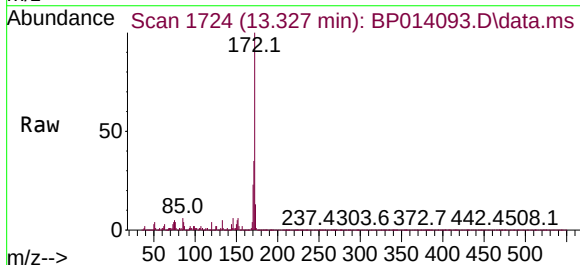

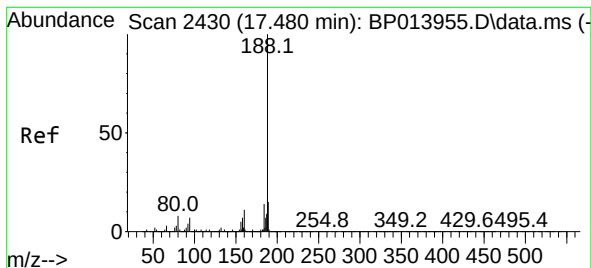

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.463 min Scan# 24

Delta R.T. -0.006 min

Lab File: BP014093.D

Acq: 14 Mar 2023 21:09

Instrument :

BNA_P

ClientSampleId :

MAPLE-2





Tgt Ion:188 Resp: 508273

Ion Ratio Lower Upper

188 100

94 8.5 5.8 8.6

80 9.8 6.6 9.8

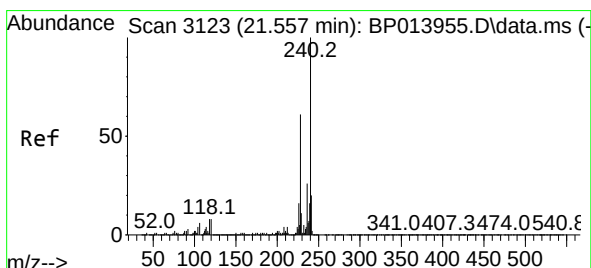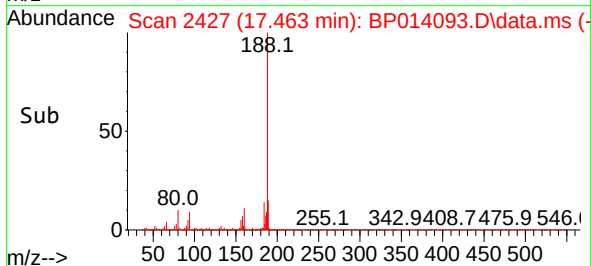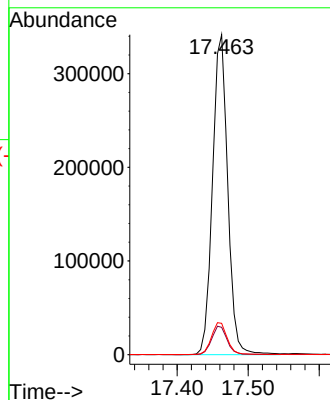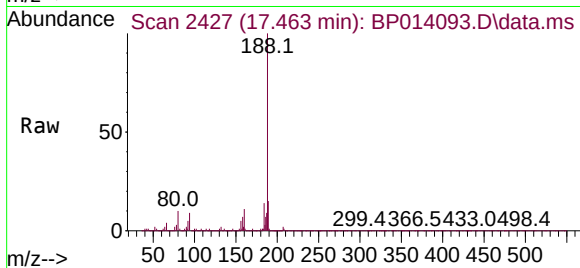

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.539 min Scan# 3120

Delta R.T. -0.006 min

Lab File: BP014093.D

Acq: 14 Mar 2023 21:09




Tgt Ion:240 Resp: 488768


Ion Ratio Lower Upper

240 100

120 9.5 6.4 9.6

236 25.6 21.2 31.8

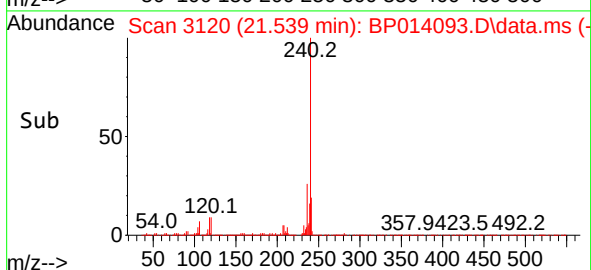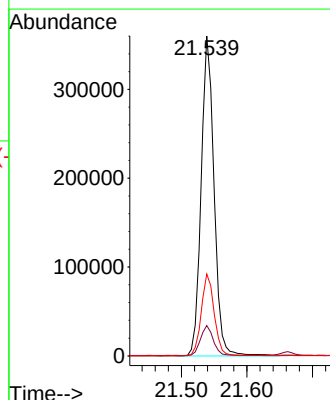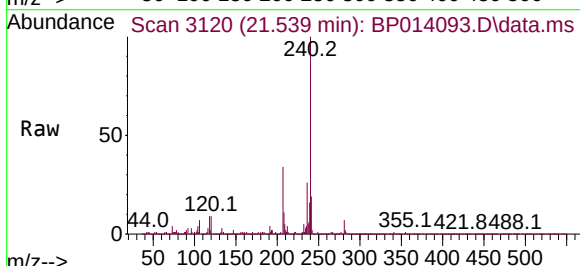

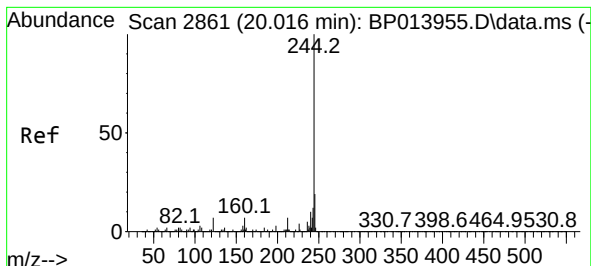

#79

Terphenyl-d14

Concen: 100.260 ng

RT: 19.998 min Scan# 2861

Delta R.T. -0.006 min

Lab File: BP014093.D

Acq: 14 Mar 2023 21:09

Instrument :

BNA_P

ClientSampleId :

MAPLE-2





Tgt Ion:244 Resp: 2971827

Ion Ratio Lower Upper

244 100

212 7.4 6.0 9.0

122 8.7 5.8 8.6#

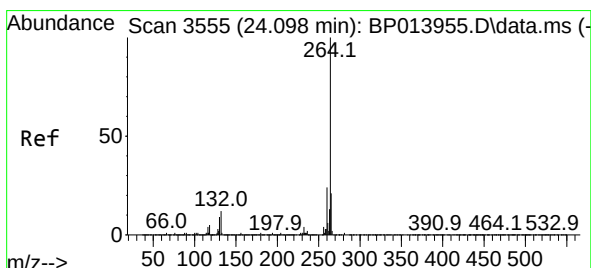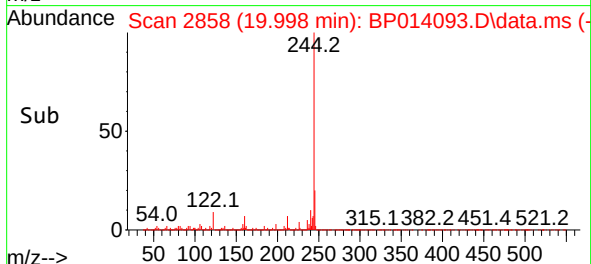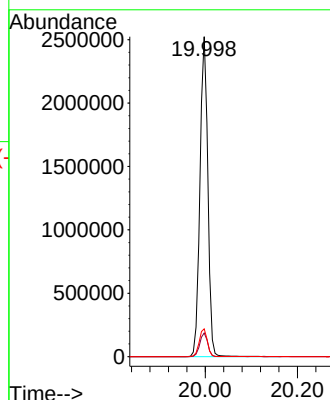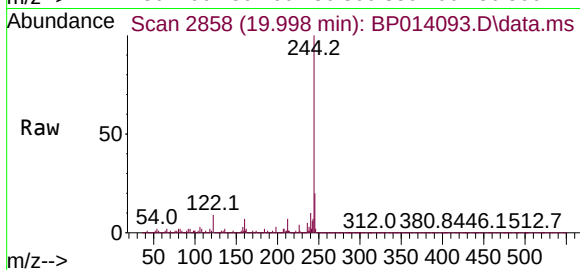

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.074 min Scan# 3551

Delta R.T. -0.006 min

Lab File: BP014093.D

Acq: 14 Mar 2023 21:09

Tgt Ion:264 Resp: 512559

Ion Ratio Lower Upper

264 100

260 24.0 19.4 29.2

265 22.5 17.8 26.8

