

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
 Data File : BP014077.D
 Acq On : 14 Mar 2023 10:58
 Operator : CG/JU
 Sample : PB151373BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB151373BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP014077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.146	327	333	345	rBV	1740114	2466616	23.29%	4.328%
2	5.617	406	413	431	rBV	4386916	6421670	60.63%	11.268%
3	7.228	679	687	701	rBV	4101161	6537634	61.72%	11.471%
4	8.069	822	830	843	rBV	782929	1237396	11.68%	2.171%
5	9.246	1022	1030	1045	rBV	2493310	4211115	39.76%	7.389%
6	10.893	1302	1310	1327	rBV	914792	1612847	15.23%	2.830%
7	13.334	1717	1725	1743	rBV	6304256	9234624	87.18%	16.204%
8	14.710	1951	1959	1972	rBV	1415389	2095738	19.79%	3.677%
9	16.198	2202	2212	2234	rBV	4712304	6991166	66.00%	12.267%
10	17.463	2420	2427	2439	rBV	1616863	2332444	22.02%	4.093%
11	19.998	2853	2858	2873	rBV	8492872	10592129	100.00%	18.586%
12	21.545	3116	3121	3129	rBV	1281719	1809054	17.08%	3.174%
13	24.080	3546	3552	3563	rVB2	673945	1448123	13.67%	2.541%




Sum of corrected areas: 56990556

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014077.D
Acq On : 14 Mar 2023 10:58
Operator : CG/JU
Sample : PB151373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB151373BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

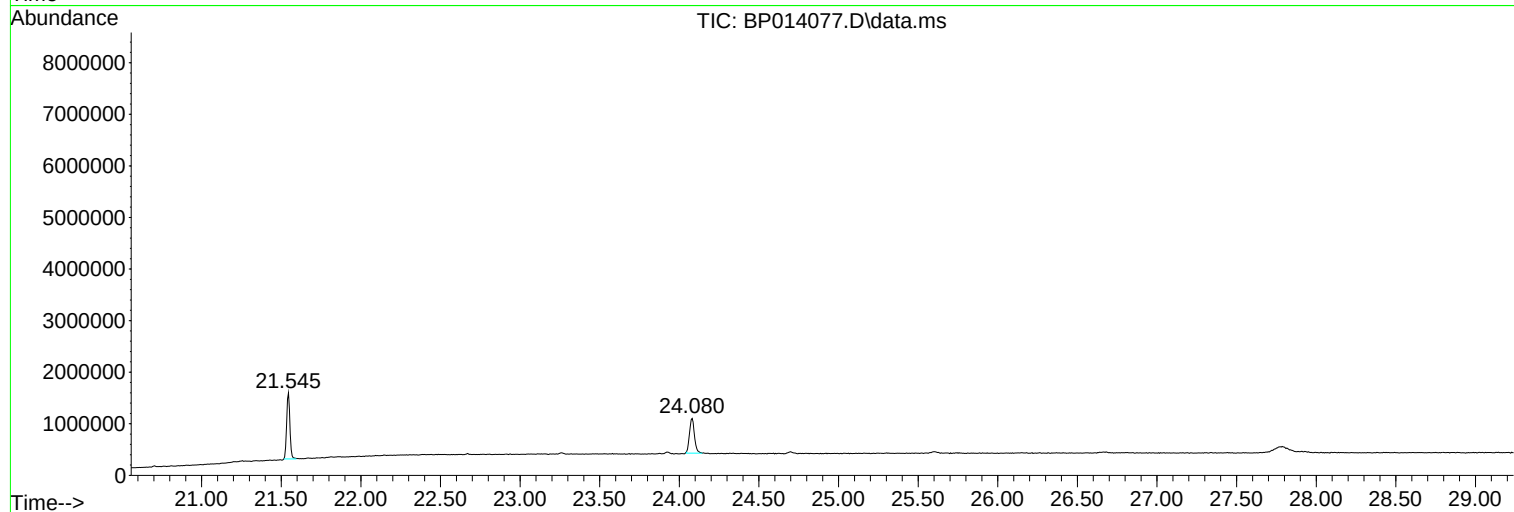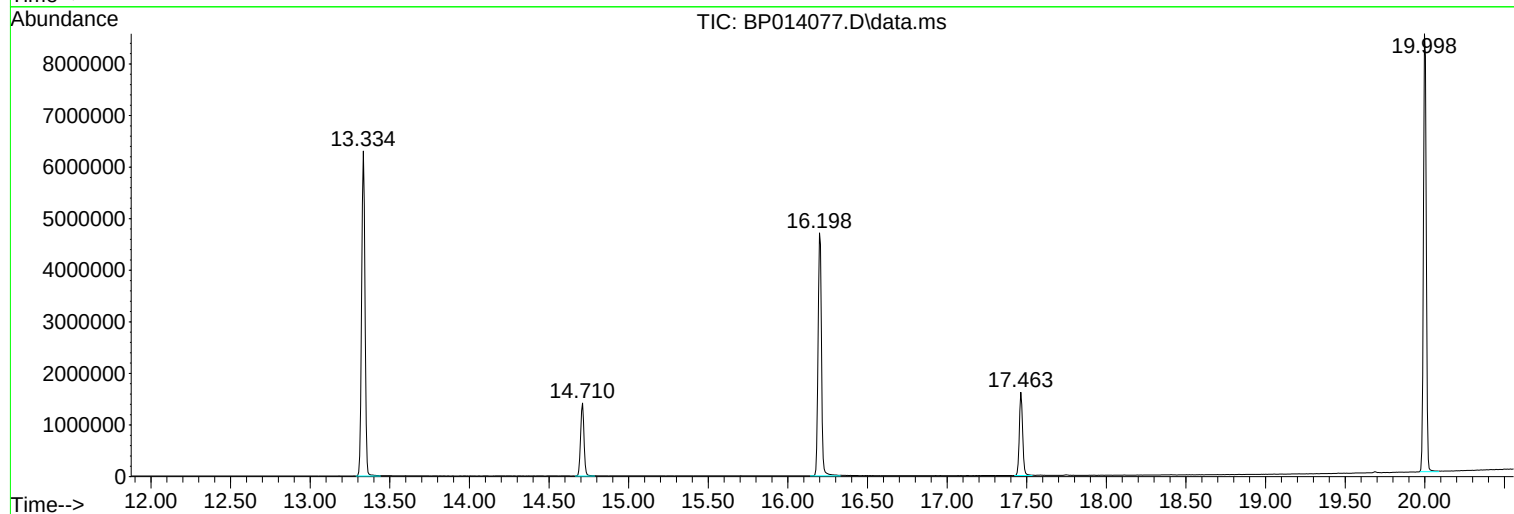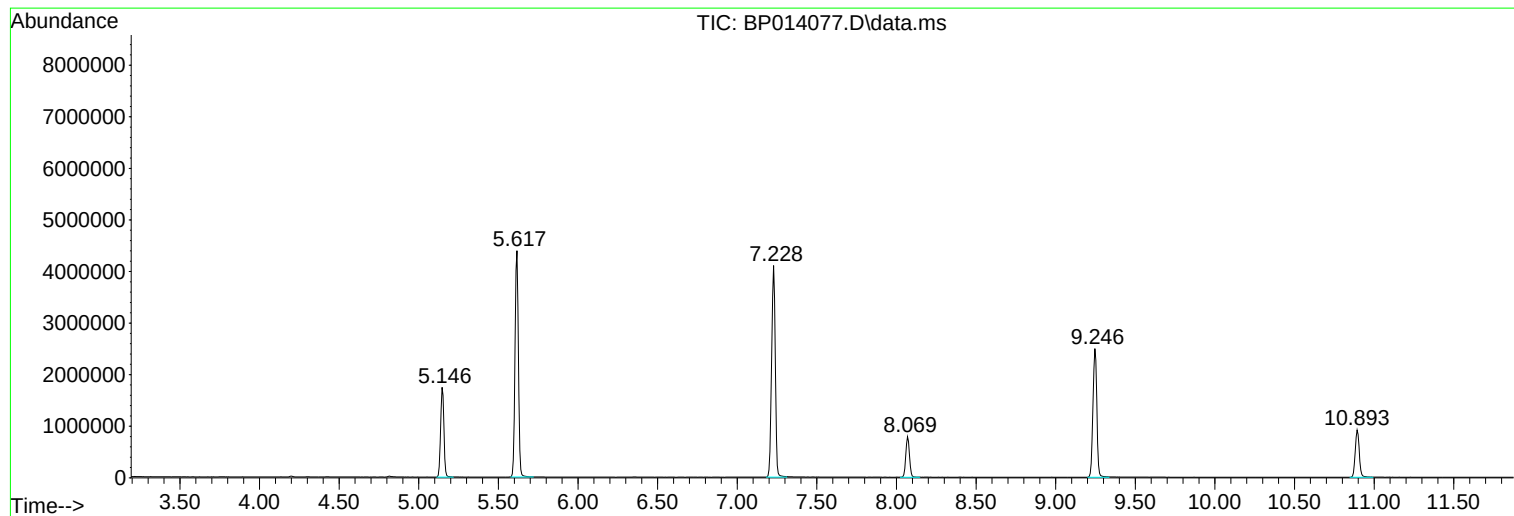

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014077.D
Acq On : 14 Mar 2023 10:58
Operator : CG/JU
Sample : PB151373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB151373BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.146	39.87 ng	2466620	1,4-Dichlorobenzene-d4	8.069

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5			5-Hexen-2-one	98	C6H10O	000109-49-9	9

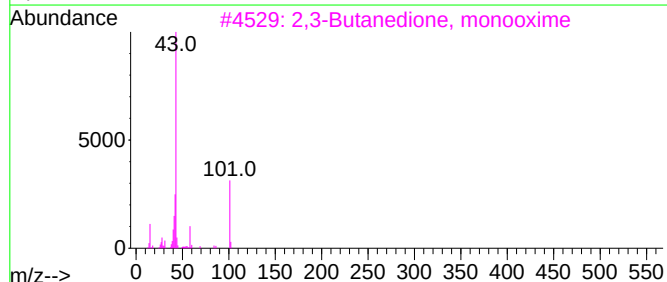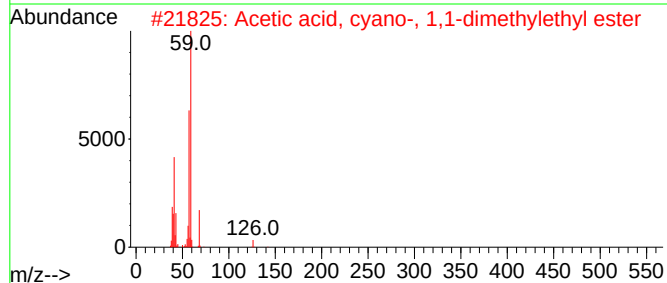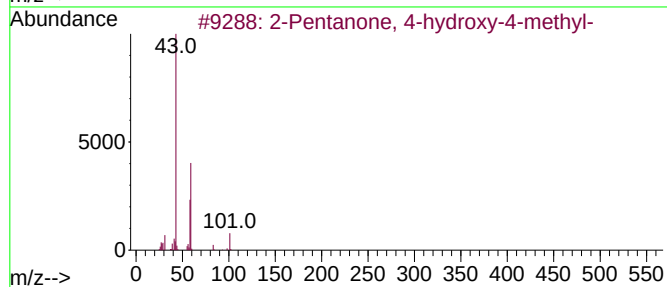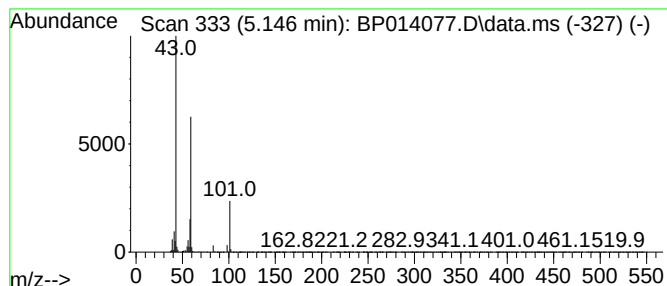

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014077.D
Acq On : 14 Mar 2023 10:58
Operator : CG/JU
Sample : PB151373BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB151373BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.146	39.9	ng	2466620	1	8.069	1237400	20.0