


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014075.D
Acq On : 14 Mar 2023 09:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 14 04:15:47 2023

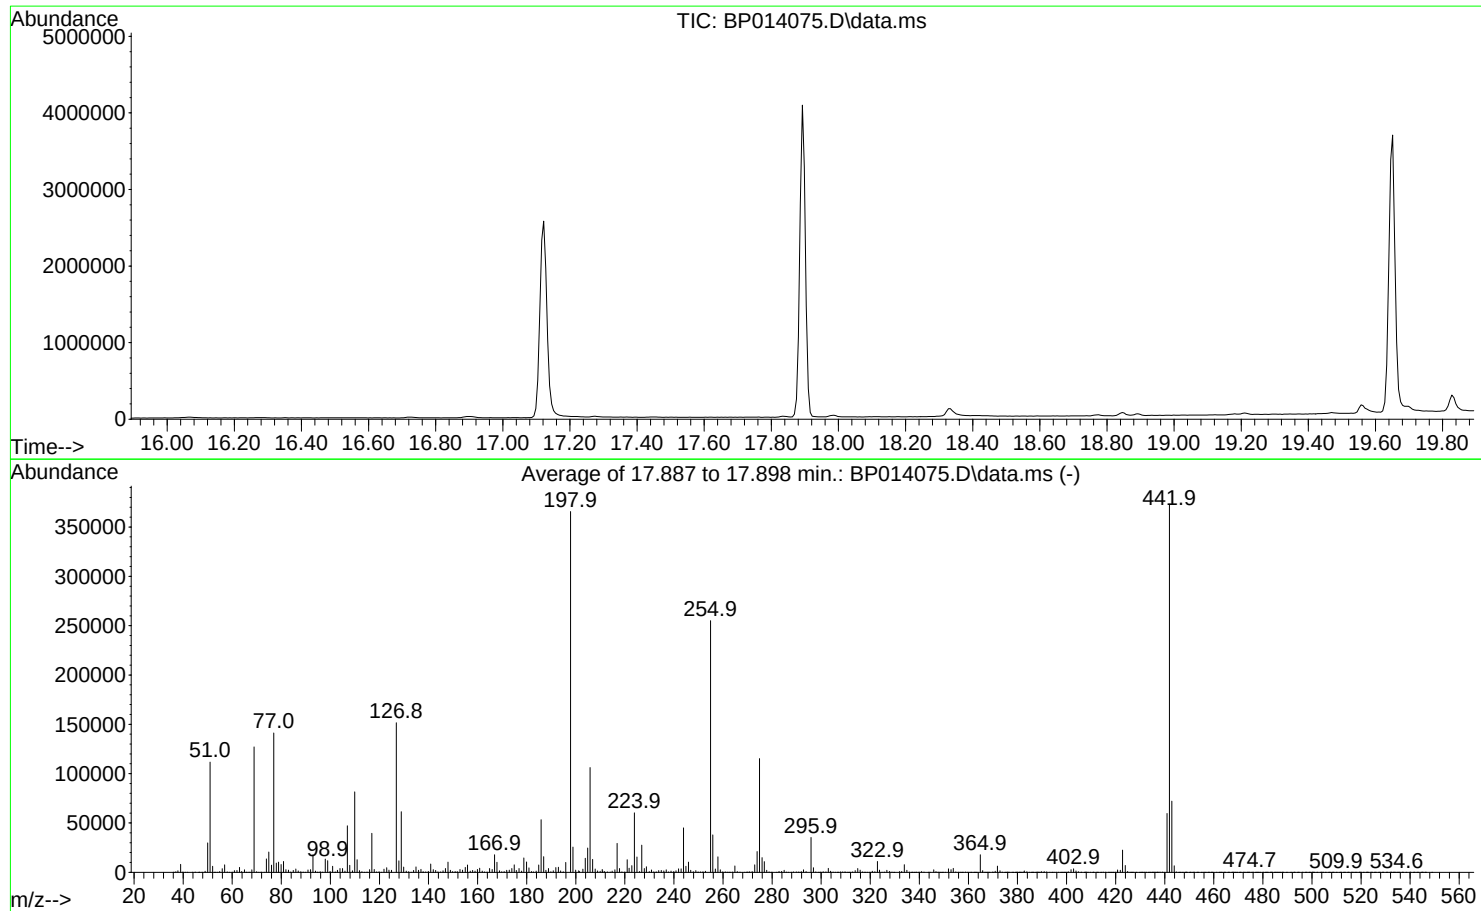




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	111658	PASS
68	69	0.00	2	1.9	2450	PASS
69	198	0.00	100	34.8	127123	PASS
70	69	0.00	2	0.5	655	PASS
127	198	10	80	41.4	151559	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	365766	PASS
199	198	5	9	7.0	25520	PASS
275	198	10	60	31.5	115231	PASS
365	198	1	100	4.9	17855	PASS
441	198	0.01	100	16.3	59701	PASS
442	442	100	100	100.0	372928	PASS
443	442	15	24	19.3	72125	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014075.D
Acq On : 14 Mar 2023 09:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 15 05:42:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 04:15:47 2023
Response via : Initial Calibration

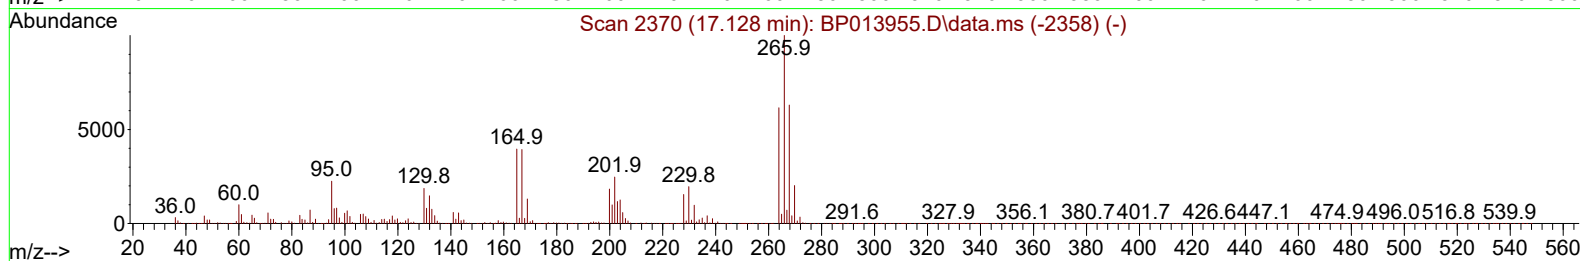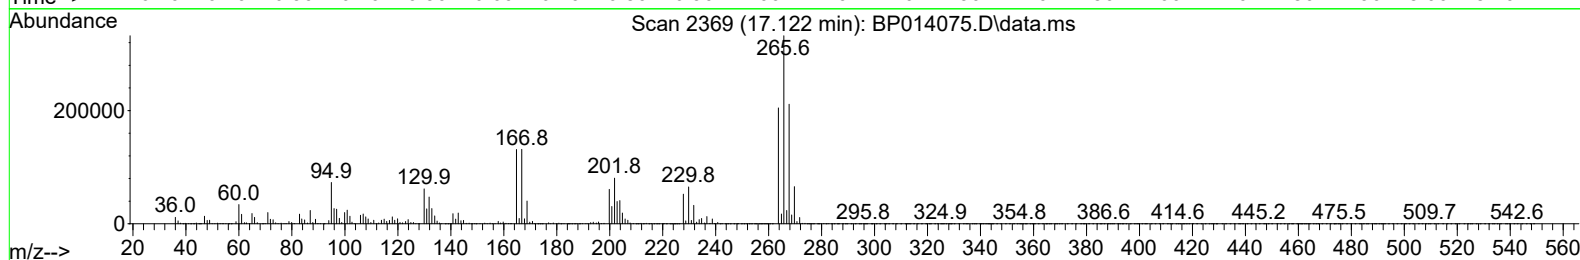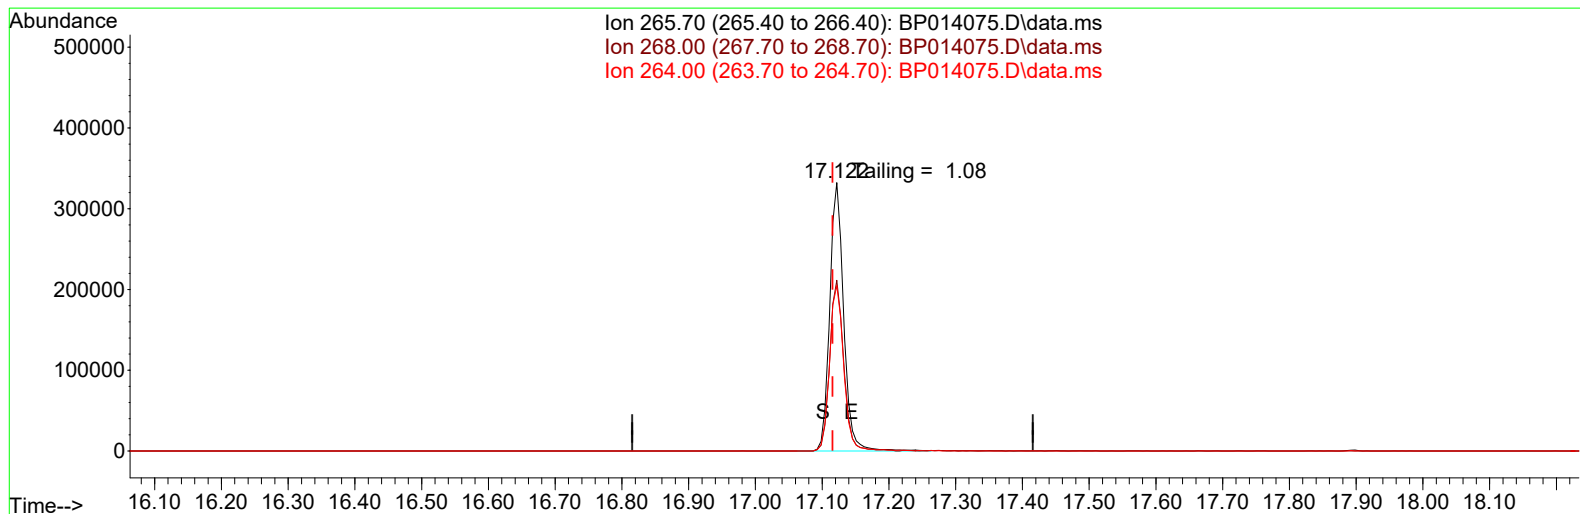

TIC: BP014075.D\data.ms

(70) Pentachlorophenol (C)

17.122min (+ 0.006) 177815.86 ng




response 481834

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	68.25
264.00	61.50	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014075.D
Acq On : 14 Mar 2023 09:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 15 05:42:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 04:15:47 2023
Response via : Initial Calibration

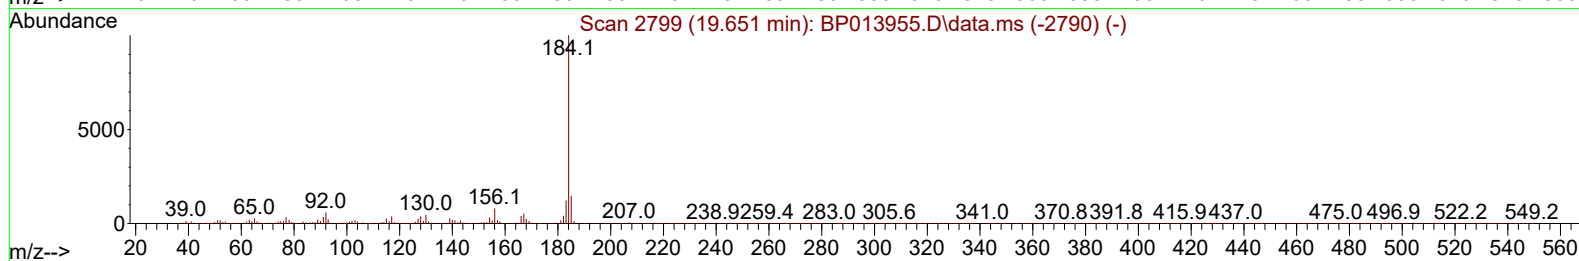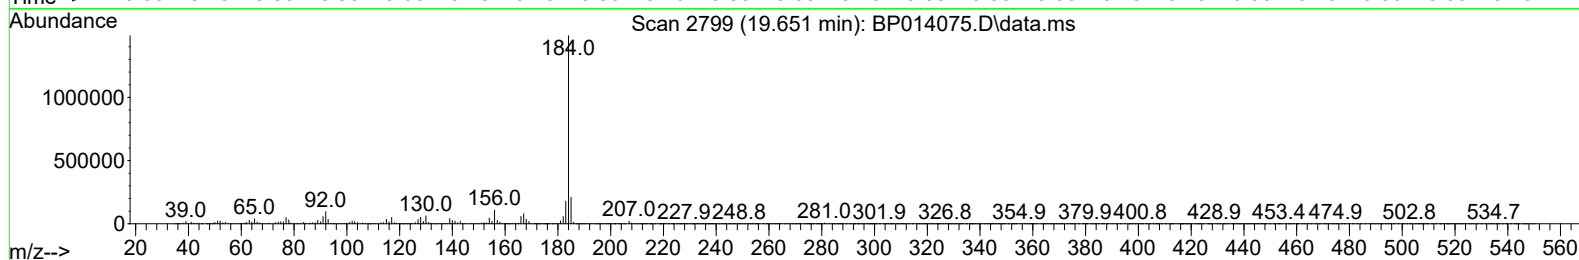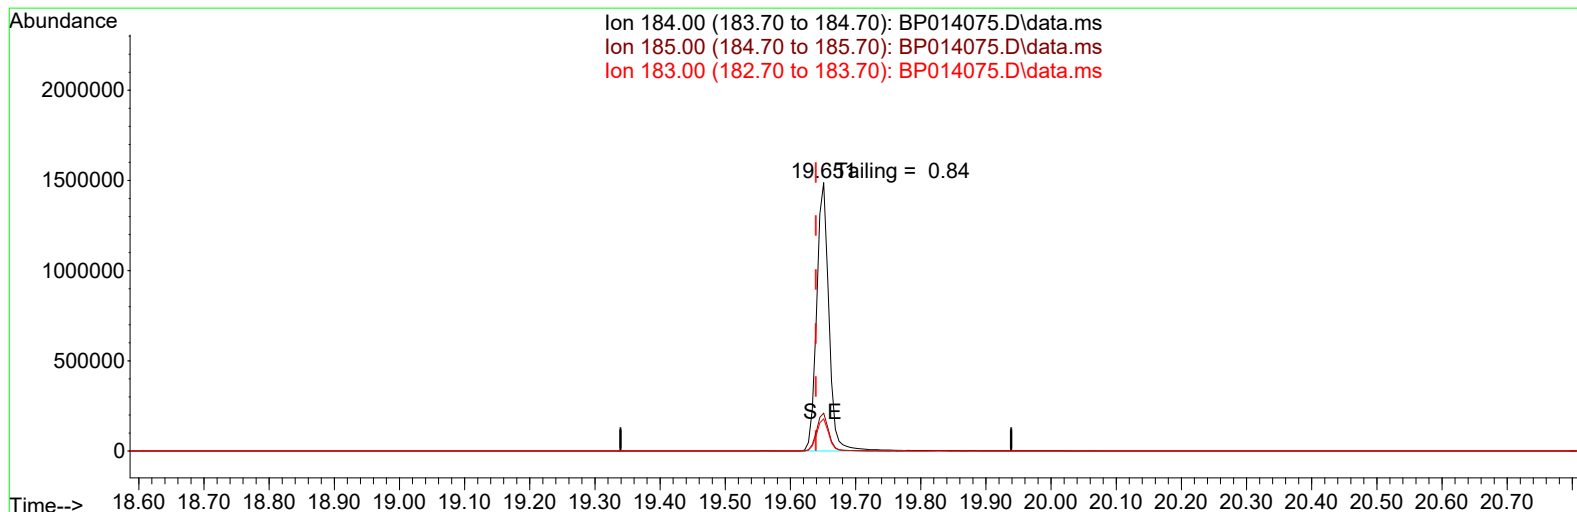

TIC: BP014075.D\data.ms

(77) Benzidine

19.651min (+ 0.012) -20.00 ng

response 1952243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.13
183.00	12.10	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2023	BNA_P	<u>BP014075.D</u>
Compound Name	Response	Retention Time
DDT	1142786	20.845
DDD	14750	20.463
DDE	881	19.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15631	1158417	1.35

Instrument :
BNA_P
ClientSampleId :
DFTPP