


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
Data File : BP014084.D
Acq On : 14 Mar 2023 15:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 14 04:15:47 2023

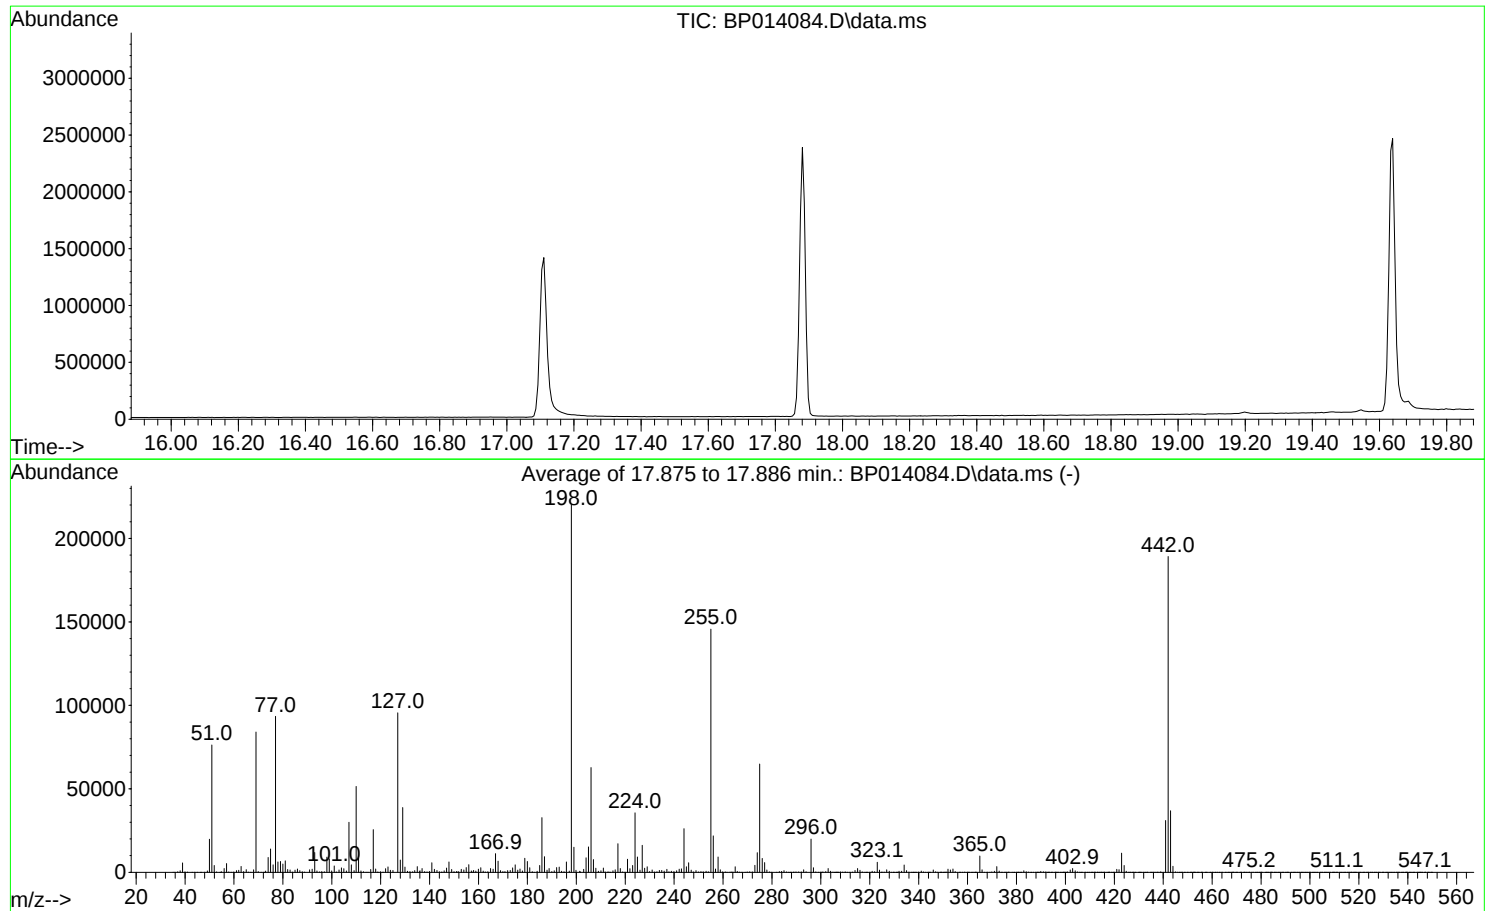




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	76256	PASS
68	69	0.00	2	1.8	1542	PASS
69	198	0.00	100	38.1	84041	PASS
70	69	0.00	2	0.5	392	PASS
127	198	10	80	43.3	95501	PASS
197	198	0.00	2	0.3	699	PASS
198	198	100	100	100.0	220373	PASS
199	198	5	9	6.8	15043	PASS
275	198	10	60	29.4	64861	PASS
365	198	1	100	4.4	9763	PASS
441	198	0.01	100	14.1	30989	PASS
442	442	100	100	100.0	189155	PASS
443	442	15	24	19.5	36816	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031423\
 Data File : BP014084.D
 Acq On : 14 Mar 2023 15:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 15 05:43:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 04:15:47 2023
 Response via : Initial Calibration

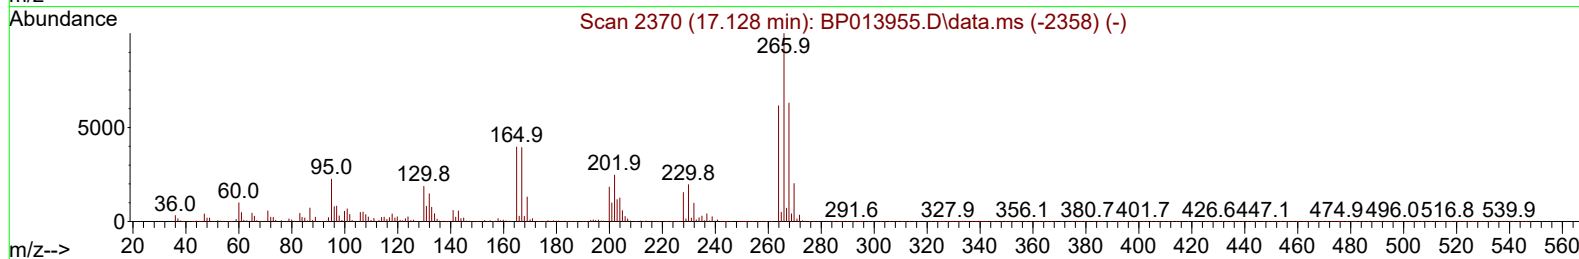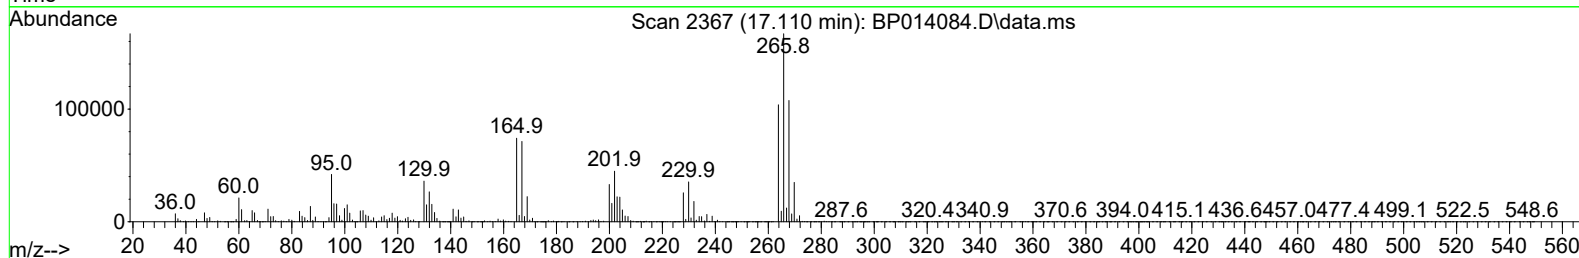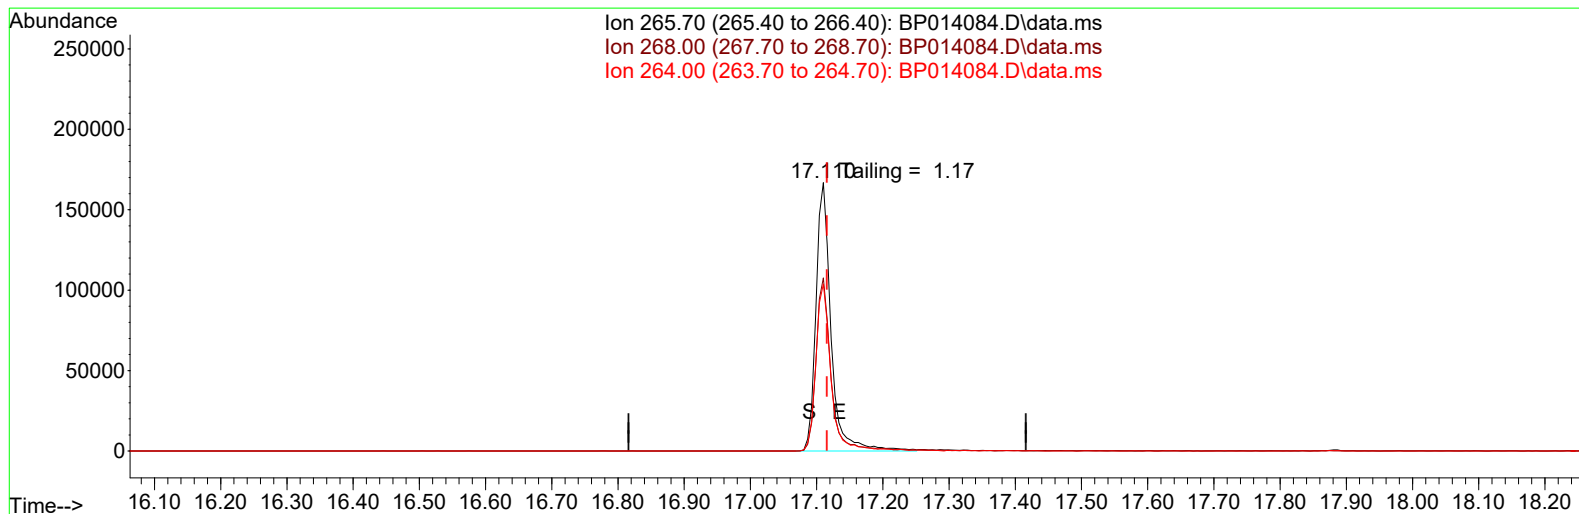

TIC: BP014084.D\data.ms

(70) Pentachlorophenol (C)

17.110min (-0.006) 1173106.07 ng

response 263901

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.52
264.00	61.50	62.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2023	BNA_P	<u>BP014084.D</u>
Compound Name	Response	Retention Time
DDT	716366	20.833
DDD	9117	20.457
DDE	500	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9617	725983	1.32

Instrument :
BNA_P
ClientSampleId :
DFTPP