
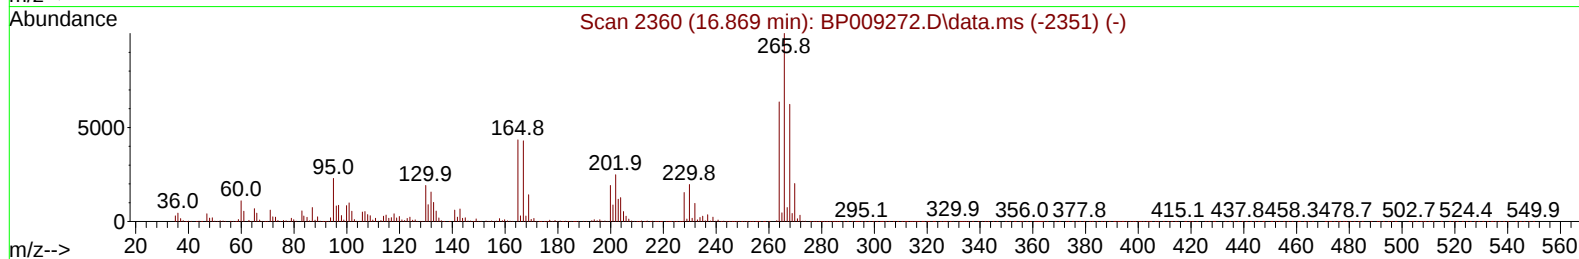
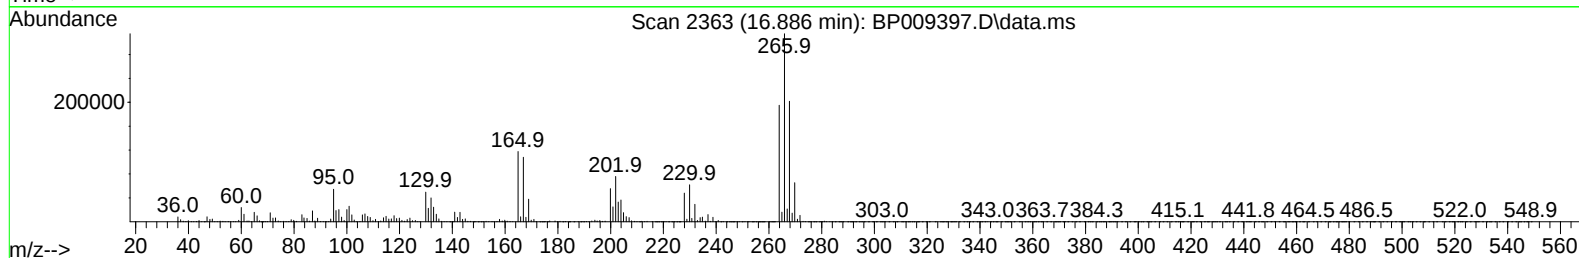


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
Data File : BP009397.D
Acq On : 15 Mar 2022 14:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 07:15:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 01:55:59 2022
Response via : Initial Calibration

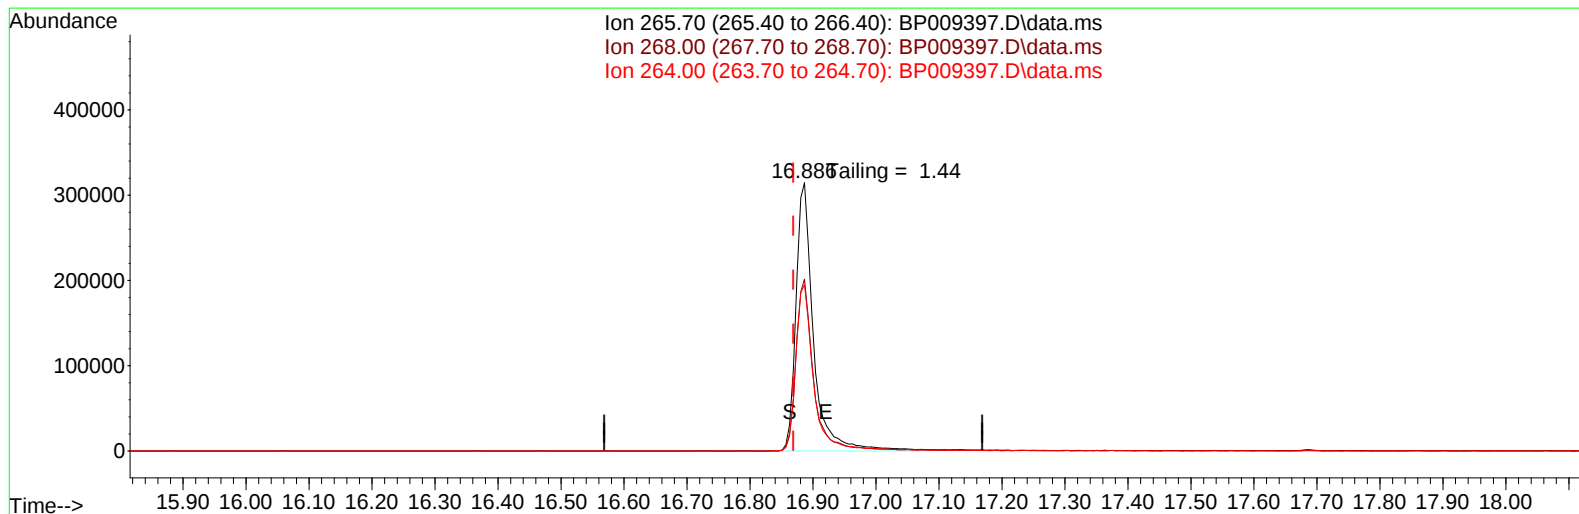

TIC: BP009397.D\data.ms

(70) Pentachlorophenol (C)




16.886min (+ 0.018) 49392.43 ng

response 616958

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.05
264.00	63.60	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
 Data File : BP009397.D
 Acq On : 15 Mar 2022 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 07:15:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

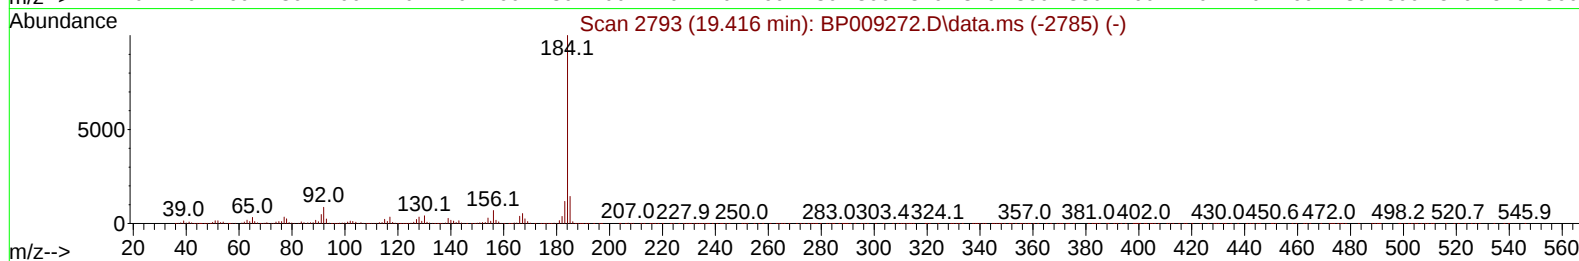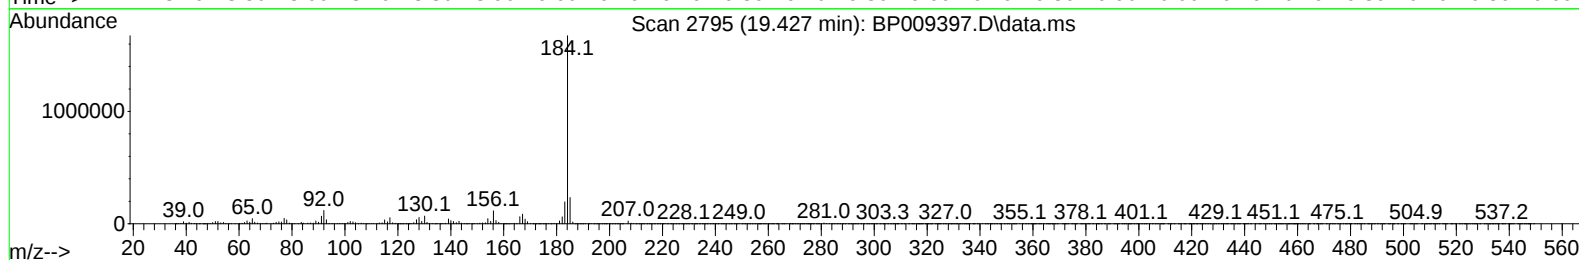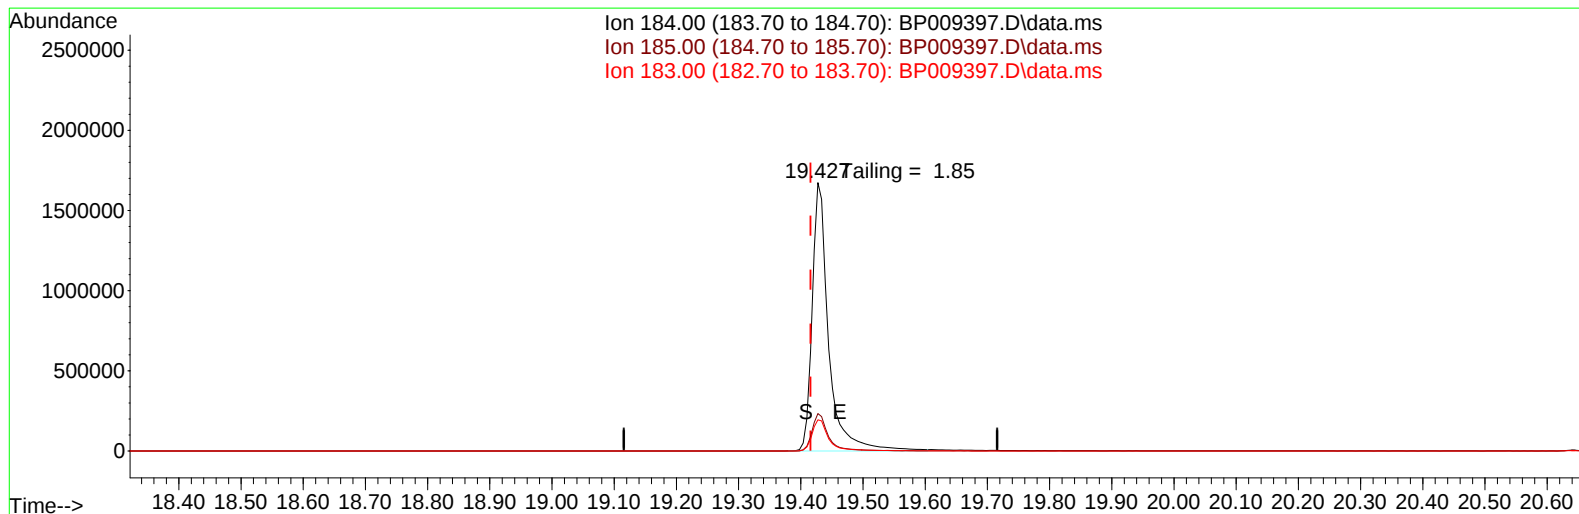

TIC: BP009397.D\data.ms

(77) Benzidine**19.427min (+ 0.012) 10325.48 ng****response 3097634**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	11.70	11.65
0.00	0.00	0.00