

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
 Data File : BP009399.D
 Acq On : 15 Mar 2022 15:39
 Operator : CG/JU
 Sample : PB143311BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143311BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	406	414	432	rBV	5006009	8445839	50.23%	10.531%
2	7.005	675	683	713	rBV	4577848	8412178	50.03%	10.489%
3	7.811	812	820	830	rBV	1001673	1695560	10.08%	2.114%
4	8.969	1008	1017	1037	rBV	3101915	5647121	33.58%	7.041%
5	10.605	1286	1295	1308	rBV	1159707	2273228	13.52%	2.835%
6	13.075	1707	1715	1740	rBV	8252276	13908383	82.71%	17.343%
7	14.457	1941	1950	1968	rBV	1637859	3046864	18.12%	3.799%
8	15.951	2197	2204	2237	rBV	4860287	10093267	60.02%	12.585%
9	17.216	2411	2419	2435	rBV	1875160	3387187	20.14%	4.224%
10	19.792	2851	2857	2872	rBV	12086228	16815469	100.00%	20.968%
11	21.327	3113	3118	3130	rBV	1963508	3210040	19.09%	4.003%
12	23.739	3521	3528	3541	rVB2	1276628	3262566	19.40%	4.068%




Sum of corrected areas: 80197702

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
Data File : BP009399.D
Acq On : 15 Mar 2022 15:39
Operator : CG/JU
Sample : PB143311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

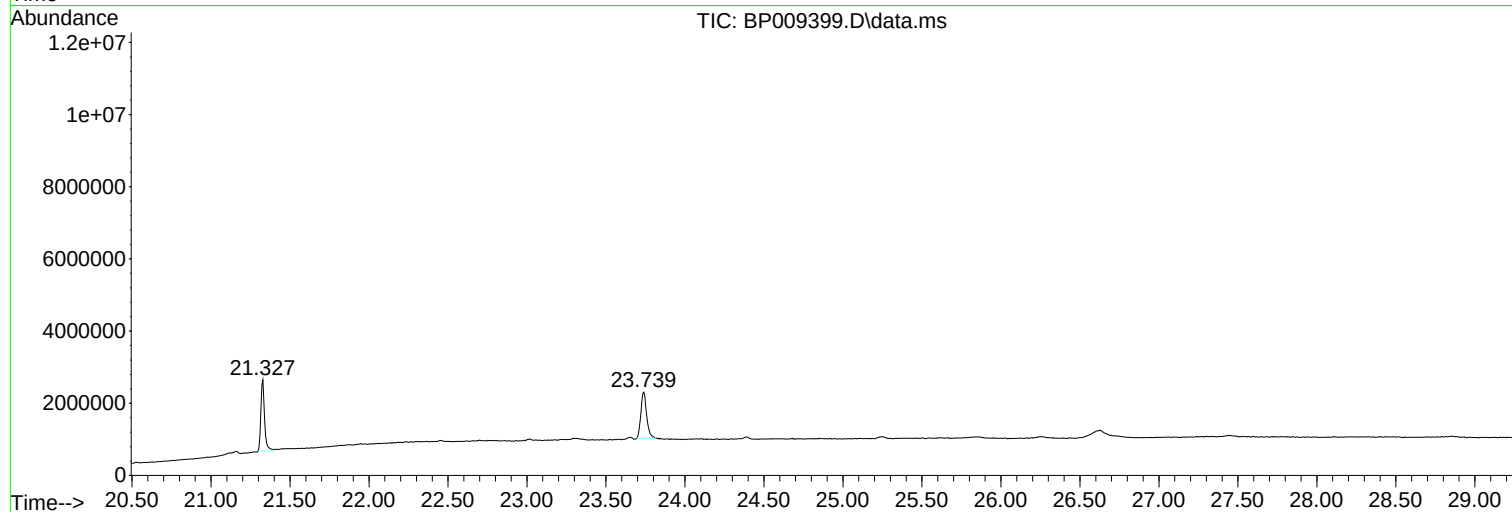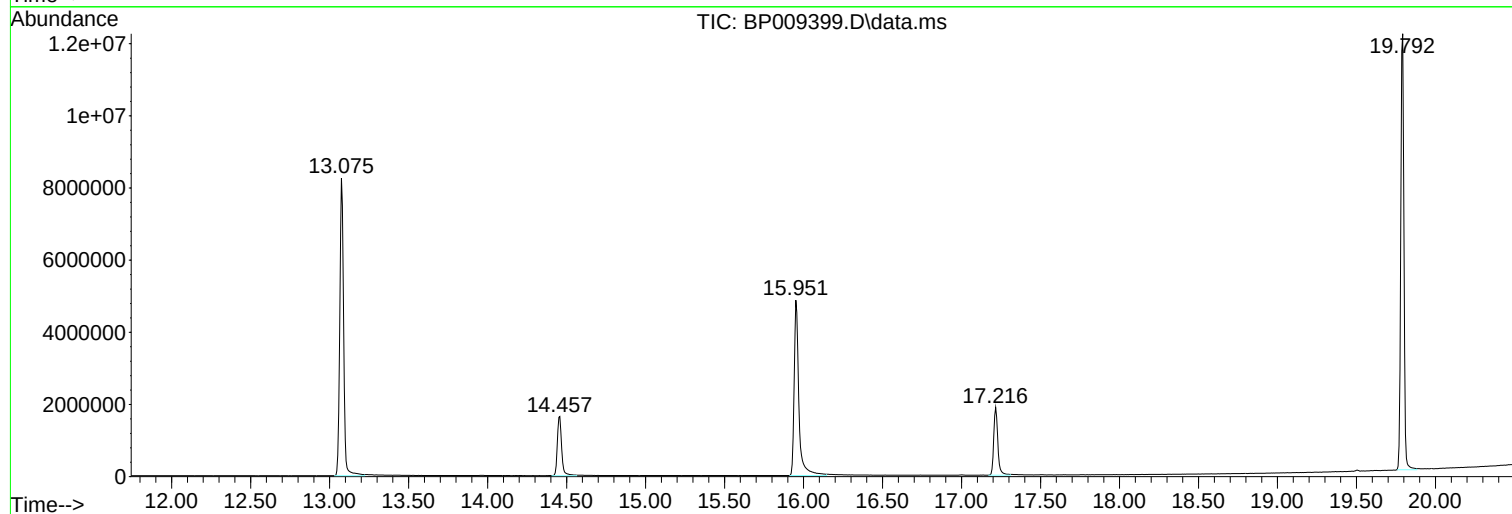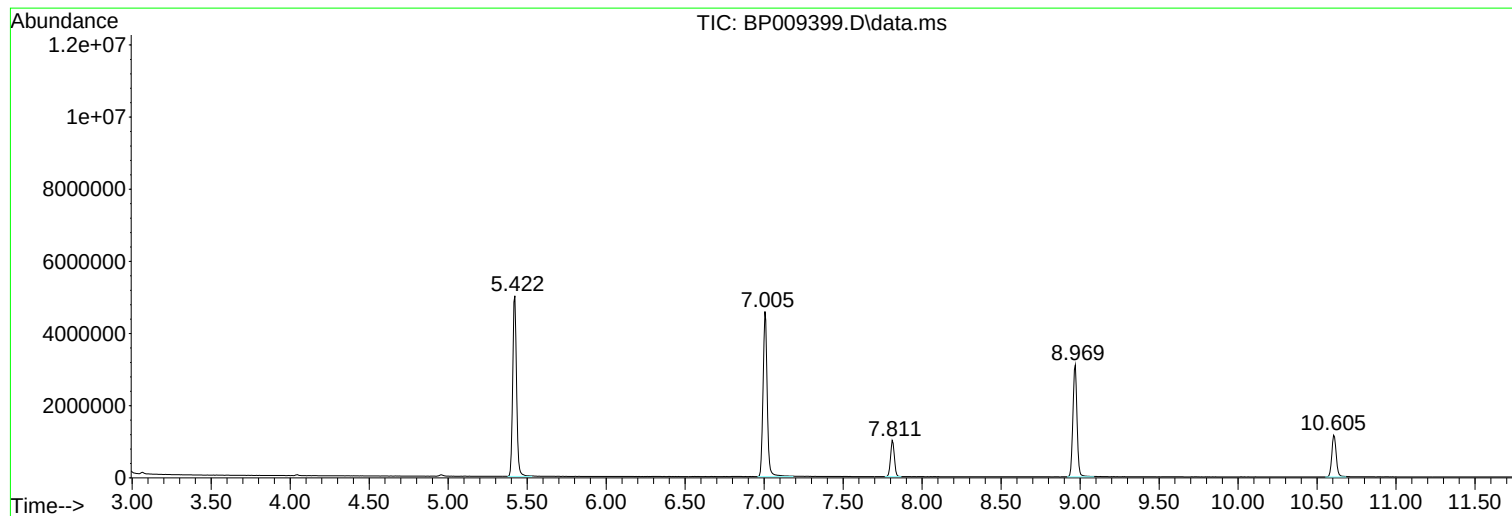

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
Data File : BP009399.D
Acq On : 15 Mar 2022 15:39
Operator : CG/JU
Sample : PB143311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
Data File : BP009399.D
Acq On : 15 Mar 2022 15:39
Operator : CG/JU
Sample : PB143311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------