
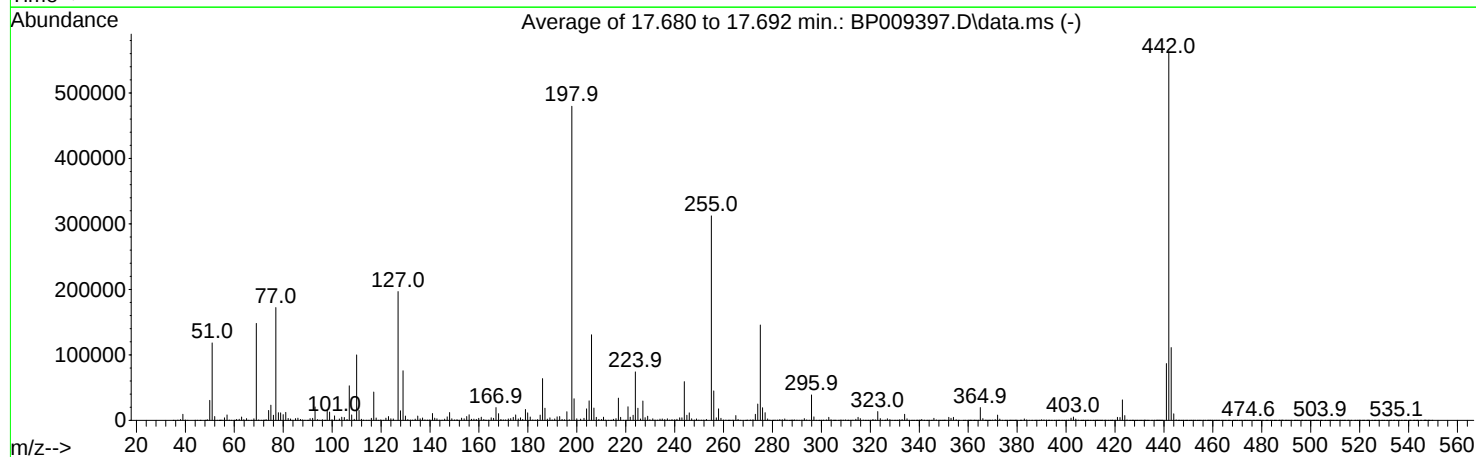


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
 Data File : BP009397.D
 Acq On : 15 Mar 2022 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 01:55:59 2022

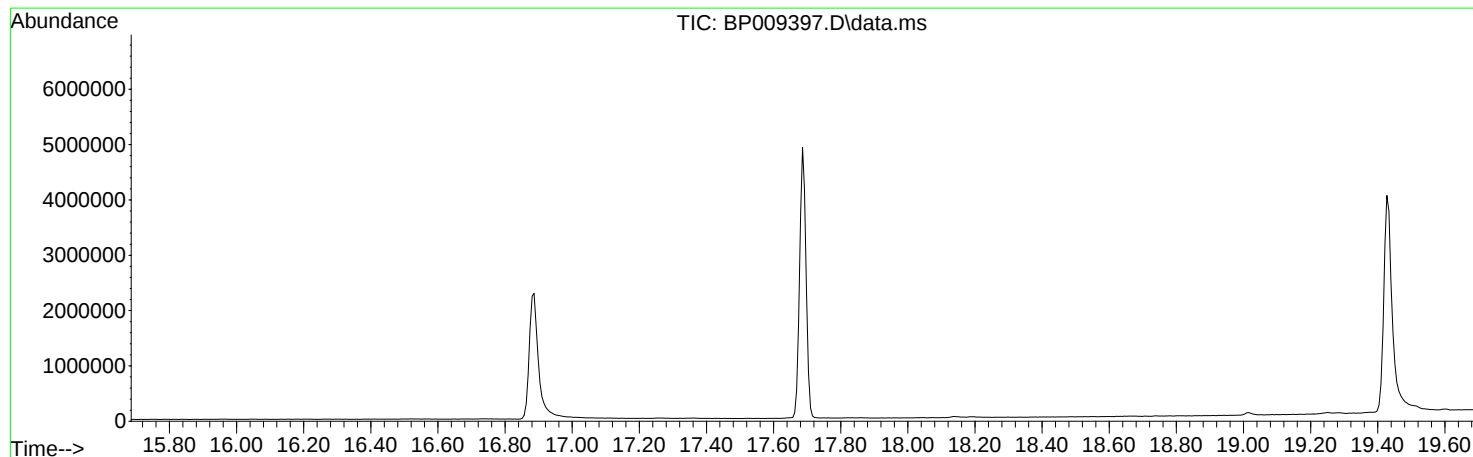




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	118207	PASS
68	69	0.00	2	1.7	2588	PASS
69	198	0.00	100	30.9	148166	PASS
70	69	0.00	2	0.5	735	PASS
127	198	10	80	41.0	196823	PASS
197	198	0.00	2	0.2	885	PASS
198	198	100	100	100.0	479612	PASS
199	198	5	9	6.9	33014	PASS
275	198	10	60	30.4	145667	PASS
365	198	1	100	4.1	19571	PASS
441	198	0.01	100	18.1	86832	PASS
442	442	100	100	100.0	561784	PASS
443	442	15	24	19.8	111107	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
 Data File : BP009397.D
 Acq On : 15 Mar 2022 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 16 07:15:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

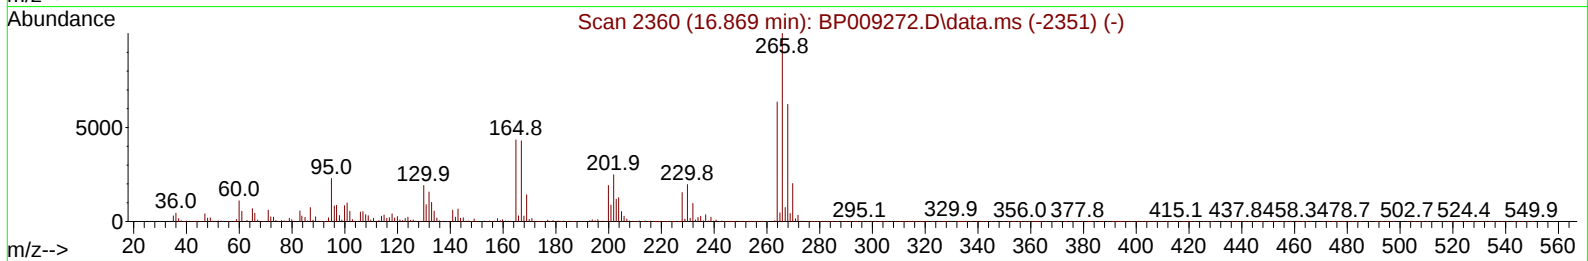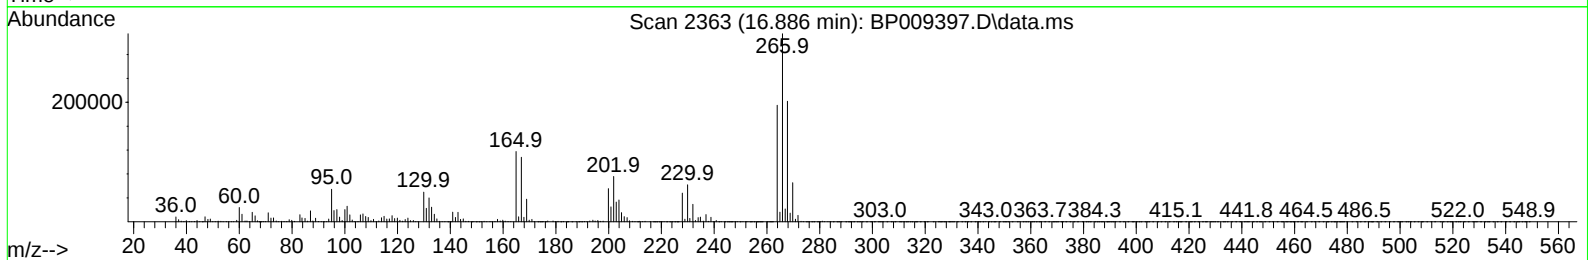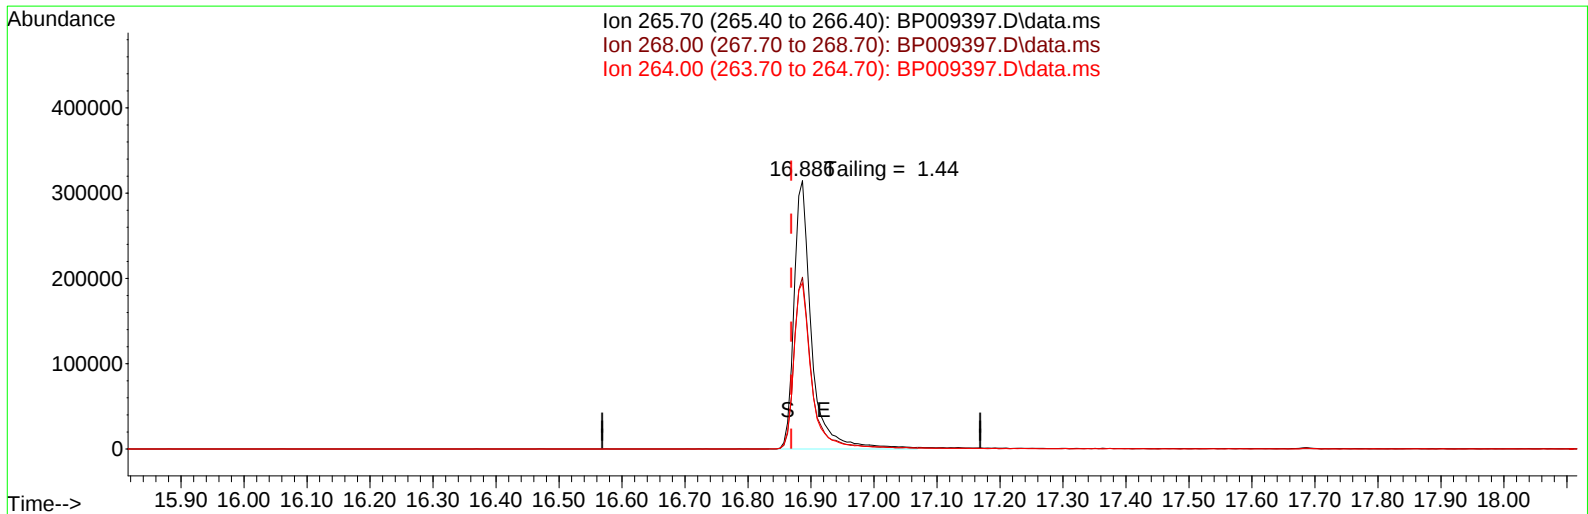

TIC: BP009397.D\data.ms

(70) Pentachlorophenol (C)

16.886min (+ 0.018) 49392.43 ng




response 616958

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.05
264.00	63.60	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031522\
 Data File : BP009397.D
 Acq On : 15 Mar 2022 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 16 07:15:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 01:55:59 2022
 Response via : Initial Calibration

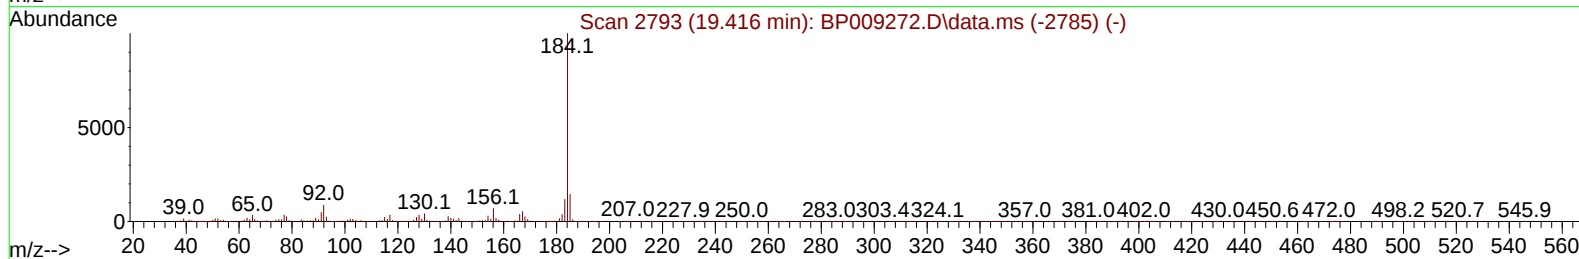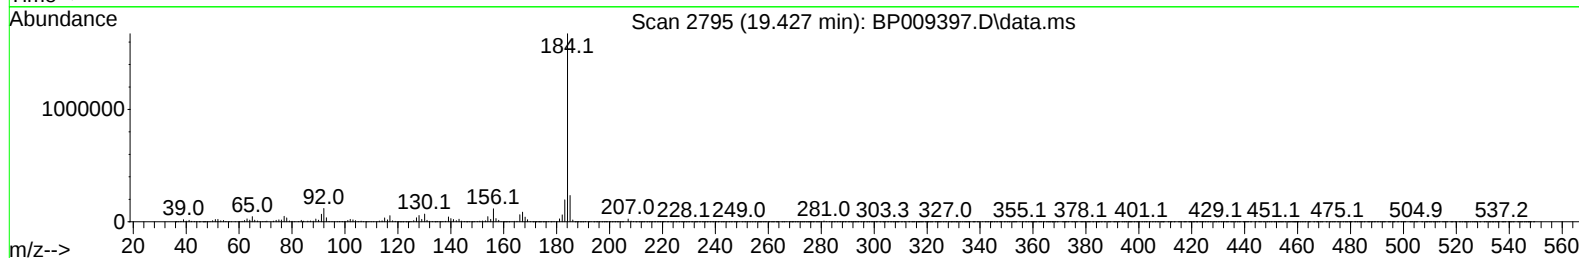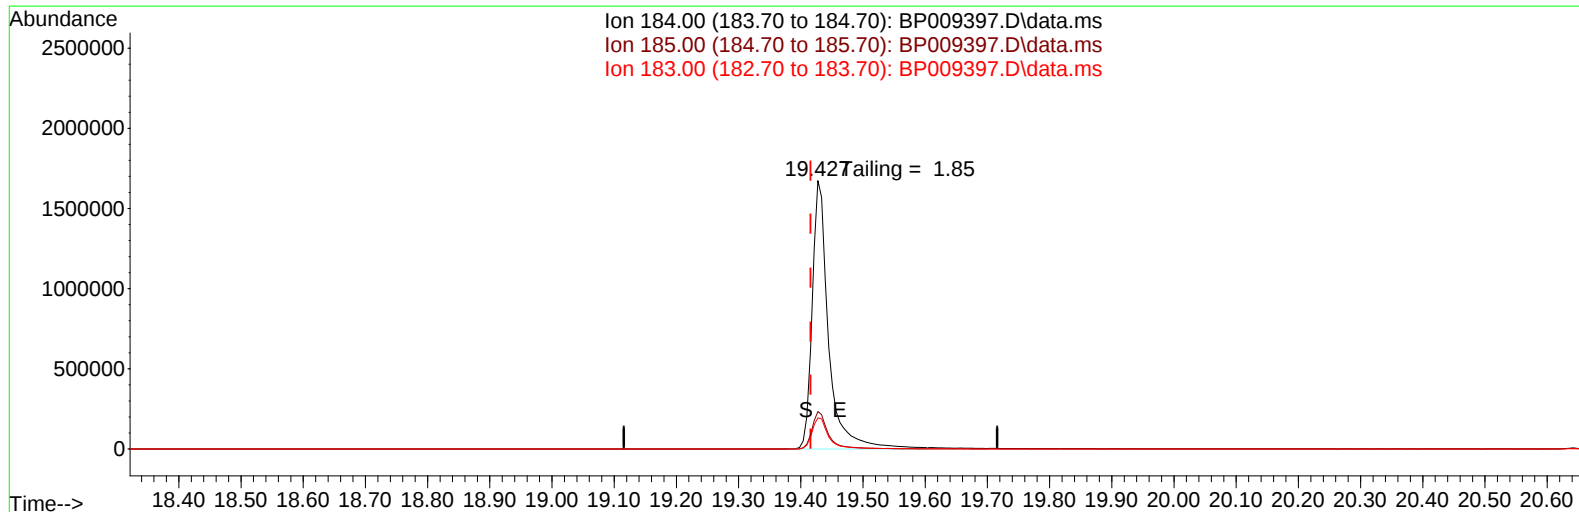

TIC: BP009397.D\data.ms

(77) Benzidine

19.427min (+ 0.012) 10325.48 ng

response 3097634

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	11.70	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/15/2022	BNA_P	<u>BP009397.D</u>
Compound Name	Response	Retention Time
DDT	1742732	20.639
DDD	37093	20.21
DDE	3857	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40950	1783682	2.30

Instrument :
BNA_P
ClientSampleId :
DFTPP