

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014101.D
 Acq On : 16 Mar 2023 14:11
 Operator : CG/JU
 Sample : 01884-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB907

Quant Time: Mar 17 00:59:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 17 00:57:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	174959	20.000	ng/u1	0.00
20) Naphthalene-d8	10.887	136	731555	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.710	164	474506	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1030580	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.545	240	860332	20.000	ng/u1	# 0.00
88) Perylene-d12	24.080	264	694000	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	16803	3.629	ng/uL	0.00
4) Pyridine-d5	3.864	84	109890	8.571	ng/u1	0.00
7) Phenol-d5	7.216	99	98814	6.400	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	300642	33.388	ng/u1	0.00
11) 2-Chlorophenol-d4	7.593	132	267743	22.761	ng/u1	0.00
15) 4-Methylphenol-d8	8.775	113	190263	15.086	ng/u1	0.00
21) Nitrobenzene-d5	9.240	128	178874	30.645	ng/u1	0.00
24) 2-Nitrophenol-d4	9.963	143	187205	26.792	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.504	165	335297	25.503	ng/u1	0.00
31) 4-Chloroaniline-d4	11.028	131	244816	14.071	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	1247093	30.968	ng/u1	0.00
49) Acenaphthylene-d8	14.404	160	1372393	32.171	ng/u1	0.00
54) 4-Nitrophenol-d4	14.916	143	30553	4.305	ng/u1	0.01
60) Fluorene-d10	15.698	176	1027044	30.093	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.822	200	190217	24.421	ng/u1	0.00
73) Anthracene-d10	17.563	188	1636730	32.715	ng/u1	0.00
81) Pyrene-d10	19.792	212	1872232	39.457	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.915	264	1219528	33.036	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.464	88	18393	3.679	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014101.D
Acq On : 16 Mar 2023 14:11
Operator : CG/JU
Sample : 01884-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB907

Quant Time: Mar 17 00:59:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

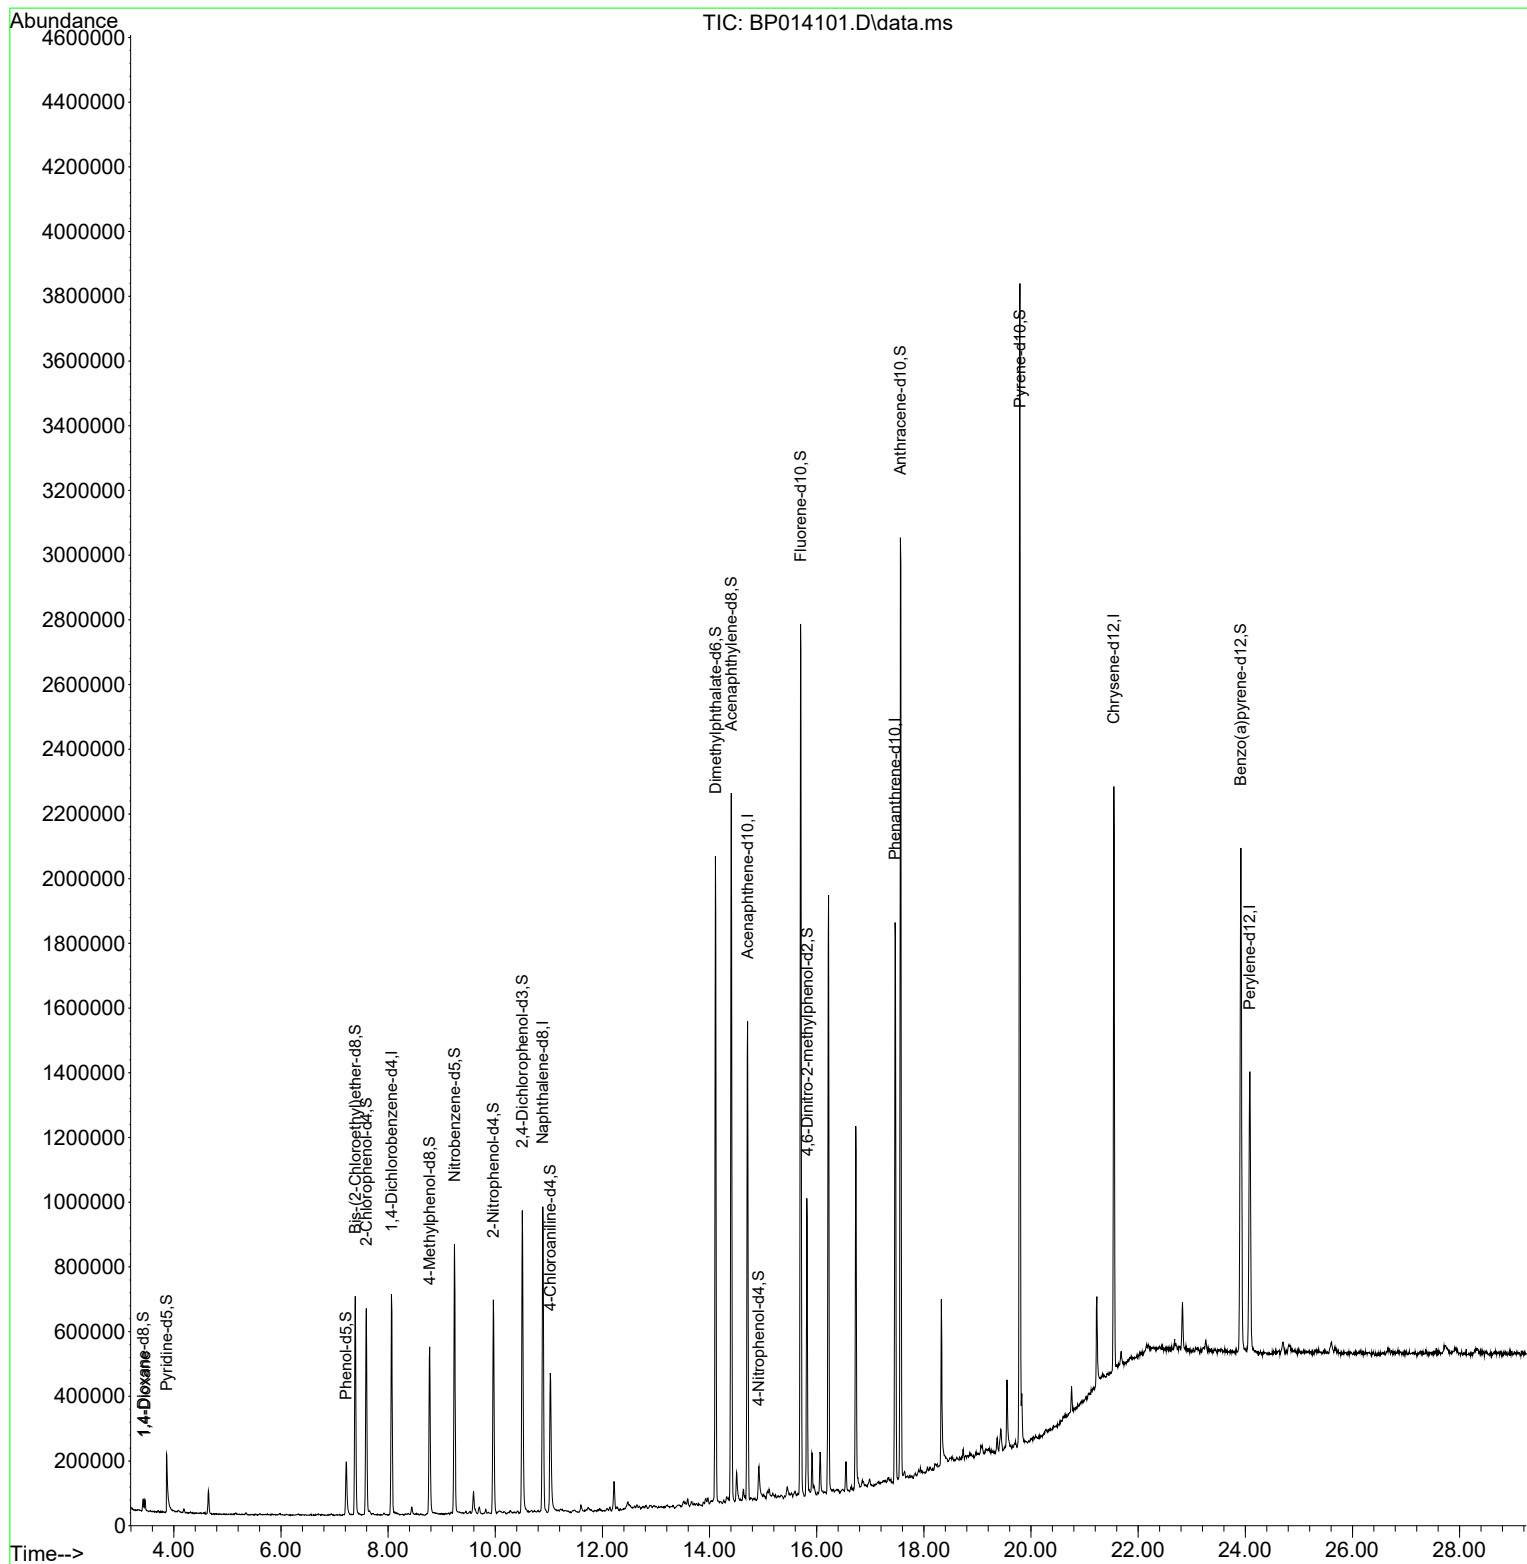

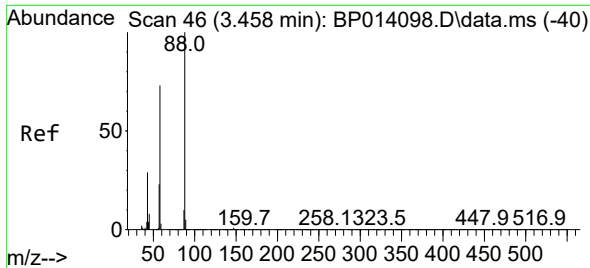

#2
 1,4-Dioxane
 Concen: 3.679 ng/uL
 RT: 3.464 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: BP014101.D
 Acq: 16 Mar 2023 14:11

Instrument :
 BNA_P
 ClientSampleId :
 CB907

Tgt Ion: 88 Resp: 18393
 Ion Ratio Lower Upper
 88 100
 43 29.9 23.9 35.9
 58 72.8 50.2 75.2

