

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014109.D
 Acq On : 16 Mar 2023 18:47
 Operator : CG/JU
 Sample : 01884-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB925


Quant Time: Mar 17 01:01:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 17 00:57:25 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	174036	20.000	ng/u1	0.00
20) Naphthalene-d8	10.887	136	729334	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.704	164	496196	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.463	188	1148809	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.545	240	1132899	20.000	ng/u1	# 0.00
88) Perylene-d12	24.080	264	1123575	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.423	96	16477	3.577	ng/uL	0.00
4) Pyridine-d5	3.864	84	157652	12.361	ng/u1	0.00
7) Phenol-d5	7.222	99	77216	5.028	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	214017	23.894	ng/u1	0.00
11) 2-Chlorophenol-d4	7.593	132	186589	15.946	ng/u1	0.00
15) 4-Methylphenol-d8	8.775	113	144587	11.525	ng/u1	0.00
21) Nitrobenzene-d5	9.240	128	127963	21.989	ng/u1	0.00
24)						

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014109.D
Acq On : 16 Mar 2023 18:47
Operator : CG/JU
Sample : 01884-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB925

Quant Time: Mar 17 01:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration




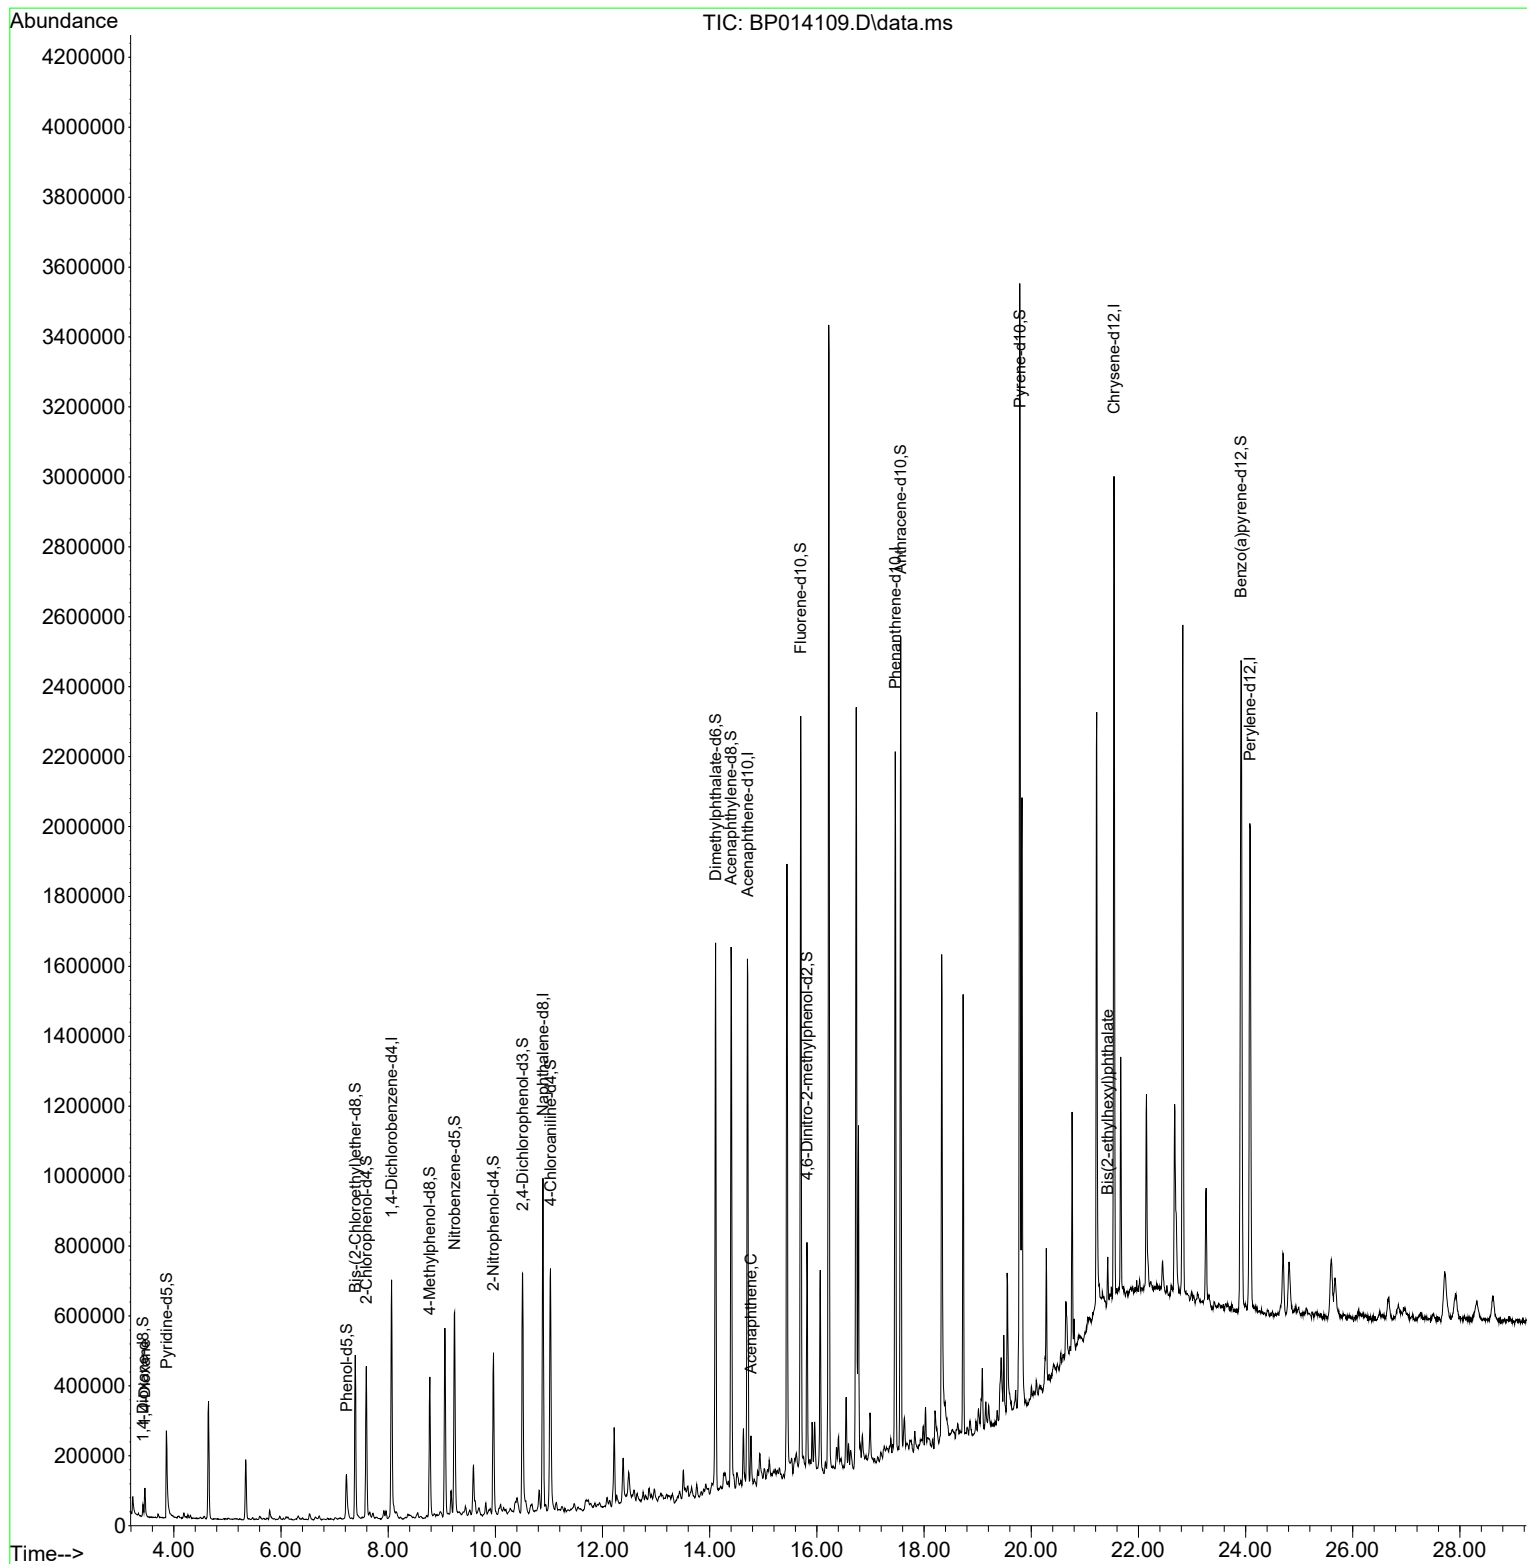


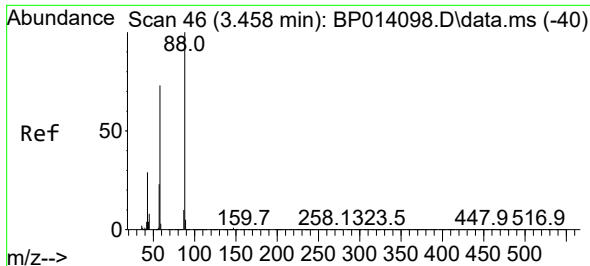

#2
 1,4-Dioxane
 Concen: 8.475 ng/uL
 RT: 3.458 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BP014109.D
 Acq: 16 Mar 2023 18:47



Instrument :
 BNA_P
 ClientSampleId :
 CB925


Tgt Ion:	88	Resp:	42144
Ion	Ratio	Lower	Upper
88	100		
43	30.5	23.9	35.9
58	75.2	50.2	75.2

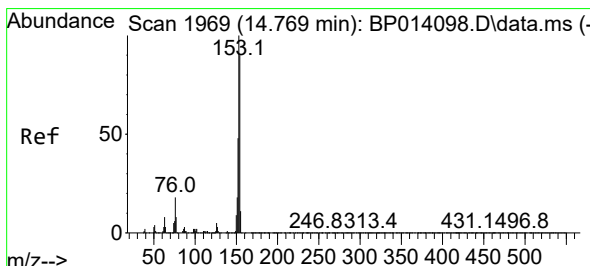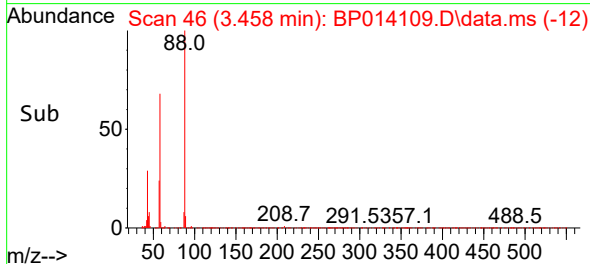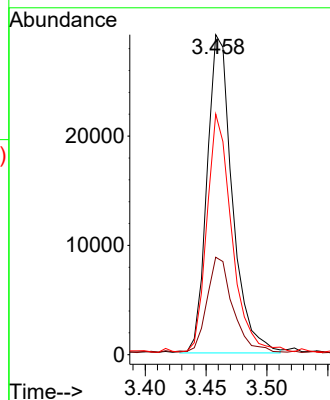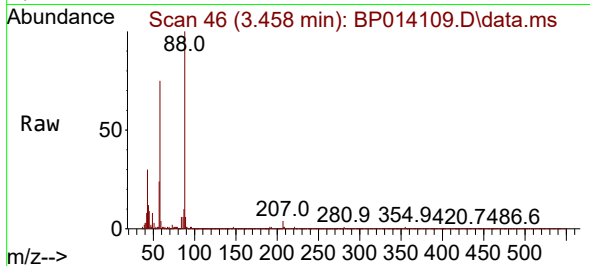

#52
 Acenaphthene
 Concen: 1.672 ng/uL
 RT: 14.769 min Scan# 1969
 Delta R.T. 0.000 min
 Lab File: BP014109.D
 Acq: 16 Mar 2023 18:47

Tgt Ion:	153	Resp:	54722
Ion	Ratio	Lower	Upper
153	100		
152	46.0	37.7	56.5
154	83.0	70.4	105.6

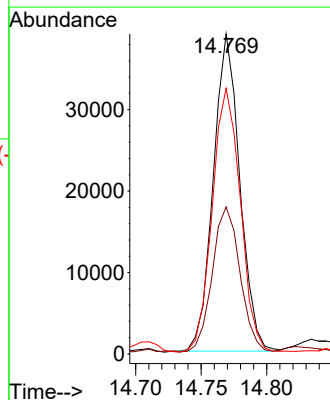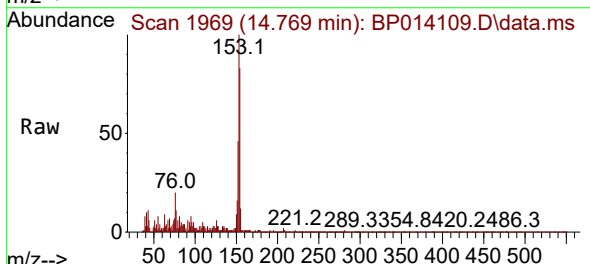

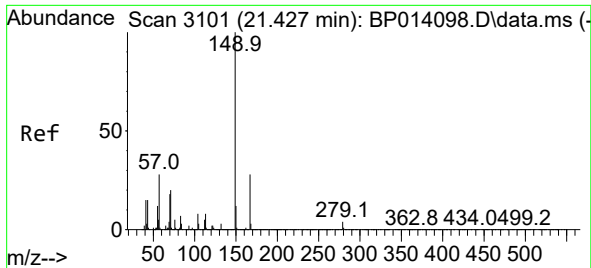

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.031 ng/ul
 RT: 21.428 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BP014109.D
 Acq: 16 Mar 2023 18:47

Instrument :
 BNA_P
 ClientSampleId :
 CB925

Tgt Ion:149 Resp: 46196
 Ion Ratio Lower Upper
 149 100
 167 28.8 22.3 33.5
 279 6.2 4.3 6.5

