




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014104.D
Acq On : 16 Mar 2023 15:54
Operator : CG/JU
Sample : 01884-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB913

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

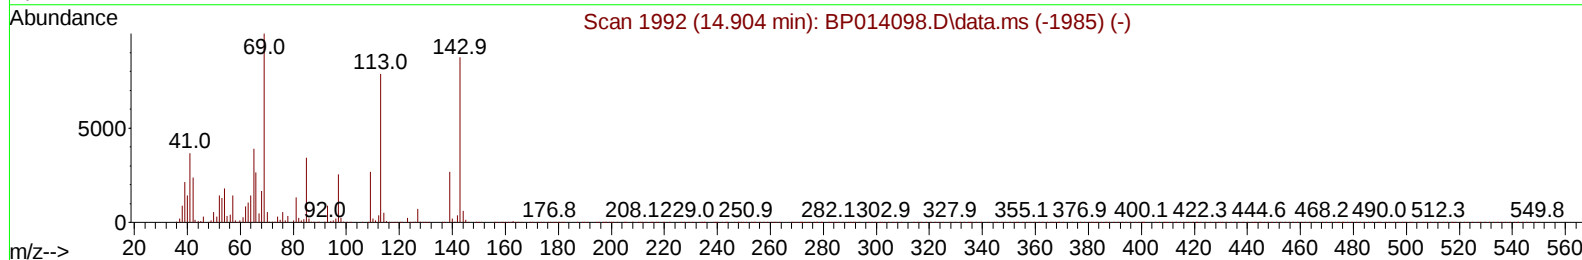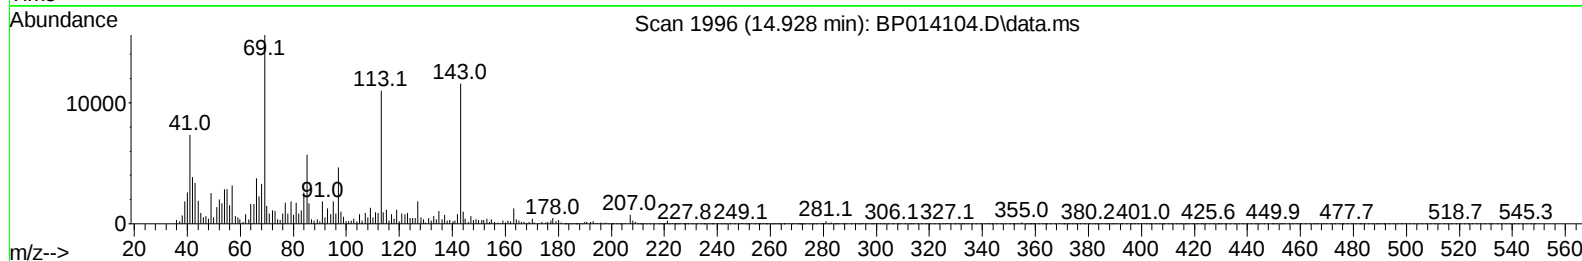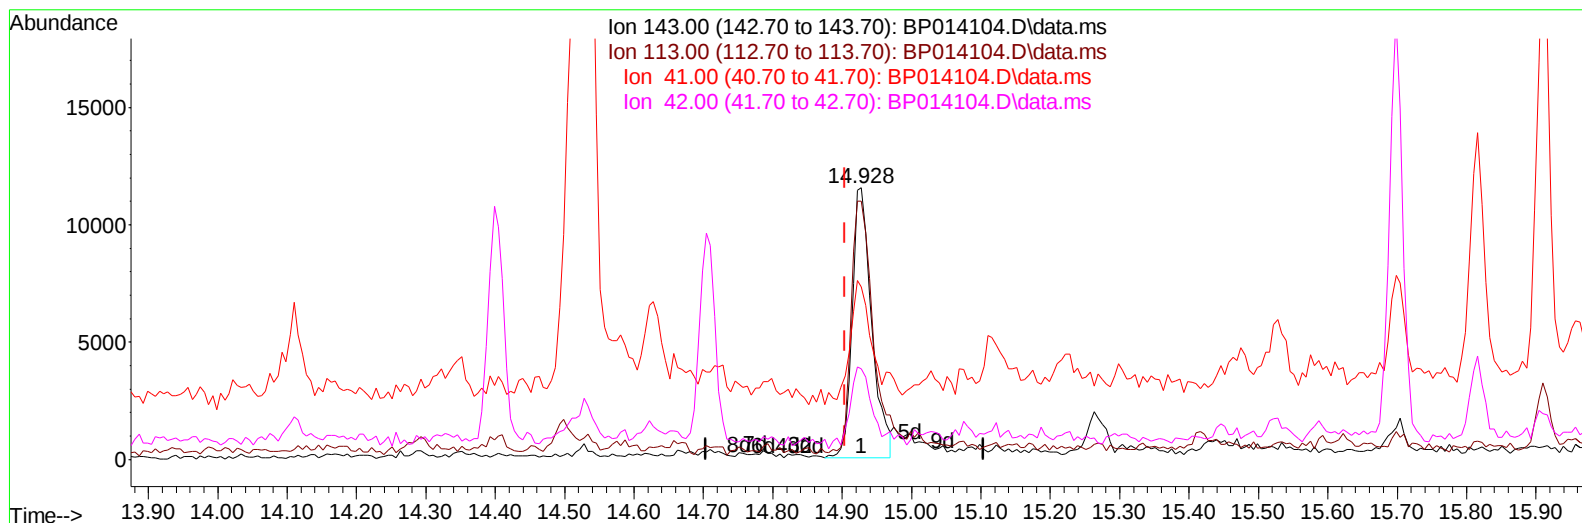

TIC: BP014104.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.928min (+ 0.024) 3.50 ng/u1****response 22398**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	95.17
41.00	40.20	63.67#
42.00	28.50	33.27




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014104.D
Acq On : 16 Mar 2023 15:54
Operator : CG/JU
Sample : 01884-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB913

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

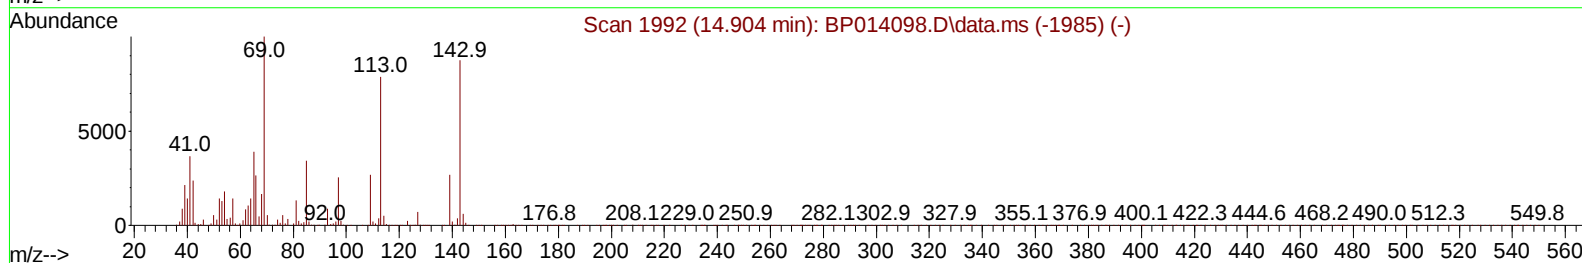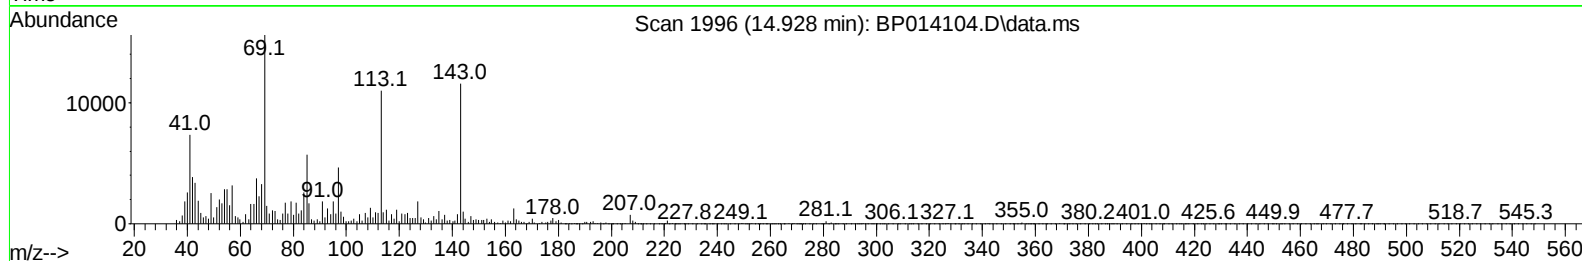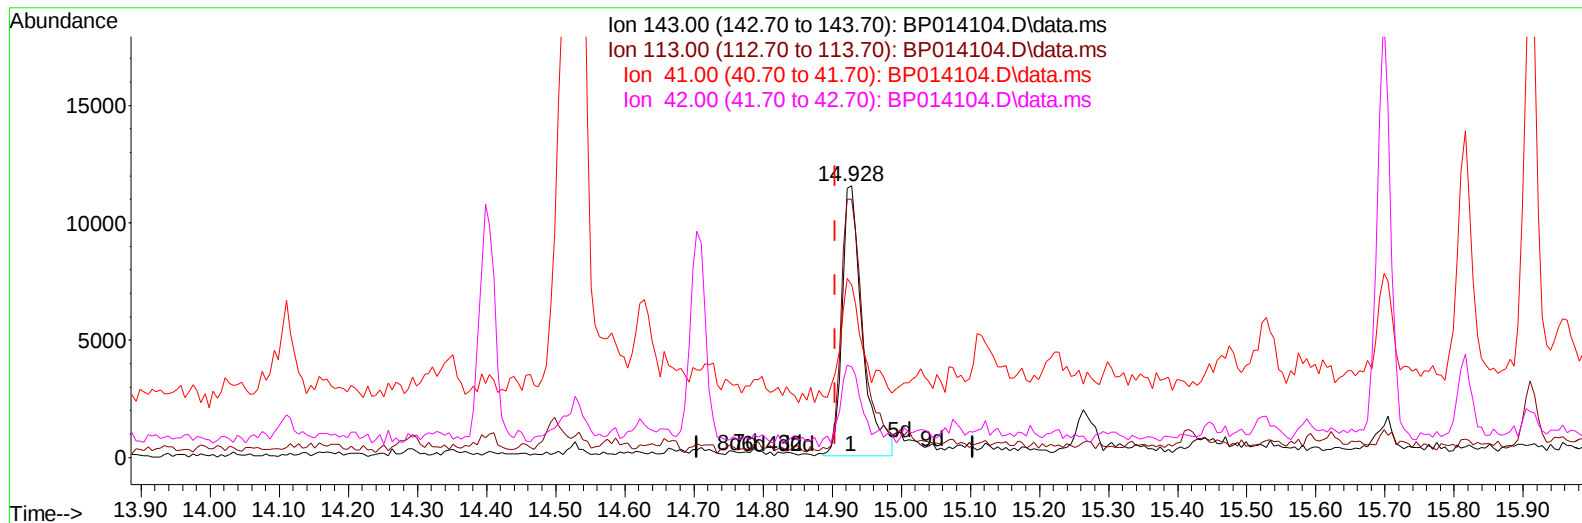

TIC: BP014104.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.928min (+ 0.024) 3.68 ng/ul m

response 23537

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	95.17
41.00	40.20	63.67#
42.00	28.50	33.27

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014104.D
 Acq On : 16 Mar 2023 15:54
 Operator : CG/JU
 Sample : 01884-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB913

Manual IntegrationsAPPROVED

Quant Time: Mar 17 01:00:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 17 00:57:25 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/17/2023
 Supervised By :Jagrut Upadhyay 03/17/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	154371	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	623365	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.704	164	428005	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1033665	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	1063756	20.000	ng/ul	# 0.00
88) Perylene-d12	24.086	264	1062003	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	16444	4.025	ng/uL	0.00
4) Pyridine-d5	3.864	84	116631	10.310	ng/ul	0.00
7) Phenol-d5	7.216	99	82006	6.020	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.381	67	253722	31.935	ng/ul	0.00
11) 2-Chlorophenol-d4	7.593	132	224543	21.634	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	171960	15.453	ng/ul	0.00
21) Nitrobenzene-d5	9.234	128	156975	31.560	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	162200	27.243	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.504	165	288901	25.788	ng/ul	0.00
31) 4-Chloroaniline-d4	11.028	131	317278	21.401	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	1169817	32.205	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	1244189	32.334	ng/ul	0.00
54) 4-Nitrophenol-d4	14.928	143	23537m	3.677	ng/ul	0.02
60) Fluorene-d10	15.698	176	948274	30.804	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	179759	23.009	ng/ul	0.00
73) Anthracene-d10	17.563	188	1585863	31.604	ng/ul	0.00
81) Pyrene-d10	19.792	212	1975806	33.677	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	1828836	32.374	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014104.D
Acq On : 16 Mar 2023 15:54
Operator : CG/JU
Sample : 01884-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB913

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

